

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051196.D
 Acq On : 07 Oct 2022 01:14
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Quant Time: Oct 07 06:30:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 02:51:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	369331	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	393968	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	127803	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	151042	40.353	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	80.700%	
7) Chloroethane-d5	1.903	69	133533	38.405	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	76.820%	
11) 1,1-Dichloroethene-d2	2.562	63	177726	32.145	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	64.280%	
21) 2-Butanone-d5	4.620	46	185839	76.551	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	76.550%	
24) Chloroform-d	5.060	84	267930	44.430	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	88.860%	
26) 1,2-Dichloroethane-d4	5.700	65	172615	46.245	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.500%	
32) Benzene-d6	5.726	84	525367	45.538	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.080%	
36) 1,2-Dichloropropane-d6	6.690	67	180208	48.137	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.280%	
41) Toluene-d8	7.896	98	406202	38.108	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	76.220%#	
43) trans-1,3-Dichloroprop...	8.179	79	63836	35.751	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	71.500%	
47) 2-Hexanone-d5	8.632	63	78275	51.783	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	51.780%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	263108	40.214	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	80.420%	
66) 1,2-Dichlorobenzene-d4	12.192	152	131473	48.155	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.300%	
Target Compounds						
13) Acetone	2.623	43	32583	16.808	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051196.D
Acq On : 07 Oct 2022 01:14
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Time: Oct 07 06:30:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 02:51:40 2022
Response via : Initial Calibration

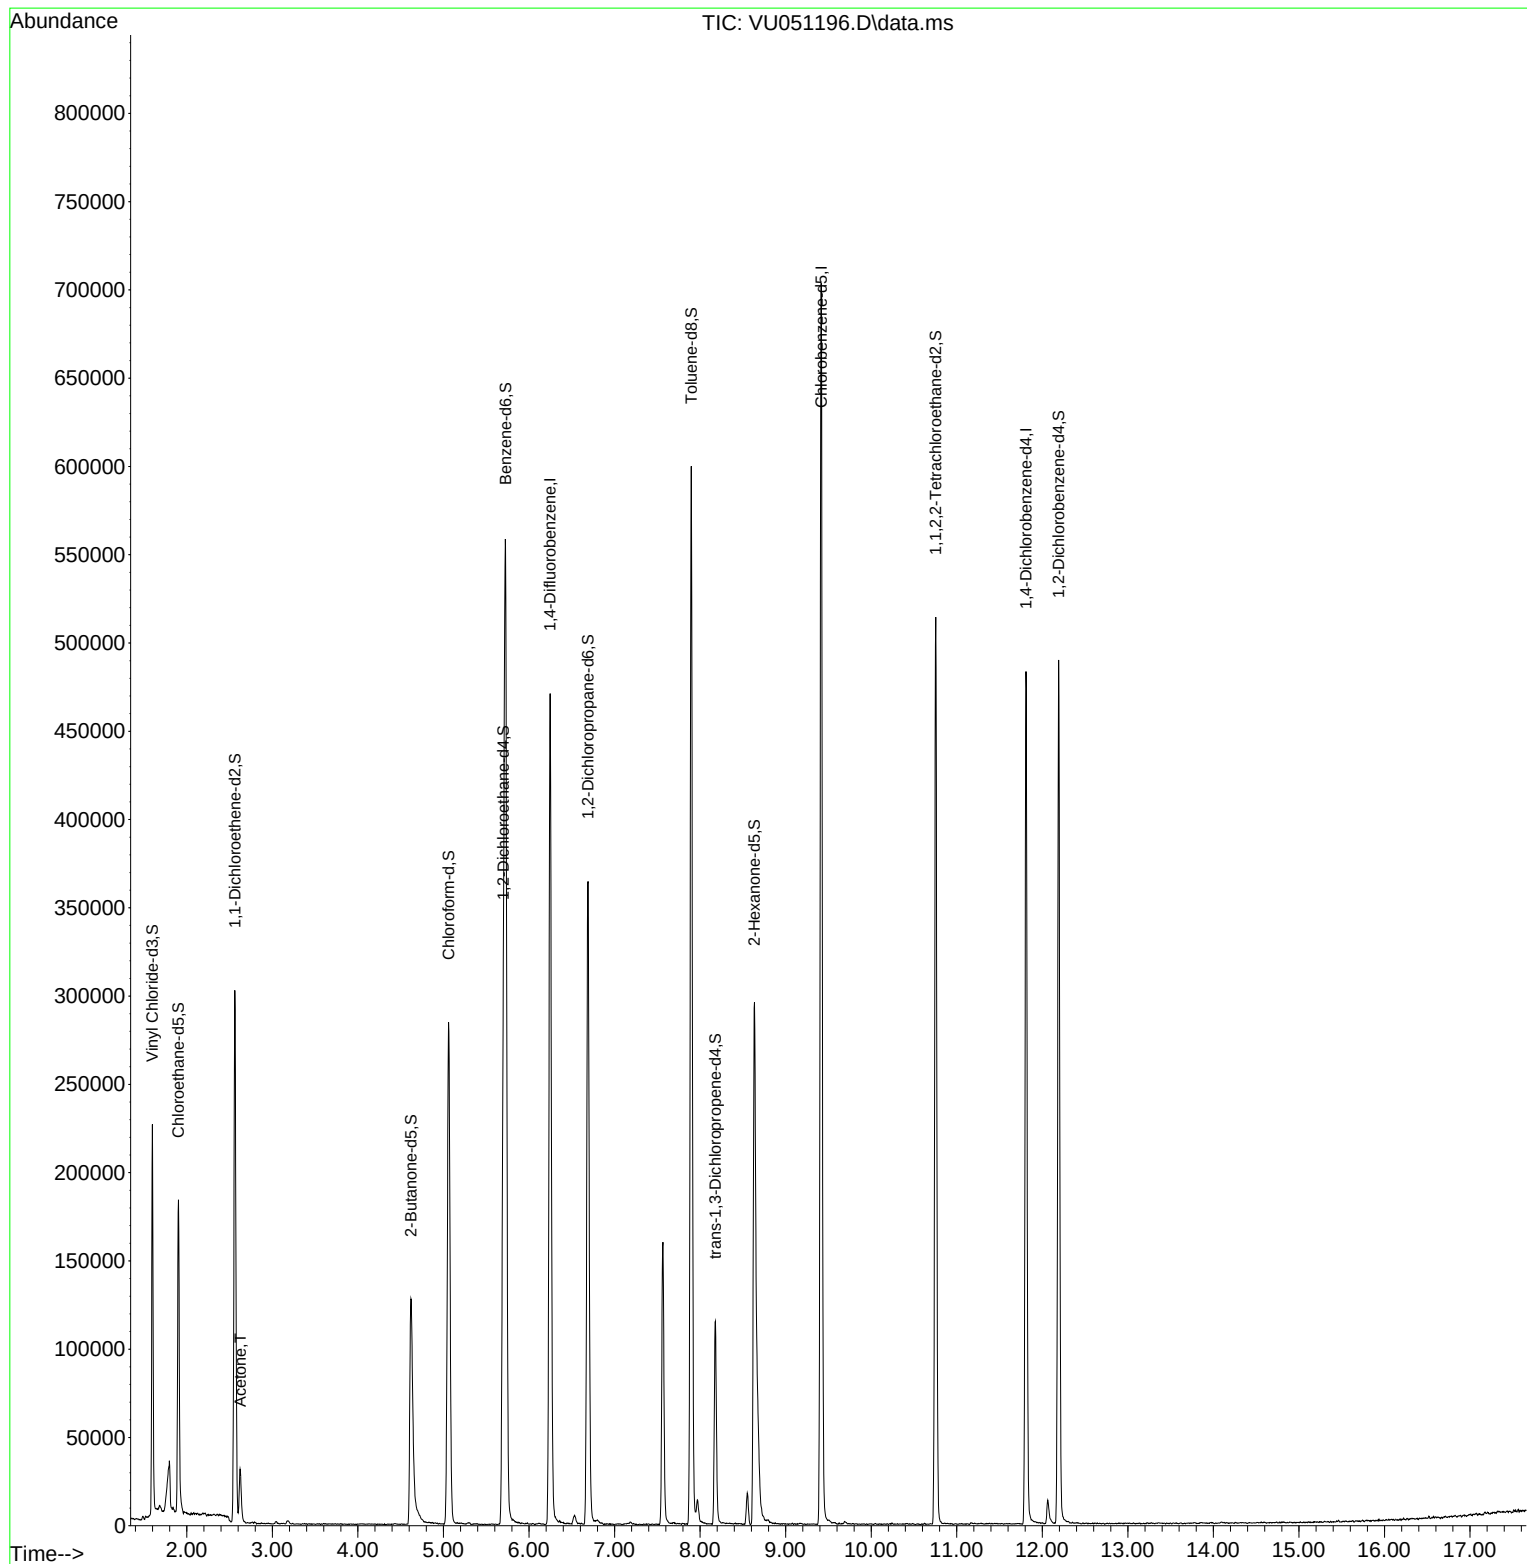

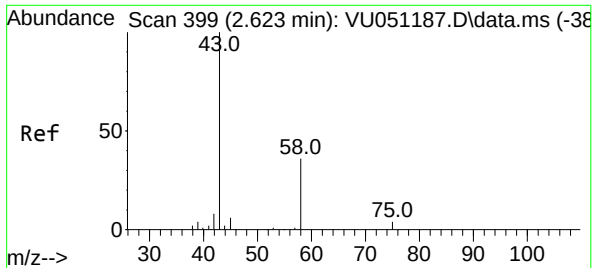

#13
 Acetone
 Concen: 16.808 ug/L
 RT: 2.623 min Scan# 399
 Delta R.T. 0.000 min
 Lab File: VU051196.D
 Acq: 07 Oct 2022 01:14

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Tgt Ion: 43 Resp: 32583
 Ion Ratio Lower Upper
 43 100
 58 35.3 0.0 73.6

