

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051198.D
 Acq On : 07 Oct 2022 02:02
 Operator : JC/MD
 Sample : N4890-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E2

Quant Time: Oct 07 06:30:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 07 02:51:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	348106	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	363531	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	118584	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	149754	42.449	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.900%	
7) Chloroethane-d5	1.899	69	132305	40.372	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	80.740%	
11) 1,1-Dichloroethene-d2	2.562	63	172887	33.176	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	66.360%	
21) 2-Butanone-d5	4.620	46	185495	81.068	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	81.070%	
24) Chloroform-d	5.060	84	264611	46.555	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.120%	
26) 1,2-Dichloroethane-d4	5.700	65	171245	48.675	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.360%	
32) Benzene-d6	5.726	84	512548	48.147	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.300%	
36) 1,2-Dichloropropane-d6	6.690	67	176839	51.193	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	102.380%	
41) Toluene-d8	7.896	98	393834	40.041	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	80.080%	
43) trans-1,3-Dichloroprop...	8.179	79	64173	38.948	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	77.900%	
47) 2-Hexanone-d5	8.632	63	76416	54.785	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	54.790%	
56) 1,1,2,2-Tetrachloroeth...	10.754	84	262504	43.481	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	86.960%	
66) 1,2-Dichlorobenzene-d4	12.192	152	124861	49.288	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.580%	
Target Compounds						
13) Acetone	2.626	43	33971	18.592	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051198.D
Acq On : 07 Oct 2022 02:02
Operator : JC/MD
Sample : N4890-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E2

Quant Time: Oct 07 06:30:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 07 02:51:40 2022
Response via : Initial Calibration

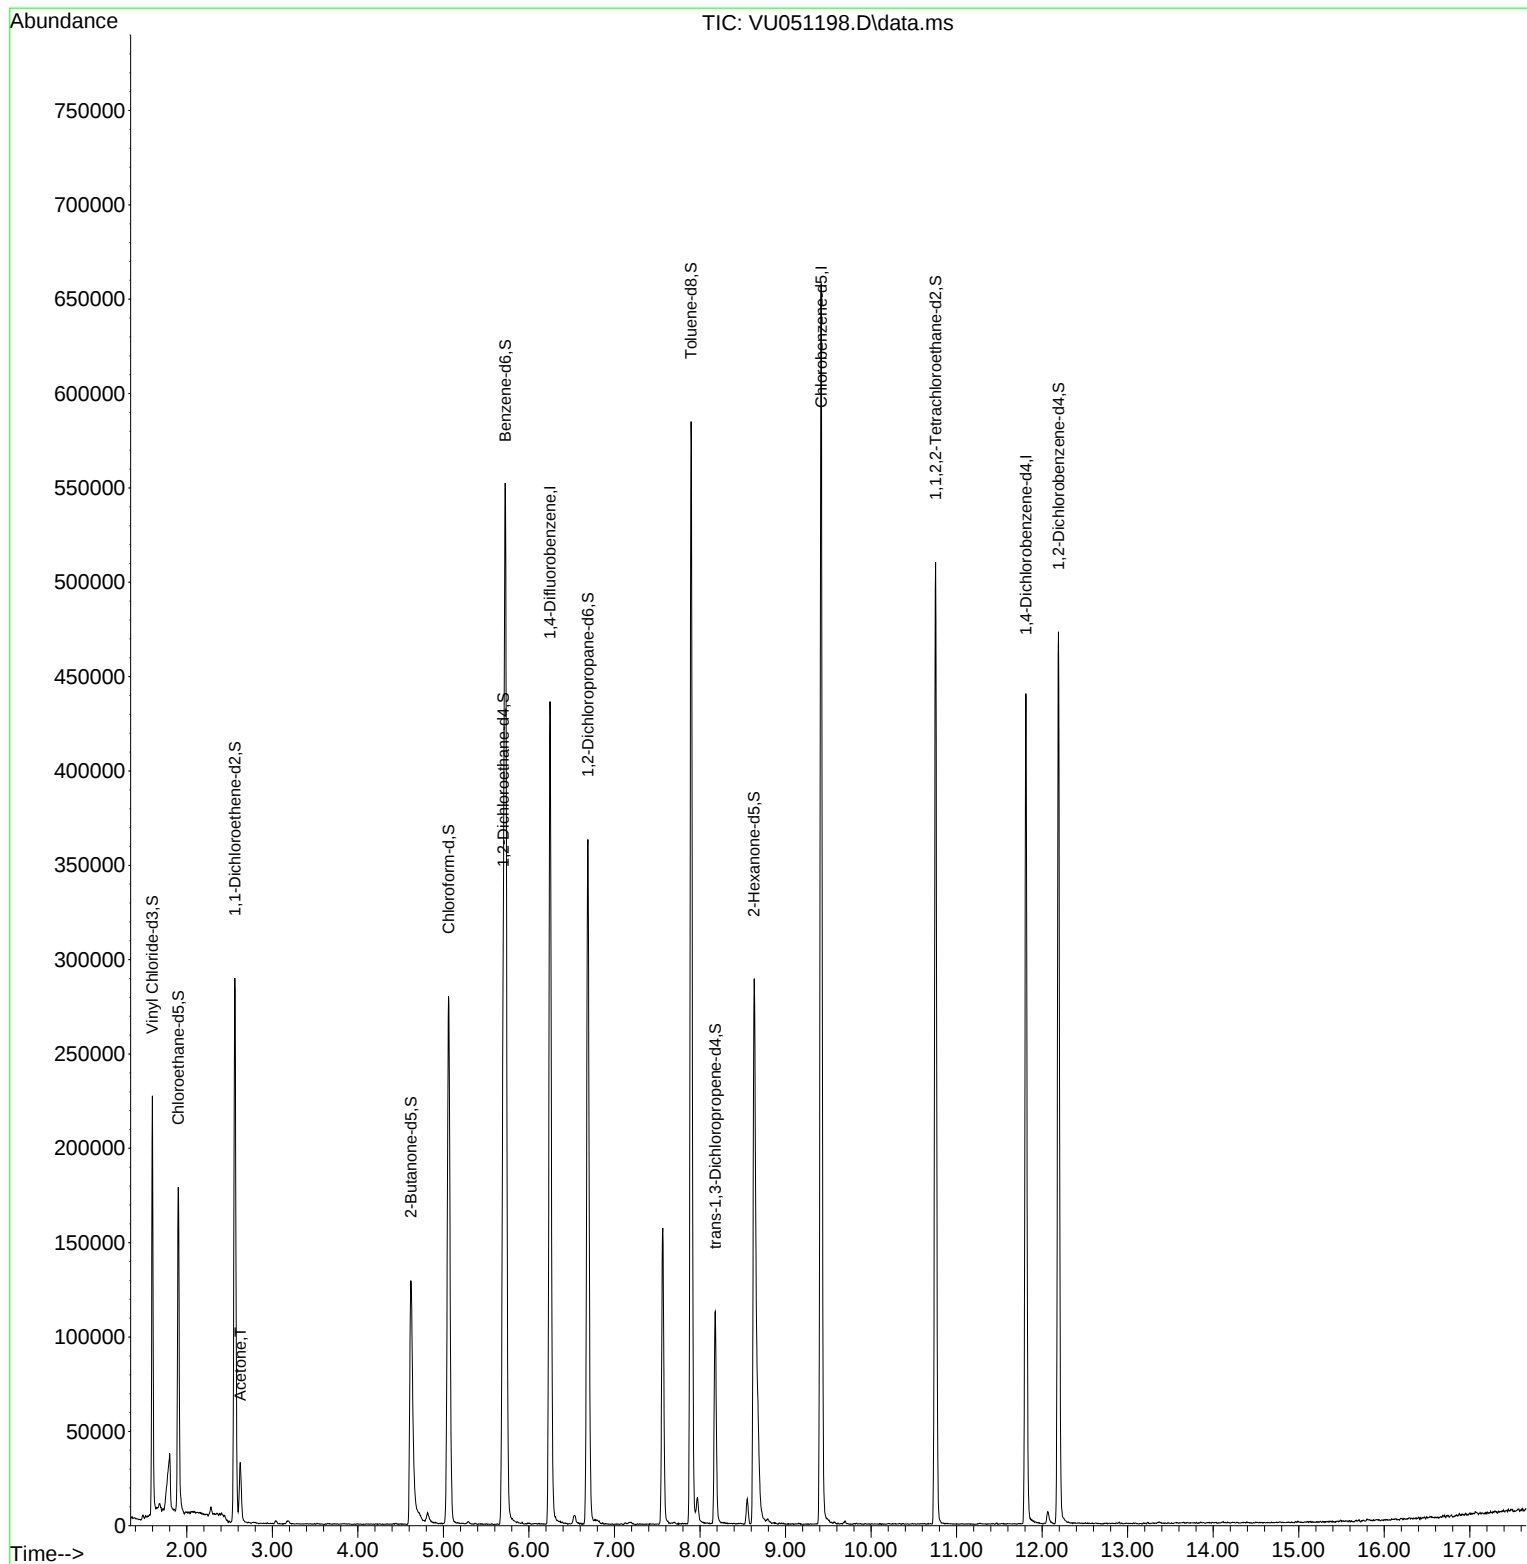

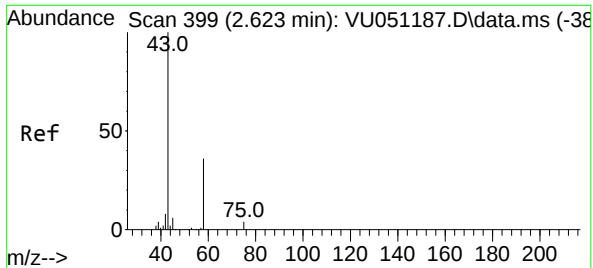

#13
 Acetone
 Concen: 18.592 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU051198.D
 Acq: 07 Oct 2022 02:02

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E2

Tgt Ion: 43 Resp: 33971
 Ion Ratio Lower Upper
 43 100
 58 35.1 0.0 73.6

