

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051165.D
 Acq On : 06 Oct 2022 12:33
 Operator : JC/MD
 Sample : VU1006MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051165.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	283863	312737	16.66%	2.278%
2	1.893	165	172	193	rVB	214396	291948	15.55%	2.126%
3	2.559	367	379	400	rBV	389738	630111	33.57%	4.589%
4	3.250	591	594	596	rBV2	430	286	0.02%	0.002%
5	3.324	615	617	619	rBV2	405	267	0.01%	0.002%
6	3.437	649	652	657	rBV	390	388	0.02%	0.003%
7	3.588	697	699	704	rVB2	392	234	0.01%	0.002%
8	3.665	721	723	726	rBV	341	144	0.01%	0.001%
9	3.684	726	729	732	rBV2	567	324	0.02%	0.002%
10	3.826	770	773	774	rBV	151	79	0.00%	0.001%
11	3.835	774	776	779	rVV	306	184	0.01%	0.001%
12	3.900	794	796	799	rBV	285	175	0.01%	0.001%
13	4.028	832	836	837	rBV	368	219	0.01%	0.002%
14	4.092	853	856	859	rBV	321	183	0.01%	0.001%
15	4.112	859	862	864	rBV2	289	227	0.01%	0.002%
16	4.269	906	911	913	rBV2	345	313	0.02%	0.002%
17	4.340	928	933	941	rBV3	433	743	0.04%	0.005%
18	4.430	958	961	966	rVB	221	167	0.01%	0.001%
19	4.469	970	973	975	rBV	325	208	0.01%	0.002%
20	4.578	1003	1007	1008	rBV2	445	263	0.01%	0.002%
21	4.620	1008	1020	1058	rVV	168653	430191	22.92%	3.133%
22	5.060	1140	1157	1176	rBV	334280	735570	39.18%	5.357%
23	5.369	1249	1253	1255	rBV2	611	498	0.03%	0.004%
24	5.488	1287	1290	1292	rBV2	253	109	0.01%	0.001%
25	5.501	1292	1294	1295	rBV2	159	70	0.00%	0.001%
26	5.584	1317	1320	1321	rBV2	268	144	0.01%	0.001%
27	5.723	1340	1363	1386	rBV2	703696	1877227	100.00%	13.672%
28	6.121	1483	1487	1495	rVB5	766	1160	0.06%	0.008%
29	6.170	1499	1502	1505	rBV	256	140	0.01%	0.001%
30	6.189	1505	1508	1511	rBV2	207	155	0.01%	0.001%
31	6.247	1512	1526	1549	rBV	564370	1075351	57.28%	7.832%
32	6.533	1605	1615	1628	rBV7	5594	11000	0.59%	0.080%
33	6.690	1645	1664	1682	rBV	441994	863343	45.99%	6.288%
34	6.948	1741	1744	1745	rBV	292	156	0.01%	0.001%
35	6.983	1751	1755	1756	rBV	189	107	0.01%	0.001%
36	7.041	1771	1773	1775	rBV	167	90	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051165.D
 Acq On : 06 Oct 2022 12:33
 Operator : JC/MD
 Sample : VU1006MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.102	1788	1792	1795	rBV	223	211	0.01%	0.002%
38	7.137	1801	1803	1806	rBV	302	194	0.01%	0.001%
39	7.179	1811	1816	1817	rBV3	909	868	0.05%	0.006%
40	7.276	1843	1846	1849	rVB2	451	240	0.01%	0.002%
41	7.298	1849	1853	1855	rBV2	159	115	0.01%	0.001%
42	7.314	1855	1858	1859	rBV2	292	179	0.01%	0.001%
43	7.362	1871	1873	1874	rBV	200	64	0.00%	0.000%
44	7.391	1879	1882	1883	rBV2	271	146	0.01%	0.001%
45	7.565	1923	1936	1957	rBV	215595	380755	20.28%	2.773%
46	7.800	2000	2009	2016	rBV5	2328	3590	0.19%	0.026%
47	7.896	2024	2039	2053	rBV	792258	1365687	72.75%	9.946%
48	8.176	2115	2126	2146	rBV2	147942	252382	13.44%	1.838%
49	8.395	2191	2194	2199	rBV2	819	829	0.04%	0.006%
50	8.507	2225	2229	2232	rBV4	526	462	0.02%	0.003%
51	8.549	2238	2242	2243	rBV3	1474	1087	0.06%	0.008%
52	8.587	2249	2254	2256	rVB3	433	401	0.02%	0.003%
53	8.636	2256	2269	2303	rBV3	420474	938844	50.01%	6.838%
54	8.915	2352	2356	2358	rBV	1079	796	0.04%	0.006%
55	8.986	2375	2378	2383	rBV2	263	271	0.01%	0.002%
56	9.012	2383	2386	2391	rVB	556	472	0.03%	0.003%
57	9.041	2391	2395	2400	rBV3	514	652	0.03%	0.005%
58	9.092	2408	2411	2416	rBV3	437	378	0.02%	0.003%
59	9.137	2423	2425	2426	rBV	183	53	0.00%	0.000%
60	9.160	2428	2432	2433	rVV	368	278	0.01%	0.002%
61	9.185	2437	2440	2441	rBV	188	95	0.01%	0.001%
62	9.417	2499	2512	2537	rBV	807317	1346477	71.73%	9.807%
63	9.571	2554	2560	2573	rVB5	3592	5675	0.30%	0.041%
64	9.694	2591	2598	2608	rVB2	7171	11310	0.60%	0.082%
65	9.771	2619	2622	2626	rVB3	349	291	0.02%	0.002%
66	9.793	2626	2629	2633	rBV2	457	460	0.02%	0.003%
67	9.845	2642	2645	2648	rVB2	360	185	0.01%	0.001%
68	9.922	2664	2669	2672	rBV2	279	205	0.01%	0.001%
69	9.944	2675	2676	2677	rBV	215	44	0.00%	0.000%
70	9.954	2677	2679	2681	rBV	331	150	0.01%	0.001%
71	10.060	2708	2712	2715	rVB2	283	252	0.01%	0.002%
72	10.105	2715	2726	2728	rBV4	2966	3794	0.20%	0.028%
73	10.366	2805	2807	2814	rBV2	316	249	0.01%	0.002%
74	10.439	2827	2830	2832	rBV2	446	287	0.02%	0.002%
75	10.636	2888	2891	2894	rBV3	535	374	0.02%	0.003%
76	10.755	2916	2928	2943	rBV	618972	996067	53.06%	7.254%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051165.D
 Acq On : 06 Oct 2022 12:33
 Operator : JC/MD
 Sample : VU1006MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK199

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

77	10.989	2995	3001	3004	rBV3	439	473	0.03%	0.003%
78	11.092	3025	3033	3037	rBV3	1573	1984	0.11%	0.014%
79	11.227	3073	3075	3080	rBV	317	290	0.02%	0.002%
80	11.468	3144	3150	3162	rVB6	2080	3516	0.19%	0.026%
81	11.517	3162	3165	3167	rBV	272	211	0.01%	0.002%
82	11.591	3186	3188	3189	rBV	303	142	0.01%	0.001%
83	11.745	3226	3236	3244	rBV6	4112	6553	0.35%	0.048%
84	11.809	3244	3256	3282	rBV	620260	1020480	54.36%	7.432%
85	12.192	3361	3375	3398	rBV	670933	1091959	58.17%	7.953%
86	13.224	3690	3696	3706	rVB6	4359	6108	0.33%	0.044%
87	13.841	3882	3888	3898	rBV5	7582	12362	0.66%	0.090%
88	14.089	3957	3965	3985	rBV2	20646	36916	1.97%	0.269%




Sum of corrected areas: 13730374

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051165.D
Acq On : 06 Oct 2022 12:33
Operator : JC/MD
Sample : VU1006MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

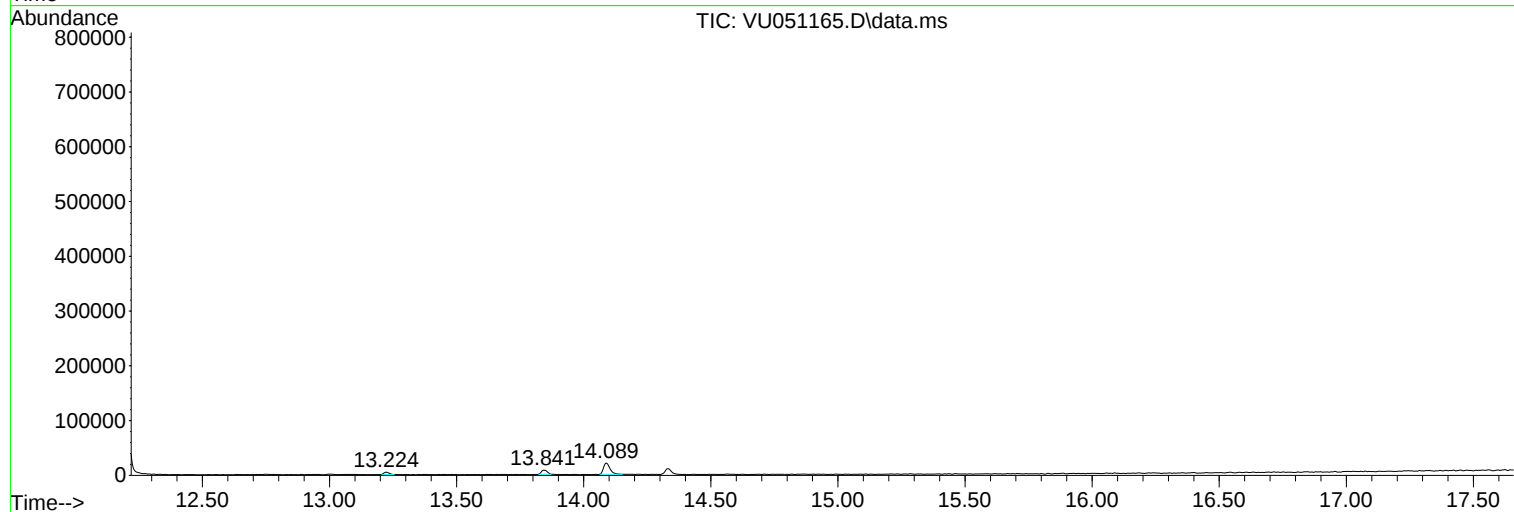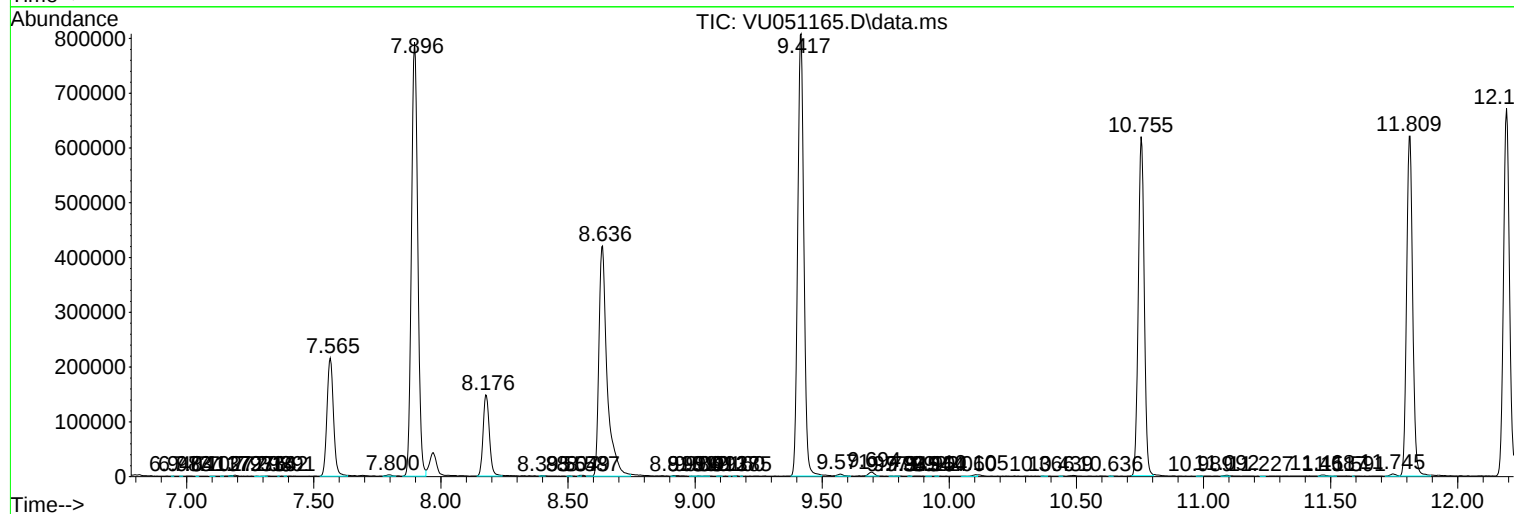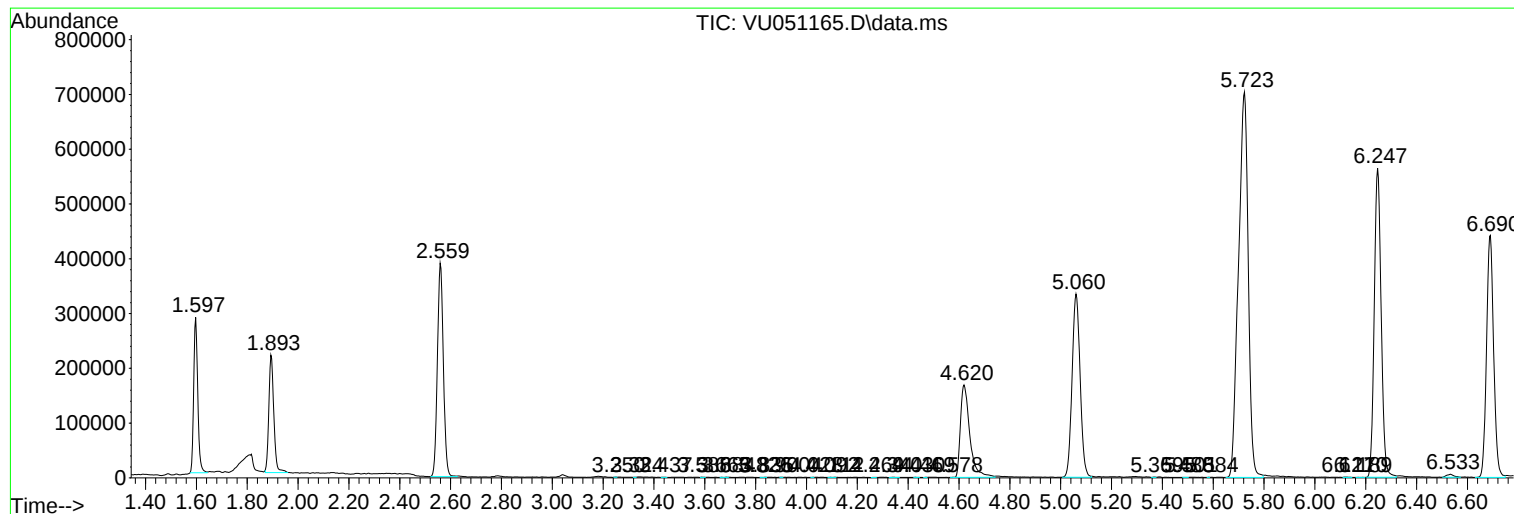

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051165.D
Acq On : 06 Oct 2022 12:33
Operator : JC/MD
Sample : VU1006MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051165.D
Acq On : 06 Oct 2022 12:33
Operator : JC/MD
Sample : VU1006MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK199

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc