

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051167.D
 Acq On : 06 Oct 2022 13:23
 Operator : JC/MD
 Sample : N4893-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051167.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	72	80	96	rBV	205156	278073	16.58%	2.182%
2	1.903	167	175	195	rVB	162730	228925	13.65%	1.796%
3	2.562	368	380	395	rBV	290318	468446	27.93%	3.676%
4	2.678	413	416	421	rVB3	1031	772	0.05%	0.006%
5	2.762	439	442	444	rBV	1218	750	0.04%	0.006%
6	2.787	444	450	462	rVB	4841	8307	0.50%	0.065%
7	3.180	561	572	590	rVB2	9651	22138	1.32%	0.174%
8	3.350	612	625	649	rBV2	132584	288977	17.23%	2.267%
9	3.855	771	782	789	rBV6	1616	3612	0.22%	0.028%
10	4.109	858	861	864	rBV3	505	333	0.02%	0.003%
11	4.151	869	874	877	rBV	432	427	0.03%	0.003%
12	4.440	960	964	966	rBV2	382	301	0.02%	0.002%
13	4.620	1008	1020	1030	rBV	163880	396522	23.64%	3.111%
14	5.060	1140	1157	1176	rBV	307993	671540	40.04%	5.269%
15	5.250	1213	1216	1219	rVB3	482	339	0.02%	0.003%
16	5.289	1223	1228	1235	rVV4	876	1141	0.07%	0.009%
17	5.401	1260	1263	1268	rVB3	762	575	0.03%	0.005%
18	5.456	1278	1280	1285	rVB3	545	325	0.02%	0.003%
19	5.723	1340	1363	1392	rBV2	614209	1677099	100.00%	13.159%
20	5.932	1425	1428	1431	rBV3	462	315	0.02%	0.002%
21	6.038	1458	1461	1466	rVB4	758	749	0.04%	0.006%
22	6.089	1475	1477	1480	rVB2	480	302	0.02%	0.002%
23	6.118	1480	1486	1488	rBV2	373	402	0.02%	0.003%
24	6.247	1510	1526	1547	rBV	442984	850922	50.74%	6.677%
25	6.430	1579	1583	1586	rBV2	454	330	0.02%	0.003%
26	6.539	1603	1617	1629	rVB2	6186	13704	0.82%	0.108%
27	6.591	1629	1633	1637	rVB4	493	393	0.02%	0.003%
28	6.687	1648	1663	1681	rBV	398496	783670	46.73%	6.149%
29	7.038	1770	1772	1777	rBV	455	328	0.02%	0.003%
30	7.166	1802	1812	1816	rBV6	3467	5817	0.35%	0.046%
31	7.350	1866	1869	1874	rVB2	346	336	0.02%	0.003%
32	7.398	1882	1884	1891	rVB	376	413	0.02%	0.003%
33	7.498	1910	1915	1917	rBV2	270	269	0.02%	0.002%
34	7.565	1923	1936	1957	rBV	182764	322458	19.23%	2.530%
35	7.691	1973	1975	1983	rVB4	1092	1168	0.07%	0.009%
36	7.790	2001	2006	2008	rBV3	1266	1111	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051167.D
 Acq On : 06 Oct 2022 13:23
 Operator : JC/MD
 Sample : N4893-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.845	2021	2023	2026	rBV2	460	275	0.02%	0.002%
38	7.896	2026	2039	2053	rBV	674177	1165363	69.49%	9.144%
39	7.970	2054	2062	2072	rVB	39501	70046	4.18%	0.550%
40	8.089	2094	2099	2102	rBV3	514	439	0.03%	0.003%
41	8.179	2115	2127	2149	rBV	131022	221501	13.21%	1.738%
42	8.279	2155	2158	2165	rVV3	498	570	0.03%	0.004%
43	8.552	2231	2243	2257	rBV	232615	392542	23.41%	3.080%
44	8.633	2257	2268	2301	rVV2	408498	886817	52.88%	6.958%
45	8.838	2328	2332	2340	rVB5	950	1016	0.06%	0.008%
46	8.867	2340	2341	2344	rBV	553	277	0.02%	0.002%
47	8.928	2355	2360	2363	rBV2	720	575	0.03%	0.005%
48	8.973	2368	2374	2376	rBV4	489	442	0.03%	0.003%
49	9.128	2419	2422	2427	rVB2	701	526	0.03%	0.004%
50	9.414	2497	2511	2531	rBV	647660	1080485	64.43%	8.478%
51	9.568	2553	2559	2570	rVB2	3468	5073	0.30%	0.040%
52	9.694	2587	2598	2606	rBV2	7928	12219	0.73%	0.096%
53	9.771	2610	2622	2634	rVB2	6703	11592	0.69%	0.091%
54	9.822	2634	2638	2645	rBV2	479	463	0.03%	0.004%
55	9.938	2672	2674	2678	rVB	454	291	0.02%	0.002%
56	10.009	2690	2696	2700	rBV2	475	501	0.03%	0.004%
57	10.102	2717	2725	2726	rBV3	2264	2174	0.13%	0.017%
58	10.343	2795	2800	2803	rBV2	361	353	0.02%	0.003%
59	10.475	2839	2841	2844	rVV2	1198	834	0.05%	0.007%
60	10.526	2848	2857	2875	rVV4	4805	10733	0.64%	0.084%
61	10.588	2875	2876	2885	rVB3	704	638	0.04%	0.005%
62	10.755	2913	2928	2947	rBV	604576	971837	57.95%	7.625%
63	10.867	2961	2963	2967	rVB3	549	346	0.02%	0.003%
64	10.893	2968	2971	2976	rVB5	618	456	0.03%	0.004%
65	10.980	2994	2998	3002	rVV3	298	329	0.02%	0.003%
66	11.047	3017	3019	3022	rBV2	480	280	0.02%	0.002%
67	11.086	3025	3031	3039	rVB6	1035	1520	0.09%	0.012%
68	11.417	3129	3134	3137	rVB3	283	336	0.02%	0.003%
69	11.469	3143	3150	3160	rVB3	1275	1902	0.11%	0.015%
70	11.517	3160	3165	3167	rVB2	300	269	0.02%	0.002%
71	11.700	3218	3222	3226	rBV2	461	460	0.03%	0.004%
72	11.748	3230	3237	3243	rBV3	2739	3000	0.18%	0.024%
73	11.809	3244	3256	3280	rBV	501096	813617	48.51%	6.384%
74	11.996	3310	3314	3316	rBV3	855	610	0.04%	0.005%
75	12.067	3327	3336	3350	rVB4	4402	7345	0.44%	0.058%
76	12.192	3360	3375	3400	rVV	611640	1009881	60.22%	7.924%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051167.D
 Acq On : 06 Oct 2022 13:23
 Operator : JC/MD
 Sample : N4893-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.362	3422	3428	3431	rBV3	695	785	0.05%	0.006%
78	12.578	3493	3495	3498	rVB3	519	273	0.02%	0.002%
79	12.597	3498	3501	3503	rBV	582	412	0.02%	0.003%
80	12.739	3543	3545	3550	rVB	445	284	0.02%	0.002%
81	12.861	3581	3583	3586	rBV	471	266	0.02%	0.002%
82	12.957	3609	3613	3617	rBV2	363	361	0.02%	0.003%
83	13.005	3622	3628	3632	rVB3	513	519	0.03%	0.004%
84	13.089	3651	3654	3660	rVB3	592	543	0.03%	0.004%
85	13.128	3660	3666	3671	rBV2	706	1023	0.06%	0.008%
86	13.157	3671	3675	3677	rBV	433	385	0.02%	0.003%
87	13.192	3682	3686	3688	rBV2	375	351	0.02%	0.003%
88	13.221	3688	3695	3697	rBV4	1931	1953	0.12%	0.015%
89	13.366	3737	3740	3745	rVB2	548	402	0.02%	0.003%
90	13.391	3745	3748	3750	rBV2	798	512	0.03%	0.004%
91	13.597	3809	3812	3815	rBV	397	306	0.02%	0.002%
92	13.806	3873	3877	3880	rBV2	476	413	0.02%	0.003%
93	13.845	3880	3889	3897	rBV9	3312	5270	0.31%	0.041%
94	13.944	3917	3920	3923	rBV2	400	340	0.02%	0.003%
95	14.092	3957	3966	3980	rBV3	5080	10338	0.62%	0.081%
96	14.330	4030	4040	4049	rBV7	4537	9123	0.54%	0.072%
97	15.221	4314	4317	4319	rBV4	713	433	0.03%	0.003%
98	15.510	4405	4407	4410	rBV3	680	419	0.02%	0.003%
99	15.767	4485	4487	4491	rVB3	1116	532	0.03%	0.004%
100	16.070	4579	4581	4584	rBV3	818	548	0.03%	0.004%




Sum of corrected areas: 12745013

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051167.D
Acq On : 06 Oct 2022 13:23
Operator : JC/MD
Sample : N4893-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

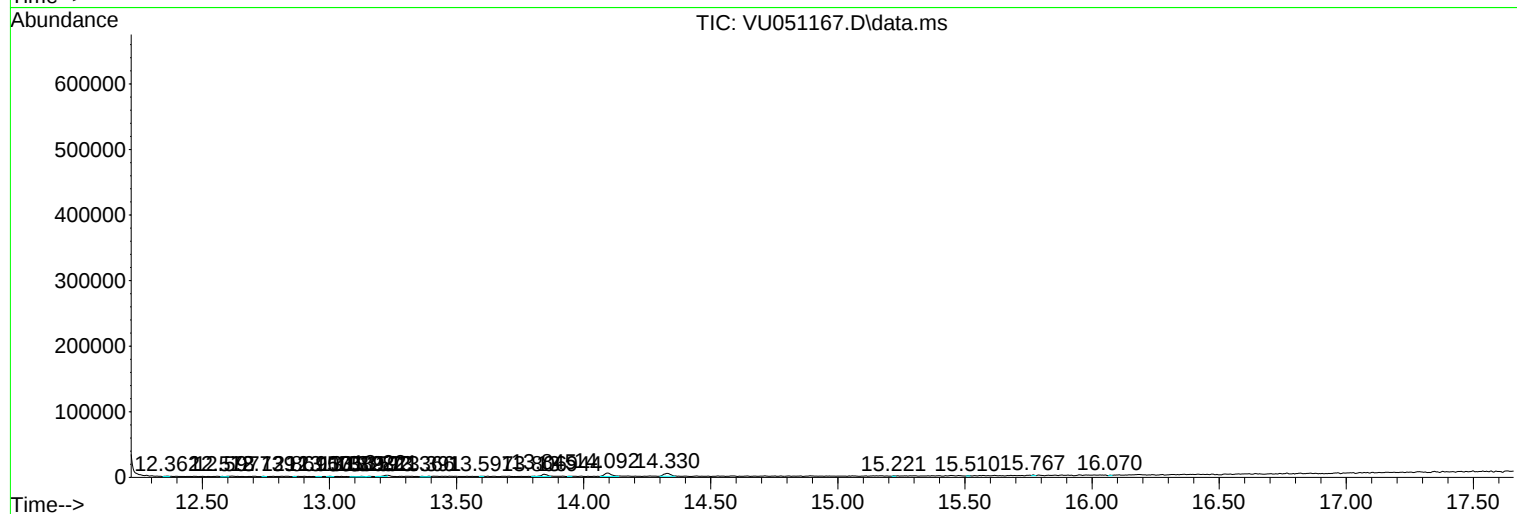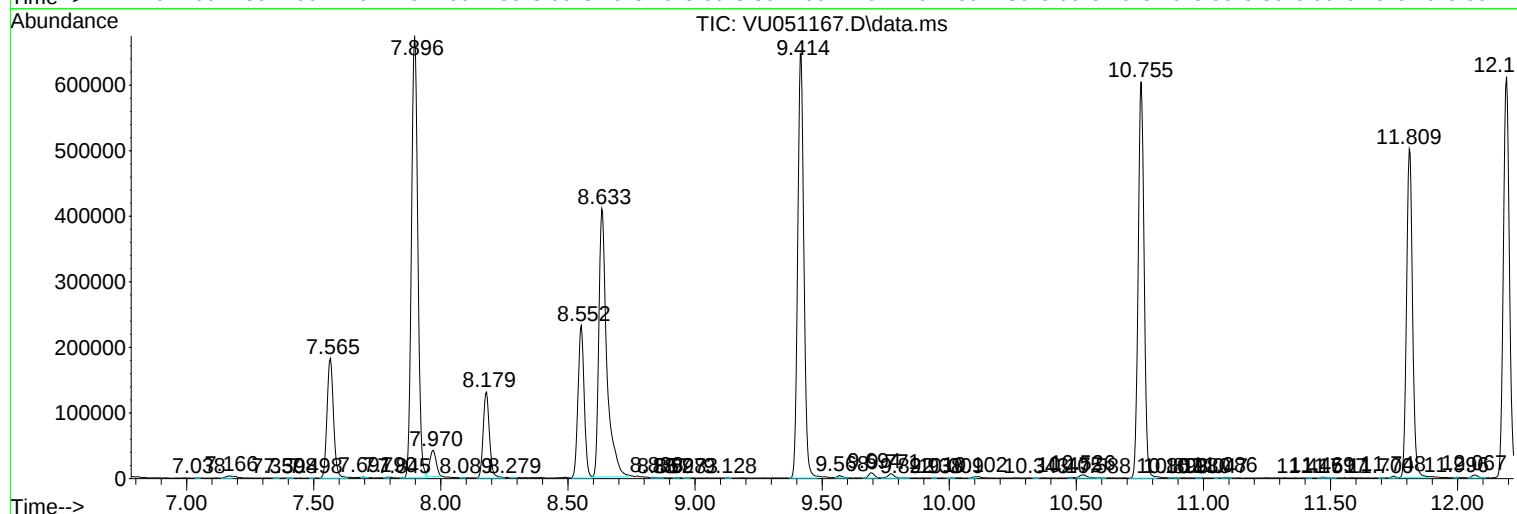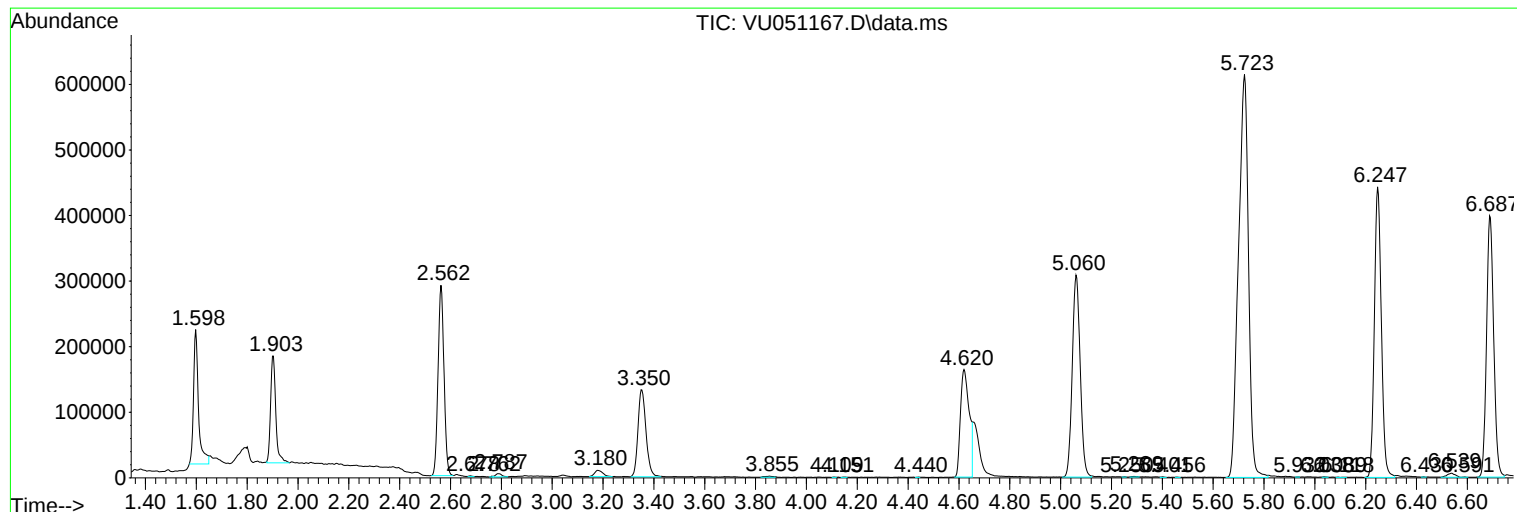

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051167.D
Acq On : 06 Oct 2022 13:23
Operator : JC/MD
Sample : N4893-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051167.D
Acq On : 06 Oct 2022 13:23
Operator : JC/MD
Sample : N4893-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc