

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051168.D
 Acq On : 06 Oct 2022 13:47
 Operator : JC/MD
 Sample : N4893-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	104	rVB	211053	276559	12.47%	1.917%
2	1.903	167	175	194	rVB	168661	232970	10.50%	1.615%
3	2.562	367	380	395	rBV	287699	473402	21.35%	3.281%
4	2.681	409	417	430	rVB5	4563	8637	0.39%	0.060%
5	2.790	445	451	461	rVB3	2632	3878	0.17%	0.027%
6	2.854	468	471	475	rVB4	608	539	0.02%	0.004%
7	2.896	481	484	487	rVB2	919	676	0.03%	0.005%
8	3.044	523	530	537	rVB6	1680	2604	0.12%	0.018%
9	3.080	537	541	543	rBV3	471	429	0.02%	0.003%
10	3.182	559	573	589	rVB	9437	20992	0.95%	0.146%
11	3.362	618	629	640	rVV5	6301	12709	0.57%	0.088%
12	3.526	677	680	683	rBV2	666	499	0.02%	0.003%
13	3.690	727	731	734	rBV2	516	523	0.02%	0.004%
14	3.784	747	760	772	rBV6	7899	16713	0.75%	0.116%
15	3.851	772	781	787	rBV4	2738	4805	0.22%	0.033%
16	3.957	808	814	817	rBV	361	442	0.02%	0.003%
17	4.067	843	848	853	rVB2	330	320	0.01%	0.002%
18	4.125	864	866	875	rVB2	252	311	0.01%	0.002%
19	4.192	882	887	890	rBV2	589	484	0.02%	0.003%
20	4.321	922	927	940	rVB	801	1114	0.05%	0.008%
21	4.436	959	963	967	rBV2	389	330	0.01%	0.002%
22	4.620	1003	1020	1051	rBV	172302	437851	19.74%	3.035%
23	4.870	1095	1098	1101	rBV3	589	506	0.02%	0.004%
24	5.060	1141	1157	1184	rVV	312333	683034	30.80%	4.734%
25	5.288	1220	1228	1231	rBV4	845	1177	0.05%	0.008%
26	5.330	1238	1241	1246	rVB3	840	544	0.02%	0.004%
27	5.385	1252	1258	1262	rVB4	817	889	0.04%	0.006%
28	5.459	1278	1281	1284	rBV	621	507	0.02%	0.004%
29	5.723	1340	1363	1390	rBV2	617176	1690930	76.25%	11.721%
30	6.105	1477	1482	1485	rVB2	369	335	0.02%	0.002%
31	6.247	1512	1526	1549	rBV	443638	845865	38.14%	5.863%
32	6.539	1606	1617	1630	rVB7	6154	12700	0.57%	0.088%
33	6.591	1630	1633	1638	rVB3	671	554	0.02%	0.004%
34	6.687	1649	1663	1682	rBV	408227	798775	36.02%	5.537%
35	7.067	1777	1781	1785	rVB2	471	394	0.02%	0.003%
36	7.102	1785	1792	1793	rBV2	337	361	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051168.D
 Acq On : 06 Oct 2022 13:47
 Operator : JC/MD
 Sample : N4893-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.115	1793	1796	1802	rVB4	533	514	0.02%	0.004%
38	7.153	1802	1808	1810	rBV2	315	343	0.02%	0.002%
39	7.182	1810	1817	1819	rBV4	1795	1869	0.08%	0.013%
40	7.565	1923	1936	1955	rBV	183081	323533	14.59%	2.243%
41	7.690	1969	1975	1985	rBV5	1294	1749	0.08%	0.012%
42	7.793	2004	2007	2017	rVB5	1620	1954	0.09%	0.014%
43	7.896	2025	2039	2053	rBV	679954	1171399	52.82%	8.120%
44	7.970	2054	2062	2077	rVV	35917	64728	2.92%	0.449%
45	8.137	2107	2114	2116	rBV4	520	531	0.02%	0.004%
46	8.179	2116	2127	2146	rVV	127471	218709	9.86%	1.516%
47	8.301	2162	2165	2173	rBV3	996	1189	0.05%	0.008%
48	8.401	2190	2196	2199	rBV3	609	637	0.03%	0.004%
49	8.484	2212	2222	2230	rBV	31234	52182	2.35%	0.362%
50	8.552	2230	2243	2257	rVV	1311436	2217713	100.00%	15.372%
51	8.632	2258	2268	2305	rVB3	451464	965109	43.52%	6.690%
52	8.857	2335	2338	2340	rVB2	604	339	0.02%	0.002%
53	8.947	2363	2366	2368	rBV	734	417	0.02%	0.003%
54	8.964	2368	2371	2375	rVV3	489	376	0.02%	0.003%
55	9.005	2381	2384	2390	rBV5	414	359	0.02%	0.002%
56	9.047	2393	2397	2399	rVV3	521	385	0.02%	0.003%
57	9.092	2408	2411	2415	rBV	448	417	0.02%	0.003%
58	9.414	2499	2511	2529	rBV	642117	1076840	48.56%	7.464%
59	9.568	2550	2559	2568	rVB2	2426	4237	0.19%	0.029%
60	9.690	2589	2597	2607	rVV2	6331	10068	0.45%	0.070%
61	9.976	2682	2686	2688	rBV2	704	667	0.03%	0.005%
62	10.108	2719	2727	2738	rVB6	1895	3300	0.15%	0.023%
63	10.246	2768	2770	2776	rVB3	472	458	0.02%	0.003%
64	10.481	2838	2843	2848	rBV2	987	1177	0.05%	0.008%
65	10.536	2855	2860	2863	rVB	566	539	0.02%	0.004%
66	10.558	2863	2867	2871	rBV2	424	398	0.02%	0.003%
67	10.648	2892	2895	2899	rVB3	455	366	0.02%	0.003%
68	10.754	2914	2928	2946	rBV	607634	987631	44.53%	6.846%
69	11.018	3006	3010	3014	rVB2	487	384	0.02%	0.003%
70	11.089	3028	3032	3034	rBV2	382	313	0.01%	0.002%
71	11.121	3039	3042	3046	rVB3	518	342	0.02%	0.002%
72	11.217	3068	3072	3075	rBV3	462	434	0.02%	0.003%
73	11.381	3117	3123	3126	rBV2	1040	1061	0.05%	0.007%
74	11.738	3227	3234	3235	rBV2	883	693	0.03%	0.005%
75	11.809	3244	3256	3278	rBV	474908	763936	34.45%	5.295%
76	12.070	3330	3337	3342	rBV5	1099	1475	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051168.D
 Acq On : 06 Oct 2022 13:47
 Operator : JC/MD
 Sample : N4893-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.140	3354	3359	3362	rBV4	672	680	0.03%	0.005%
78	12.192	3362	3375	3399	rBV	582884	966150	43.57%	6.697%
79	12.478	3459	3464	3473	rVV4	2476	3486	0.16%	0.024%
80	12.674	3520	3525	3531	rBV2	610	631	0.03%	0.004%
81	12.774	3552	3556	3558	rBV3	489	367	0.02%	0.003%
82	12.787	3558	3560	3565	rBV3	349	339	0.02%	0.002%
83	12.861	3581	3583	3588	rVB2	592	419	0.02%	0.003%
84	12.947	3603	3610	3620	rVB4	3928	5551	0.25%	0.038%
85	13.179	3678	3682	3685	rBV2	552	427	0.02%	0.003%
86	13.227	3689	3697	3705	rVB7	1407	2254	0.10%	0.016%
87	13.291	3715	3717	3722	rVV2	522	410	0.02%	0.003%
88	13.439	3760	3763	3766	rBV	510	325	0.01%	0.002%
89	13.651	3827	3829	3833	rBV3	420	374	0.02%	0.003%
90	13.735	3849	3855	3863	rVV5	2979	3571	0.16%	0.025%
91	13.841	3885	3888	3890	rBV4	1066	741	0.03%	0.005%
92	14.095	3958	3967	3974	rBV2	3407	6187	0.28%	0.043%
93	14.304	4023	4032	4034	rBV2	590	830	0.04%	0.006%
94	14.336	4035	4042	4047	rVV7	2093	2879	0.13%	0.020%
95	14.558	4108	4111	4112	rBV3	617	349	0.02%	0.002%
96	14.696	4151	4154	4158	rVB2	497	396	0.02%	0.003%
97	14.719	4158	4161	4163	rBV2	606	353	0.02%	0.002%
98	14.970	4236	4239	4244	rBV2	669	616	0.03%	0.004%
99	15.719	4469	4472	4475	rBV3	1159	841	0.04%	0.006%
100	16.767	4792	4798	4807	rVB6	11869	16437	0.74%	0.114%




Sum of corrected areas: 14426742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051168.D
Acq On : 06 Oct 2022 13:47
Operator : JC/MD
Sample : N4893-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

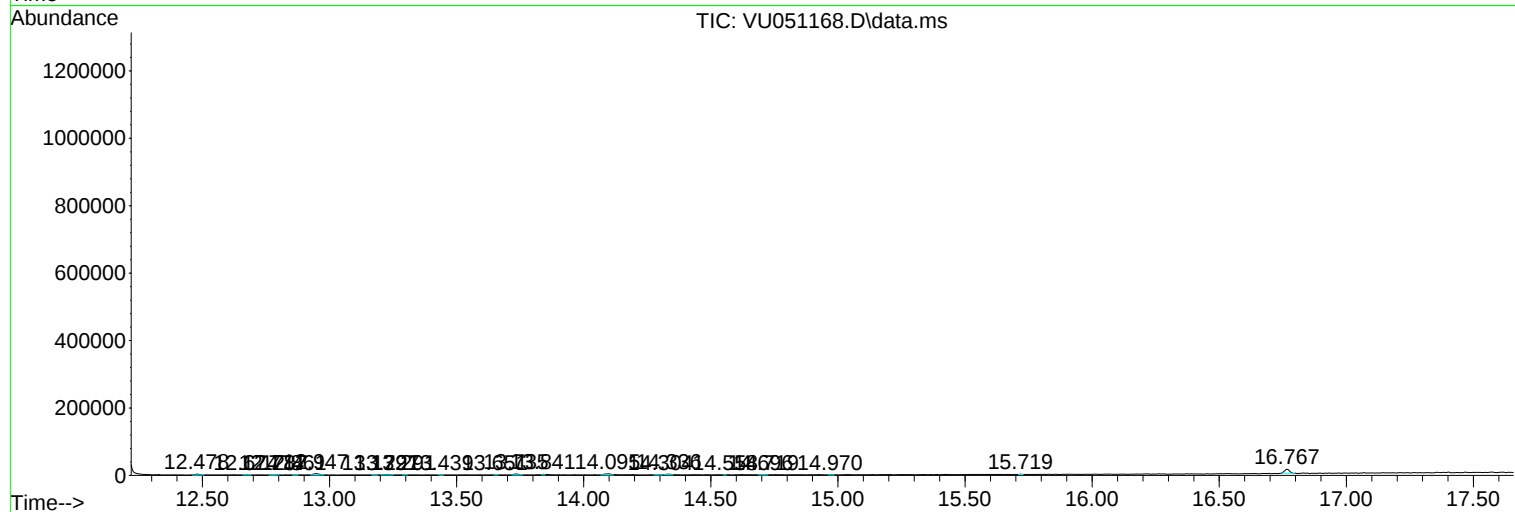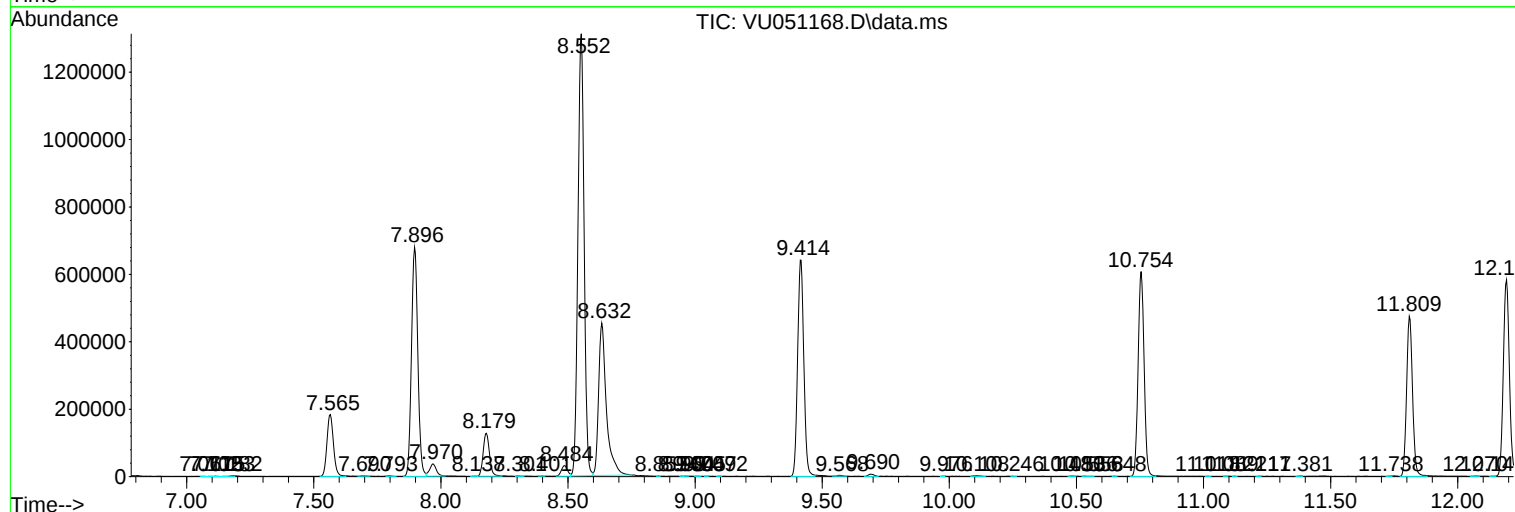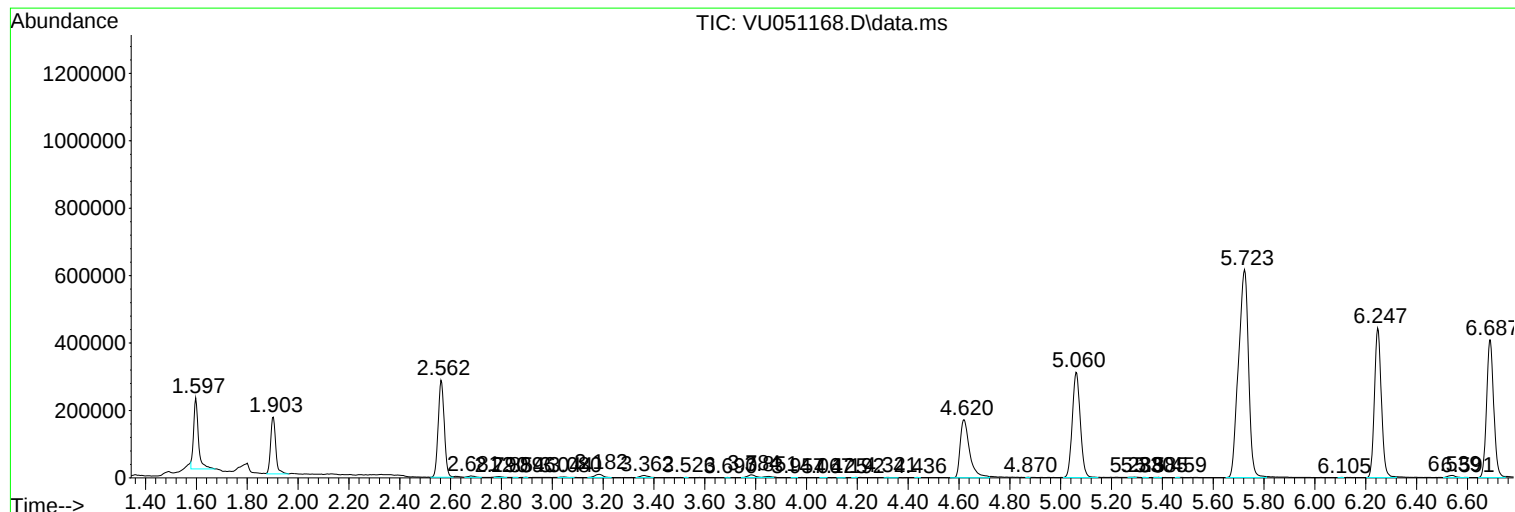

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051168.D
Acq On : 06 Oct 2022 13:47
Operator : JC/MD
Sample : N4893-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051168.D
Acq On : 06 Oct 2022 13:47
Operator : JC/MD
Sample : N4893-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------