

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051169.D
 Acq On : 06 Oct 2022 14:11
 Operator : JC/MD
 Sample : N4893-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	75	80	96	rVB	198603	237422	14.26%	1.978%
2	1.900	167	174	202	rVB	167367	235775	14.16%	1.964%
3	2.562	368	380	395	rBV	282968	462305	27.77%	3.852%
4	3.182	560	573	589	rVB	9326	21168	1.27%	0.176%
5	3.411	641	644	647	rBV2	491	458	0.03%	0.004%
6	3.523	673	679	683	rBV2	474	546	0.03%	0.005%
7	3.674	721	726	729	rBV3	449	459	0.03%	0.004%
8	3.707	733	736	739	rVV2	342	220	0.01%	0.002%
9	3.793	760	763	766	rBV2	373	259	0.02%	0.002%
10	3.957	811	814	818	rBV2	429	291	0.02%	0.002%
11	4.012	827	831	833	rBV2	261	178	0.01%	0.001%
12	4.105	857	860	866	rBV2	336	279	0.02%	0.002%
13	4.134	866	869	875	rVB2	289	232	0.01%	0.002%
14	4.224	893	897	900	rBV	390	374	0.02%	0.003%
15	4.295	913	919	923	rBV2	526	487	0.03%	0.004%
16	4.314	923	925	928	rVV	234	133	0.01%	0.001%
17	4.362	938	940	943	rBV2	192	105	0.01%	0.001%
18	4.436	960	963	967	rVB2	485	357	0.02%	0.003%
19	4.472	971	974	978	rBV2	260	257	0.02%	0.002%
20	4.510	984	986	989	rBV	254	138	0.01%	0.001%
21	4.620	1007	1020	1049	rBV	171742	432557	25.99%	3.604%
22	5.060	1142	1157	1184	rVB	309581	671944	40.37%	5.598%
23	5.436	1272	1274	1275	rBV	220	79	0.00%	0.001%
24	5.497	1289	1293	1294	rBV	247	170	0.01%	0.001%
25	5.536	1303	1305	1309	rBV	234	162	0.01%	0.001%
26	5.565	1312	1314	1318	rVB2	340	192	0.01%	0.002%
27	5.616	1328	1330	1332	rBV	210	84	0.01%	0.001%
28	5.642	1335	1338	1339	rBV2	183	100	0.01%	0.001%
29	5.723	1341	1363	1386	rBV2	615250	1664591	100.00%	13.869%
30	6.118	1482	1486	1488	rBV3	452	278	0.02%	0.002%
31	6.247	1510	1526	1546	rBV	449695	849990	51.06%	7.082%
32	6.533	1606	1615	1629	rBV7	4310	8747	0.53%	0.073%
33	6.620	1640	1642	1646	rVB2	464	309	0.02%	0.003%
34	6.687	1649	1663	1681	rBV	405148	786387	47.24%	6.552%
35	6.954	1744	1746	1747	rBV2	236	73	0.00%	0.001%
36	7.038	1770	1772	1776	rBV	318	269	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051169.D
 Acq On : 06 Oct 2022 14:11
 Operator : JC/MD
 Sample : N4893-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.076	1782	1784	1789	rBV	210	158	0.01%	0.001%
38	7.108	1791	1794	1799	rVB2	304	242	0.01%	0.002%
39	7.144	1799	1805	1806	rBV2	317	298	0.02%	0.002%
40	7.169	1810	1813	1814	rBV2	871	482	0.03%	0.004%
41	7.243	1832	1836	1841	rBV2	452	392	0.02%	0.003%
42	7.295	1848	1852	1856	rBV3	327	298	0.02%	0.002%
43	7.340	1862	1866	1872	rVB2	316	376	0.02%	0.003%
44	7.369	1872	1875	1876	rBV	449	215	0.01%	0.002%
45	7.411	1883	1888	1889	rBV2	236	169	0.01%	0.001%
46	7.436	1894	1896	1901	rVB	225	129	0.01%	0.001%
47	7.565	1923	1936	1956	rBV	177577	315510	18.95%	2.629%
48	7.784	2001	2004	2014	rBV6	769	1490	0.09%	0.012%
49	7.896	2025	2039	2053	rBV	677622	1157466	69.53%	9.643%
50	8.111	2103	2106	2110	rBV2	399	323	0.02%	0.003%
51	8.176	2115	2126	2143	rBV	125435	213288	12.81%	1.777%
52	8.552	2231	2243	2256	rBV	83539	140660	8.45%	1.172%
53	8.632	2257	2268	2315	rVV2	428209	930042	55.87%	7.749%
54	8.883	2343	2346	2348	rBV2	489	242	0.01%	0.002%
55	8.954	2366	2368	2371	rVB	663	336	0.02%	0.003%
56	8.980	2371	2376	2381	rBV2	732	629	0.04%	0.005%
57	9.137	2423	2425	2428	rBV2	329	150	0.01%	0.001%
58	9.160	2428	2432	2436	rVV3	534	483	0.03%	0.004%
59	9.343	2484	2489	2493	rBV	311	380	0.02%	0.003%
60	9.414	2498	2511	2539	rVV	648301	1085658	65.22%	9.045%
61	9.619	2574	2575	2576	rBV	200	61	0.00%	0.001%
62	9.658	2584	2587	2589	rBV2	438	301	0.02%	0.003%
63	9.690	2591	2597	2611	rVV2	6086	9362	0.56%	0.078%
64	9.754	2615	2617	2621	rVB	660	359	0.02%	0.003%
65	9.912	2663	2666	2669	rVB3	485	276	0.02%	0.002%
66	10.002	2693	2694	2696	rBV	233	115	0.01%	0.001%
67	10.182	2748	2750	2751	rBV	170	77	0.00%	0.001%
68	10.198	2753	2755	2756	rBV	205	72	0.00%	0.001%
69	10.250	2768	2771	2774	rBV2	353	199	0.01%	0.002%
70	10.279	2777	2780	2783	rBV2	326	248	0.01%	0.002%
71	10.430	2822	2827	2830	rBV2	369	339	0.02%	0.003%
72	10.542	2859	2862	2864	rBV2	383	216	0.01%	0.002%
73	10.610	2881	2883	2888	rVB2	685	504	0.03%	0.004%
74	10.639	2888	2892	2893	rBV2	276	163	0.01%	0.001%
75	10.700	2907	2911	2915	rBV2	489	489	0.03%	0.004%
76	10.754	2915	2928	2947	rVV	613488	985838	59.22%	8.214%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051169.D
 Acq On : 06 Oct 2022 14:11
 Operator : JC/MD
 Sample : N4893-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.976	2994	2997	2999	rVB2	337	205	0.01%	0.002%
78	10.992	2999	3002	3004	rBV	467	276	0.02%	0.002%
79	11.060	3020	3023	3025	rBV2	328	212	0.01%	0.002%
80	11.282	3089	3092	3097	rBV	315	215	0.01%	0.002%
81	11.369	3117	3119	3122	rBV2	240	178	0.01%	0.001%
82	11.404	3128	3130	3133	rVB3	657	278	0.02%	0.002%
83	11.558	3176	3178	3180	rBV	284	140	0.01%	0.001%
84	11.642	3202	3204	3208	rBV2	324	205	0.01%	0.002%
85	11.742	3230	3235	3236	rBV2	1271	973	0.06%	0.008%
86	11.809	3243	3256	3280	rBV	496721	795149	47.77%	6.625%
87	12.037	3325	3327	3329	rBV2	397	201	0.01%	0.002%
88	12.108	3347	3349	3350	rBV2	288	130	0.01%	0.001%
89	12.192	3362	3375	3404	rBV	590276	977272	58.71%	8.142%
90	12.484	3463	3466	3472	rVB3	669	697	0.04%	0.006%
91	12.658	3516	3520	3523	rBV2	457	376	0.02%	0.003%
92	12.774	3552	3556	3559	rBV3	761	634	0.04%	0.005%




Sum of corrected areas: 12002551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051169.D
Acq On : 06 Oct 2022 14:11
Operator : JC/MD
Sample : N4893-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

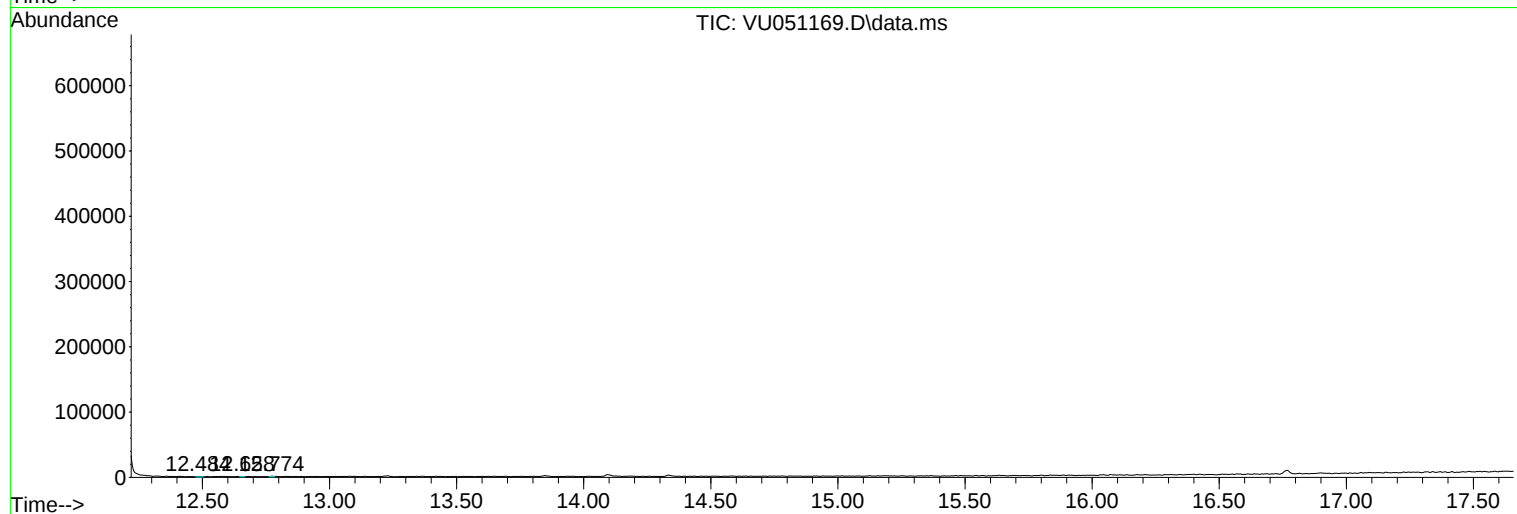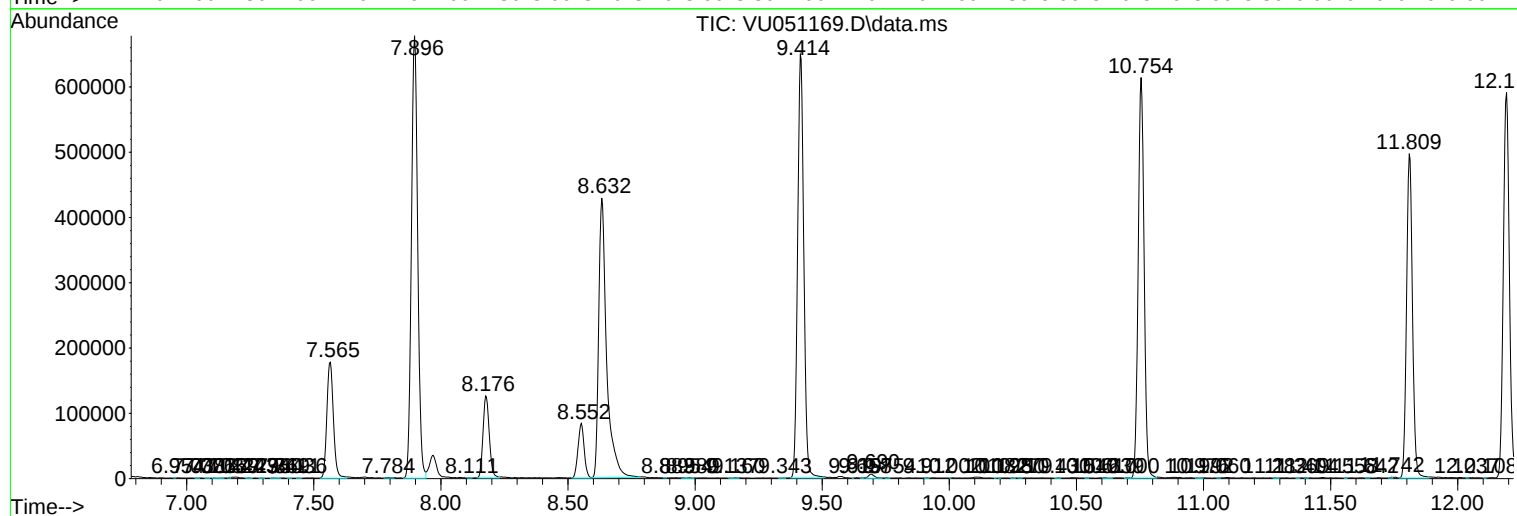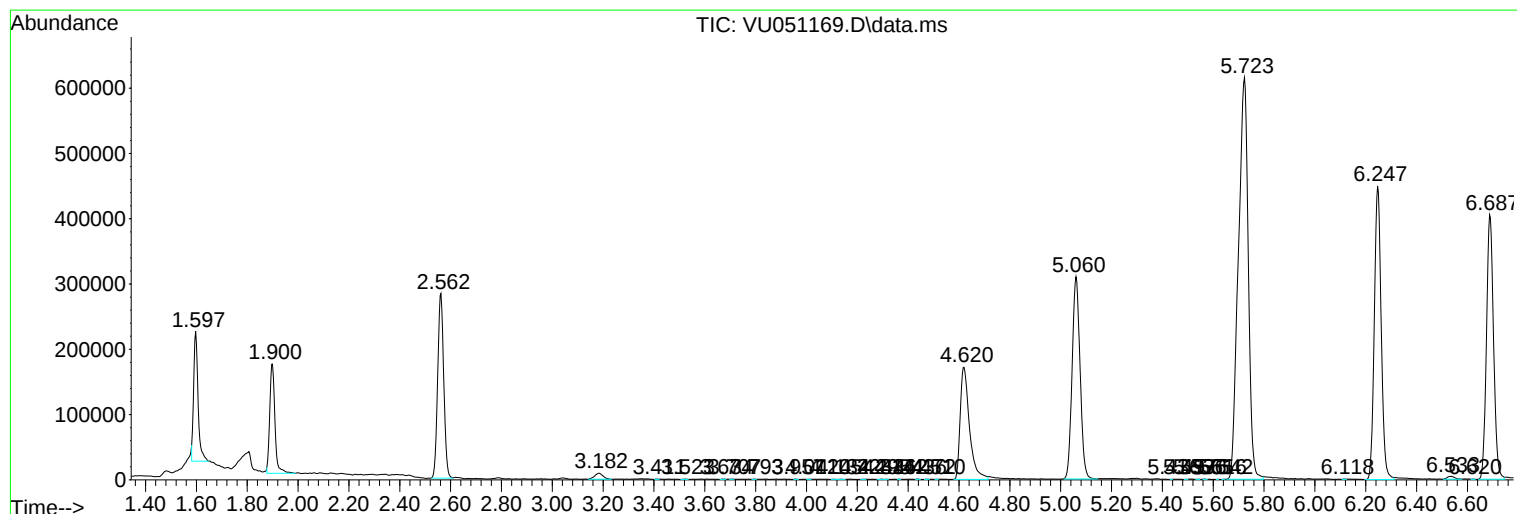

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051169.D
Acq On : 06 Oct 2022 14:11
Operator : JC/MD
Sample : N4893-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051169.D
Acq On : 06 Oct 2022 14:11
Operator : JC/MD
Sample : N4893-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc