

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051173.D
 Acq On : 06 Oct 2022 15:45
 Operator : JC/MD
 Sample : N4853-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW831

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	100	rVB	230529	264225	17.27%	2.278%
2	1.900	167	174	193	rVB	177536	239841	15.67%	2.068%
3	2.562	368	380	396	rBV	299439	491145	32.10%	4.235%
4	3.041	519	529	545	rVB2	12432	22979	1.50%	0.198%
5	3.105	545	549	555	rVB2	457	610	0.04%	0.005%
6	3.134	555	558	559	rBV2	291	177	0.01%	0.002%
7	3.269	598	600	603	rVB	235	82	0.01%	0.001%
8	3.391	636	638	641	rBV	314	233	0.02%	0.002%
9	3.485	663	667	670	rBV2	355	348	0.02%	0.003%
10	3.517	674	677	682	rVB	338	238	0.02%	0.002%
11	3.600	701	703	706	rBV	158	84	0.01%	0.001%
12	3.700	730	734	736	rBV2	273	164	0.01%	0.001%
13	3.716	736	739	743	rVB	639	471	0.03%	0.004%
14	3.748	743	749	753	rBV3	304	366	0.02%	0.003%
15	3.800	763	765	766	rBV	122	59	0.00%	0.001%
16	3.829	772	774	776	rBV2	211	102	0.01%	0.001%
17	3.861	782	784	786	rVB2	221	92	0.01%	0.001%
18	3.877	786	789	791	rBV	279	157	0.01%	0.001%
19	3.954	810	813	815	rBV	150	94	0.01%	0.001%
20	4.076	849	851	853	rBV	224	110	0.01%	0.001%
21	4.125	864	866	870	rVB2	329	226	0.01%	0.002%
22	4.179	880	883	884	rBV	108	49	0.00%	0.000%
23	4.218	892	895	897	rBV	247	119	0.01%	0.001%
24	4.276	909	913	916	rBV	398	273	0.02%	0.002%
25	4.369	938	942	944	rBV	341	255	0.02%	0.002%
26	4.530	988	992	994	rBV3	702	498	0.03%	0.004%
27	4.620	1008	1020	1043	rBV	139021	341502	22.32%	2.945%
28	5.060	1141	1157	1185	rBV2	277612	615866	40.25%	5.310%
29	5.369	1250	1253	1254	rBV2	442	246	0.02%	0.002%
30	5.507	1293	1296	1300	rBV2	212	142	0.01%	0.001%
31	5.533	1301	1304	1307	rBV2	317	254	0.02%	0.002%
32	5.723	1341	1363	1386	rBV2	564072	1530196	100.00%	13.194%
33	5.996	1446	1448	1451	rBV3	352	193	0.01%	0.002%
34	6.247	1509	1526	1551	rBV	554946	1056535	69.05%	9.110%
35	6.533	1607	1615	1622	rBV5	2808	4676	0.31%	0.040%
36	6.587	1629	1632	1633	rBV2	815	419	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051173.D
 Acq On : 06 Oct 2022 15:45
 Operator : JC/MD
 Sample : N4853-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW831

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1686	rBV	364192	714080	46.67%	6.157%
38	6.951	1742	1745	1748	rBV	408	205	0.01%	0.002%
39	6.976	1751	1753	1756	rBV2	372	137	0.01%	0.001%
40	6.993	1756	1758	1760	rBV	171	87	0.01%	0.001%
41	7.044	1772	1774	1777	rVB	190	92	0.01%	0.001%
42	7.076	1777	1784	1790	rBV3	580	794	0.05%	0.007%
43	7.108	1790	1794	1797	rVV2	320	269	0.02%	0.002%
44	7.124	1797	1799	1804	rVB2	294	234	0.02%	0.002%
45	7.153	1804	1808	1811	rBV	357	304	0.02%	0.003%
46	7.240	1832	1835	1837	rBV	272	136	0.01%	0.001%
47	7.282	1847	1848	1849	rBV	201	75	0.00%	0.001%
48	7.333	1862	1864	1869	rVB2	273	201	0.01%	0.002%
49	7.388	1875	1881	1882	rBV	268	209	0.01%	0.002%
50	7.417	1888	1890	1893	rBV2	271	163	0.01%	0.001%
51	7.488	1907	1912	1915	rBV2	302	315	0.02%	0.003%
52	7.565	1920	1936	1955	rBV	171684	303005	19.80%	2.613%
53	7.690	1971	1975	1984	rVB5	1060	1492	0.10%	0.013%
54	7.838	2018	2021	2022	rBV2	229	128	0.01%	0.001%
55	7.896	2026	2039	2053	rBV	617704	1054077	68.89%	9.089%
56	8.176	2116	2126	2145	rBV	119815	202164	13.21%	1.743%
57	8.555	2237	2244	2253	rVB8	3184	4969	0.32%	0.043%
58	8.632	2256	2268	2306	rBV3	336013	756259	49.42%	6.521%
59	8.896	2347	2350	2352	rBV3	531	358	0.02%	0.003%
60	8.951	2364	2367	2369	rVB2	536	256	0.02%	0.002%
61	9.037	2392	2394	2395	rBV	228	93	0.01%	0.001%
62	9.076	2404	2406	2408	rBV	322	167	0.01%	0.001%
63	9.102	2412	2414	2415	rBV	230	76	0.00%	0.001%
64	9.201	2442	2445	2447	rBV	219	135	0.01%	0.001%
65	9.317	2479	2481	2483	rBV	247	150	0.01%	0.001%
66	9.414	2498	2511	2539	rBV	795076	1329983	86.92%	11.468%
67	9.693	2590	2598	2609	rBV3	5389	8122	0.53%	0.070%
68	9.751	2614	2616	2618	rBV	258	144	0.01%	0.001%
69	9.774	2618	2623	2625	rBV2	401	402	0.03%	0.003%
70	9.819	2635	2637	2640	rBV	199	80	0.01%	0.001%
71	9.967	2681	2683	2686	rVB	440	194	0.01%	0.002%
72	9.986	2686	2689	2690	rBV2	233	144	0.01%	0.001%
73	10.092	2718	2722	2724	rBV	650	506	0.03%	0.004%
74	10.234	2764	2766	2771	rBV2	220	147	0.01%	0.001%
75	10.320	2790	2793	2796	rBV	297	257	0.02%	0.002%
76	10.481	2840	2843	2846	rBV2	529	415	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051173.D
 Acq On : 06 Oct 2022 15:45
 Operator : JC/MD
 Sample : N4853-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW831

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.520	2852	2855	2859	rVB3	443	291	0.02%	0.003%
78	10.754	2915	2928	2949	rBV	526871	838338	54.79%	7.229%
79	10.922	2977	2980	2984	rBV	258	181	0.01%	0.002%
80	11.015	3007	3009	3011	rBV	273	178	0.01%	0.002%
81	11.266	3084	3087	3091	rBV2	342	314	0.02%	0.003%
82	11.639	3200	3203	3205	rBV2	240	103	0.01%	0.001%
83	11.809	3244	3256	3276	rBV	581714	938700	61.35%	8.094%
84	12.028	3320	3324	3326	rBV2	420	375	0.02%	0.003%
85	12.066	3326	3336	3358	rVB5	11786	23665	1.55%	0.204%
86	12.192	3362	3375	3393	rBV	516747	840718	54.94%	7.249%
87	12.433	3448	3450	3452	rBV2	402	233	0.02%	0.002%
88	12.552	3485	3487	3489	rBV	333	187	0.01%	0.002%




Sum of corrected areas: 11597333

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051173.D
Acq On : 06 Oct 2022 15:45
Operator : JC/MD
Sample : N4853-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW831

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

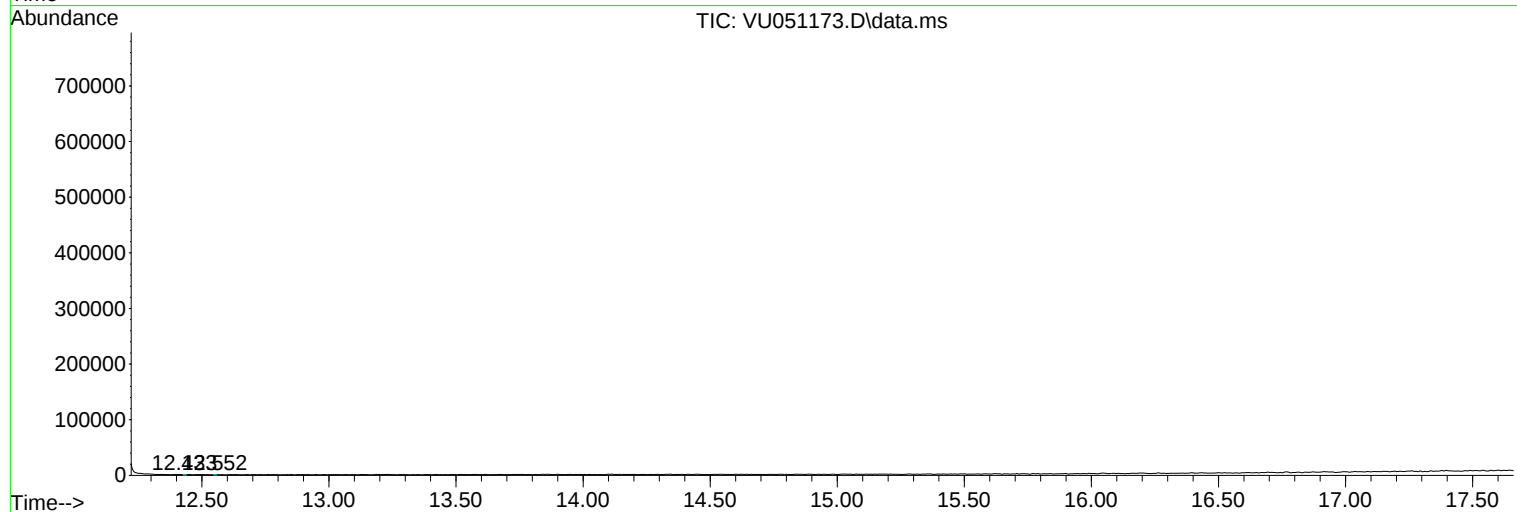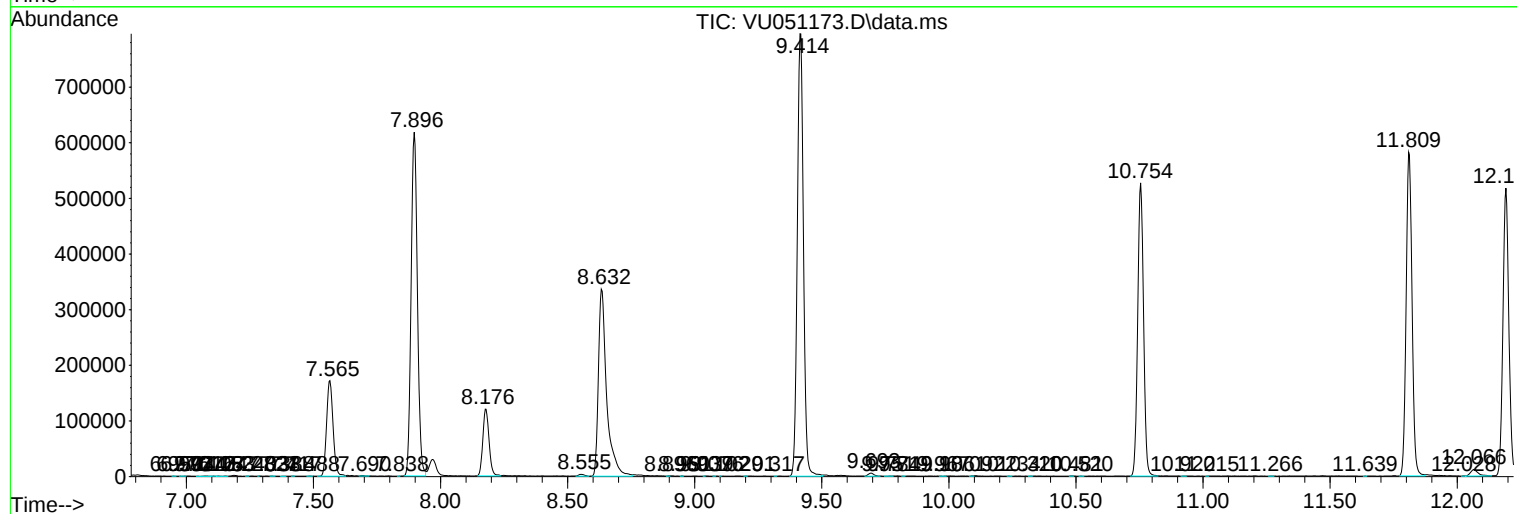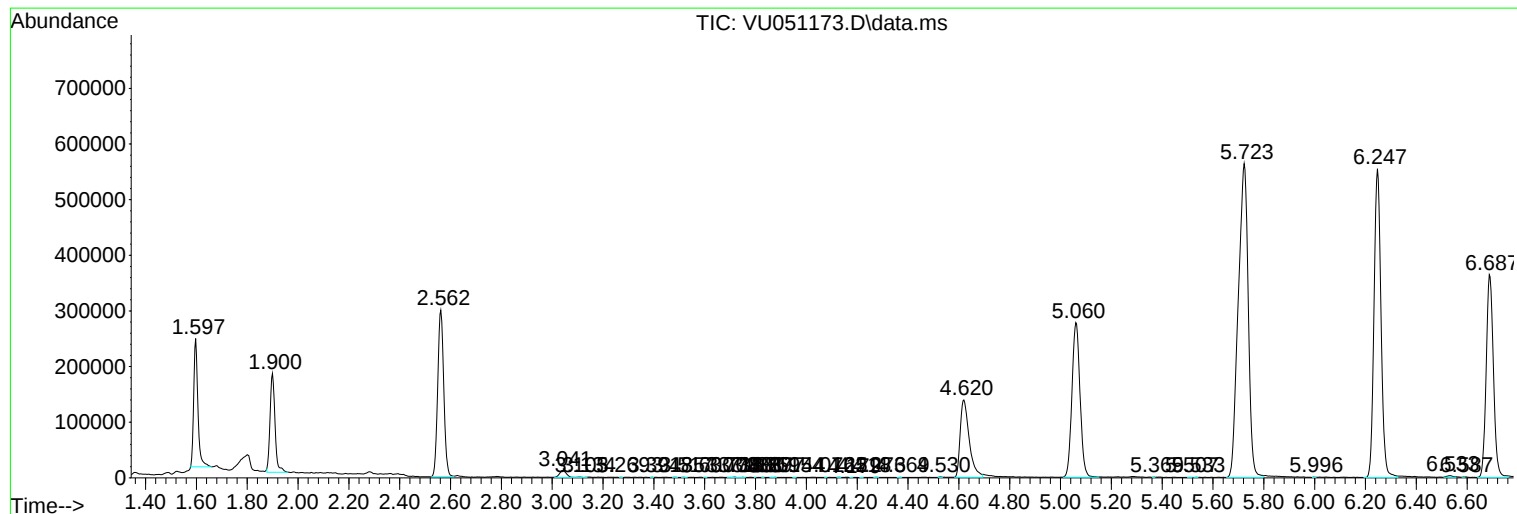

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051173.D
Acq On : 06 Oct 2022 15:45
Operator : JC/MD
Sample : N4853-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW831

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051173.D
Acq On : 06 Oct 2022 15:45
Operator : JC/MD
Sample : N4853-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW831

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc