

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051174.D
 Acq On : 06 Oct 2022 16:09
 Operator : JC/MD
 Sample : N4853-14DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW836DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051174.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rBV	269211	317500	18.37%	2.350%
2	1.900	166	174	191	rVB	200032	268601	15.54%	1.988%
3	2.562	368	380	395	rBV	354951	578672	33.48%	4.284%
4	2.729	429	432	434	rBV2	363	263	0.02%	0.002%
5	2.912	487	489	494	rBV2	300	288	0.02%	0.002%
6	3.038	519	528	544	rVB3	5740	11671	0.68%	0.086%
7	3.182	555	573	588	rBV	27685	63427	3.67%	0.470%
8	3.395	636	639	642	rVV2	344	257	0.01%	0.002%
9	3.417	643	646	652	rVB3	480	403	0.02%	0.003%
10	3.482	660	666	670	rBV3	516	584	0.03%	0.004%
11	3.652	716	719	724	rBV	323	346	0.02%	0.003%
12	3.691	729	731	735	rBV2	438	287	0.02%	0.002%
13	3.832	771	775	781	rBV2	442	441	0.03%	0.003%
14	4.009	825	830	834	rBV2	350	361	0.02%	0.003%
15	4.150	871	874	878	rBV2	323	275	0.02%	0.002%
16	4.301	913	921	925	rBV2	400	446	0.03%	0.003%
17	4.536	991	994	998	rVB2	438	312	0.02%	0.002%
18	4.620	1008	1020	1066	rBV	167524	435357	25.19%	3.223%
19	4.848	1088	1091	1095	rVB5	425	357	0.02%	0.003%
20	4.871	1095	1098	1101	rBV3	651	488	0.03%	0.004%
21	5.060	1140	1157	1177	rBV	316275	693373	40.12%	5.133%
22	5.173	1190	1192	1196	rBV2	458	294	0.02%	0.002%
23	5.292	1221	1229	1235	rBV5	1514	2175	0.13%	0.016%
24	5.379	1250	1256	1261	rBV5	633	844	0.05%	0.006%
25	5.494	1289	1292	1297	rVB2	370	315	0.02%	0.002%
26	5.591	1318	1322	1326	rBV2	260	268	0.02%	0.002%
27	5.723	1341	1363	1389	rBV2	636698	1728178	100.00%	12.793%
28	6.002	1446	1450	1455	rVB4	478	469	0.03%	0.003%
29	6.034	1455	1460	1466	rVB4	599	795	0.05%	0.006%
30	6.118	1480	1486	1492	rVB3	516	626	0.04%	0.005%
31	6.247	1511	1526	1546	rBV	537700	1025374	59.33%	7.590%
32	6.478	1595	1598	1603	rVB2	572	374	0.02%	0.003%
33	6.533	1603	1615	1623	rBV7	3962	8404	0.49%	0.062%
34	6.581	1627	1630	1632	rBV2	431	334	0.02%	0.002%
35	6.690	1649	1664	1686	rBV	406203	803325	46.48%	5.947%
36	7.009	1758	1763	1768	rBV2	255	293	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051174.D
 Acq On : 06 Oct 2022 16:09
 Operator : JC/MD
 Sample : N4853-14DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW836DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.038	1768	1772	1776	rVB	411	276	0.02%	0.002%
38	7.176	1809	1815	1817	rBV2	923	841	0.05%	0.006%
39	7.208	1823	1825	1832	rVB3	736	703	0.04%	0.005%
40	7.305	1848	1855	1858	rBV2	286	330	0.02%	0.002%
41	7.333	1858	1864	1868	rVB2	266	273	0.02%	0.002%
42	7.565	1923	1936	1952	rBV	189544	335608	19.42%	2.484%
43	7.697	1971	1977	1982	rBV4	1046	1319	0.08%	0.010%
44	7.896	2026	2039	2053	rBV	705181	1213461	70.22%	8.983%
45	7.967	2056	2061	2084	rVB	25979	47107	2.73%	0.349%
46	8.179	2111	2127	2145	rBV	137131	231528	13.40%	1.714%
47	8.317	2168	2170	2175	rVB2	406	275	0.02%	0.002%
48	8.552	2229	2243	2257	rBV	455072	769587	44.53%	5.697%
49	8.632	2257	2268	2296	rVV3	392699	851538	49.27%	6.304%
50	8.809	2321	2323	2327	rVB3	794	550	0.03%	0.004%
51	8.829	2327	2329	2334	rVB4	541	285	0.02%	0.002%
52	8.906	2351	2353	2356	rVB3	503	288	0.02%	0.002%
53	8.938	2361	2363	2367	rVB	506	273	0.02%	0.002%
54	8.993	2377	2380	2384	rBV3	487	351	0.02%	0.003%
55	9.157	2429	2431	2436	rVB3	415	330	0.02%	0.002%
56	9.182	2436	2439	2442	rBV	292	256	0.01%	0.002%
57	9.417	2498	2512	2542	rBV	777265	1302073	75.34%	9.639%
58	9.568	2554	2559	2565	rVB4	1535	2065	0.12%	0.015%
59	9.690	2590	2597	2606	rBV2	3583	5723	0.33%	0.042%
60	9.896	2657	2661	2666	rVV2	349	398	0.02%	0.003%
61	9.941	2670	2675	2679	rVB3	491	471	0.03%	0.003%
62	10.099	2721	2724	2728	rBV3	529	404	0.02%	0.003%
63	10.166	2743	2745	2750	rBV2	370	311	0.02%	0.002%
64	10.240	2762	2768	2769	rBV	416	300	0.02%	0.002%
65	10.282	2777	2781	2785	rVB3	370	294	0.02%	0.002%
66	10.317	2786	2792	2796	rVB3	381	407	0.02%	0.003%
67	10.456	2830	2835	2838	rBV	365	333	0.02%	0.002%
68	10.755	2915	2928	2951	rBV	580458	937334	54.24%	6.939%
69	10.919	2974	2979	2983	rBV3	520	459	0.03%	0.003%
70	11.102	3029	3036	3039	rBV5	517	624	0.04%	0.005%
71	11.214	3068	3071	3078	rVB2	370	306	0.02%	0.002%
72	11.253	3081	3083	3088	rVB	441	309	0.02%	0.002%
73	11.410	3129	3132	3136	rBV	387	359	0.02%	0.003%
74	11.645	3201	3205	3209	rBV2	410	283	0.02%	0.002%
75	11.719	3223	3228	3232	rBV2	389	439	0.03%	0.003%
76	11.751	3234	3238	3241	rVB2	629	521	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051174.D
 Acq On : 06 Oct 2022 16:09
 Operator : JC/MD
 Sample : N4853-14DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW836DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.809	3242	3256	3282	rBV	560899	903936	52.31%	6.692%
78	12.066	3329	3336	3351	rBV7	3780	6960	0.40%	0.052%
79	12.192	3360	3375	3398	rBV	566971	933379	54.01%	6.909%
80	12.353	3422	3425	3428	rVB2	415	332	0.02%	0.002%
81	12.517	3471	3476	3478	rBV	344	324	0.02%	0.002%
82	12.690	3527	3530	3536	rBV2	297	314	0.02%	0.002%
83	12.825	3568	3572	3575	rBV2	369	255	0.01%	0.002%
84	12.848	3577	3579	3586	rVB	586	547	0.03%	0.004%
85	12.941	3604	3608	3617	rBV2	1192	1578	0.09%	0.012%
86	13.031	3632	3636	3637	rBV2	485	355	0.02%	0.003%
87	13.086	3651	3653	3656	rBV2	452	325	0.02%	0.002%
88	13.150	3667	3673	3676	rBV2	405	401	0.02%	0.003%
89	13.205	3686	3690	3694	rBV3	497	386	0.02%	0.003%
90	13.590	3806	3810	3811	rBV2	442	282	0.02%	0.002%
91	13.992	3931	3935	3937	rBV3	687	532	0.03%	0.004%
92	14.176	3990	3992	3997	rVB2	584	519	0.03%	0.004%
93	14.285	4023	4026	4027	rBV	491	256	0.01%	0.002%
94	14.330	4037	4040	4041	rBV	528	315	0.02%	0.002%
95	14.748	4168	4170	4173	rVB2	525	280	0.02%	0.002%
96	14.790	4179	4183	4185	rBV3	409	387	0.02%	0.003%
97	14.822	4190	4193	4197	rBV2	745	600	0.03%	0.004%
98	15.108	4280	4282	4289	rVB3	886	752	0.04%	0.006%
99	15.423	4377	4380	4383	rBV2	869	685	0.04%	0.005%
100	15.462	4390	4392	4396	rVB2	950	580	0.03%	0.004%




Sum of corrected areas: 13508649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051174.D
Acq On : 06 Oct 2022 16:09
Operator : JC/MD
Sample : N4853-14DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW836DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

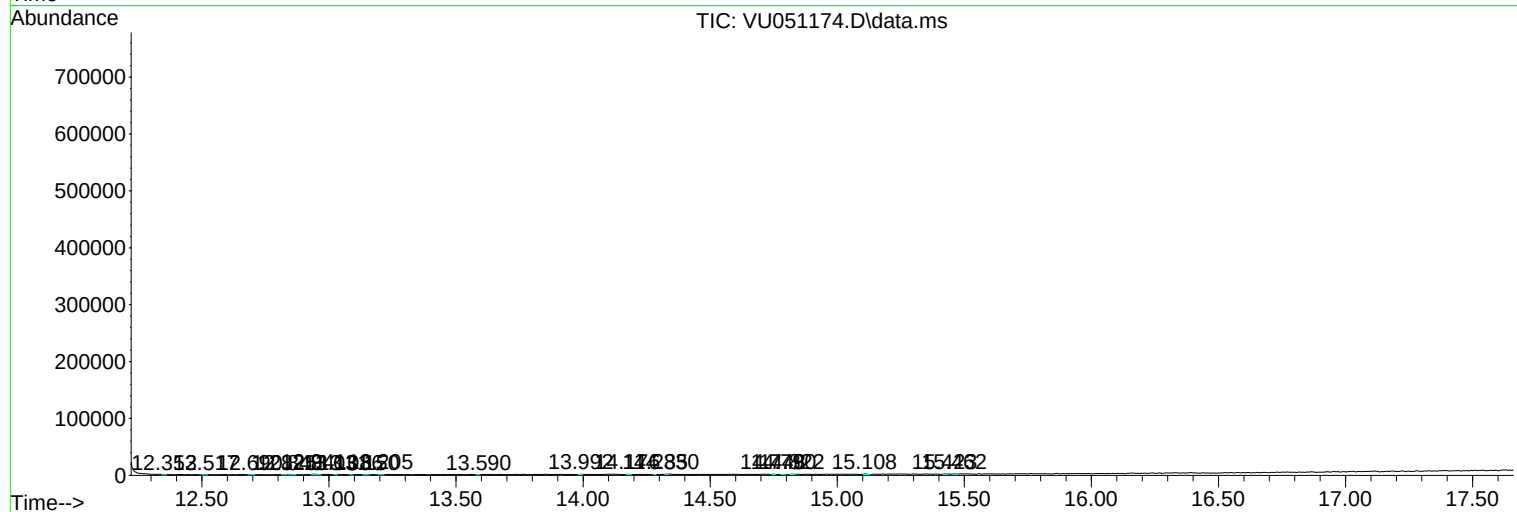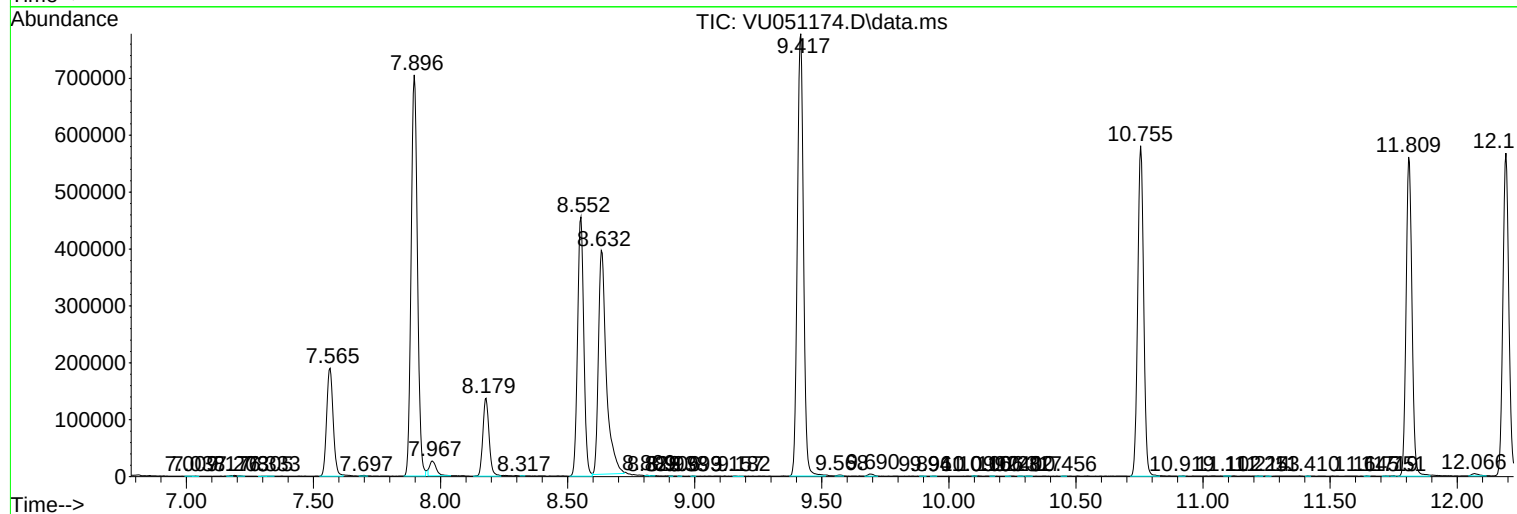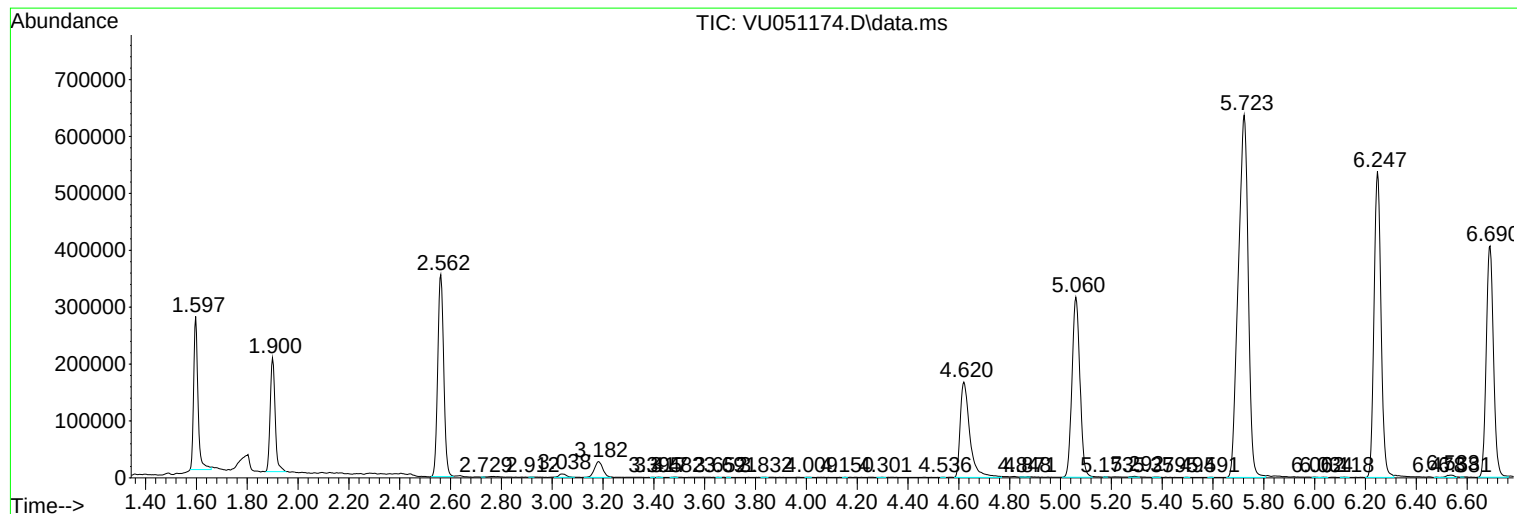

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051174.D
Acq On : 06 Oct 2022 16:09
Operator : JC/MD
Sample : N4853-14DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW836DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051174.D
Acq On : 06 Oct 2022 16:09
Operator : JC/MD
Sample : N4853-14DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW836DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------