

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051182.D
 Acq On : 06 Oct 2022 19:19
 Operator : JC/MD
 Sample : N4893-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	97	rBV	252069	286379	8.78%	1.909%
2	1.900	165	174	190	rVB	189116	253544	7.77%	1.690%
3	2.562	367	380	398	rBV	322660	532811	16.34%	3.552%
4	2.781	444	448	457	rBV5	772	969	0.03%	0.006%
5	3.041	525	529	538	rVB5	1520	2143	0.07%	0.014%
6	3.173	562	570	571	rBV2	2405	2314	0.07%	0.015%
7	3.363	617	629	643	rBV3	4873	11815	0.36%	0.079%
8	3.514	671	676	680	rVB3	381	406	0.01%	0.003%
9	3.555	680	689	690	rBV2	347	273	0.01%	0.002%
10	3.633	704	713	717	rBV2	626	772	0.02%	0.005%
11	3.816	764	770	774	rBV3	539	625	0.02%	0.004%
12	3.883	786	791	795	rVB3	334	313	0.01%	0.002%
13	3.944	805	810	812	rBV2	448	398	0.01%	0.003%
14	4.054	840	844	851	rVB2	320	391	0.01%	0.003%
15	4.144	868	872	877	rBV3	343	294	0.01%	0.002%
16	4.218	889	895	898	rVB2	411	356	0.01%	0.002%
17	4.372	935	943	947	rBV	301	360	0.01%	0.002%
18	4.469	969	973	976	rBV2	464	346	0.01%	0.002%
19	4.620	1006	1020	1048	rBV	139143	351312	10.77%	2.342%
20	4.851	1088	1092	1097	rVB3	569	552	0.02%	0.004%
21	4.922	1111	1114	1121	rVB4	799	716	0.02%	0.005%
22	5.060	1141	1157	1176	rBV	300953	656071	20.12%	4.374%
23	5.224	1205	1208	1212	rVB2	1025	714	0.02%	0.005%
24	5.285	1220	1227	1232	rBV4	1142	1554	0.05%	0.010%
25	5.372	1250	1254	1257	rBV3	496	412	0.01%	0.003%
26	5.443	1273	1276	1280	rVB	414	317	0.01%	0.002%
27	5.469	1280	1284	1288	rBV2	376	399	0.01%	0.003%
28	5.536	1302	1305	1310	rVB2	451	311	0.01%	0.002%
29	5.723	1341	1363	1384	rBV2	596930	1626340	49.87%	10.843%
30	6.009	1449	1452	1457	rVB3	393	377	0.01%	0.003%
31	6.044	1458	1463	1467	rBV3	533	506	0.02%	0.003%
32	6.079	1470	1474	1479	rVB4	472	566	0.02%	0.004%
33	6.153	1495	1497	1505	rVB2	500	458	0.01%	0.003%
34	6.247	1512	1526	1547	rBV	473576	898703	27.56%	5.992%
35	6.459	1588	1592	1596	rVV3	402	339	0.01%	0.002%
36	6.539	1602	1617	1635	rBV6	16117	34378	1.05%	0.229%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051182.D
 Acq On : 06 Oct 2022 19:19
 Operator : JC/MD
 Sample : N4893-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1682	rBV	395791	766774	23.51%	5.112%
38	6.841	1709	1711	1714	rVB3	558	279	0.01%	0.002%
39	7.018	1764	1766	1772	rVB2	418	287	0.01%	0.002%
40	7.067	1779	1781	1785	rVB2	435	340	0.01%	0.002%
41	7.189	1813	1819	1826	rVV7	1199	1972	0.06%	0.013%
42	7.465	1898	1905	1908	rBV	385	399	0.01%	0.003%
43	7.565	1922	1936	1953	rBV	177008	314428	9.64%	2.096%
44	7.896	2025	2039	2054	rBV	653981	1129205	34.63%	7.528%
45	7.970	2055	2062	2079	rVB	20732	37622	1.15%	0.251%
46	8.176	2113	2126	2145	rBV	127541	214190	6.57%	1.428%
47	8.243	2145	2147	2150	rVB2	589	307	0.01%	0.002%
48	8.340	2174	2177	2179	rBV3	459	320	0.01%	0.002%
49	8.443	2204	2209	2214	rVB4	370	475	0.01%	0.003%
50	8.475	2214	2219	2223	rBV3	391	355	0.01%	0.002%
51	8.552	2227	2243	2258	rBV	1942735	3261215	100.00%	21.742%
52	8.636	2258	2269	2301	rVB4	360131	825935	25.33%	5.506%
53	8.854	2335	2337	2340	rBV2	503	297	0.01%	0.002%
54	8.890	2345	2348	2352	rVB2	713	462	0.01%	0.003%
55	8.976	2370	2375	2377	rBV3	571	438	0.01%	0.003%
56	9.163	2429	2433	2438	rBV2	574	537	0.02%	0.004%
57	9.414	2498	2511	2541	rBV	702849	1176971	36.09%	7.847%
58	9.693	2591	2598	2604	rBV5	2919	4356	0.13%	0.029%
59	9.812	2629	2635	2639	rVB2	573	485	0.01%	0.003%
60	9.845	2641	2645	2650	rBV	806	952	0.03%	0.006%
61	9.909	2660	2665	2667	rBV2	370	319	0.01%	0.002%
62	9.925	2668	2670	2673	rVB3	658	380	0.01%	0.003%
63	9.951	2673	2678	2681	rBV2	441	468	0.01%	0.003%
64	10.095	2719	2723	2727	rVB4	540	524	0.02%	0.003%
65	10.253	2764	2772	2774	rBV2	730	854	0.03%	0.006%
66	10.324	2790	2794	2796	rBV2	391	336	0.01%	0.002%
67	10.423	2823	2825	2835	rVB3	502	496	0.02%	0.003%
68	10.468	2835	2839	2841	rBV2	363	315	0.01%	0.002%
69	10.533	2854	2859	2862	rBV2	604	459	0.01%	0.003%
70	10.709	2910	2914	2915	rBV2	437	272	0.01%	0.002%
71	10.754	2915	2928	2951	rVV	546358	890005	27.29%	5.934%
72	11.115	3035	3040	3042	rBV4	619	464	0.01%	0.003%
73	11.224	3070	3074	3078	rVB3	305	310	0.01%	0.002%
74	11.301	3093	3098	3103	rBV3	453	441	0.01%	0.003%
75	11.365	3112	3118	3119	rBV	422	312	0.01%	0.002%
76	11.523	3163	3167	3169	rBV2	508	344	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051182.D
 Acq On : 06 Oct 2022 19:19
 Operator : JC/MD
 Sample : N4893-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.581	3180	3185	3187	rBV	548	451	0.01%	0.003%
78	11.623	3195	3198	3204	rBV3	517	577	0.02%	0.004%
79	11.674	3211	3214	3219	rVB2	395	427	0.01%	0.003%
80	11.809	3243	3256	3280	rBV	501168	808560	24.79%	5.391%
81	11.944	3296	3298	3301	rVB2	733	420	0.01%	0.003%
82	11.992	3310	3313	3315	rBV	405	281	0.01%	0.002%
83	12.076	3335	3339	3340	rBV3	661	380	0.01%	0.003%
84	12.192	3361	3375	3397	rBV	525550	877238	26.90%	5.849%
85	12.555	3485	3488	3493	rBV2	525	485	0.01%	0.003%
86	12.581	3493	3496	3500	rBV3	463	357	0.01%	0.002%
87	12.809	3564	3567	3569	rBV	433	285	0.01%	0.002%
88	13.169	3675	3679	3684	rVB2	539	531	0.02%	0.004%
89	13.259	3703	3707	3708	rBV2	401	342	0.01%	0.002%
90	13.394	3746	3749	3753	rBV	513	422	0.01%	0.003%
91	13.471	3769	3773	3777	rVB3	389	354	0.01%	0.002%
92	13.616	3815	3818	3825	rBV3	503	562	0.02%	0.004%
93	14.044	3949	3951	3954	rVB	553	307	0.01%	0.002%
94	14.166	3987	3989	3993	rBV2	334	271	0.01%	0.002%
95	14.330	4037	4040	4048	rVB2	734	950	0.03%	0.006%
96	14.899	4215	4217	4224	rBV2	650	615	0.02%	0.004%
97	14.941	4227	4230	4232	rBV3	432	320	0.01%	0.002%
98	15.378	4363	4366	4367	rBV	571	369	0.01%	0.002%
99	15.468	4391	4394	4395	rBV2	806	469	0.01%	0.003%
100	15.658	4448	4453	4456	rBV6	895	949	0.03%	0.006%




Sum of corrected areas: 14999356

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051182.D
Acq On : 06 Oct 2022 19:19
Operator : JC/MD
Sample : N4893-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

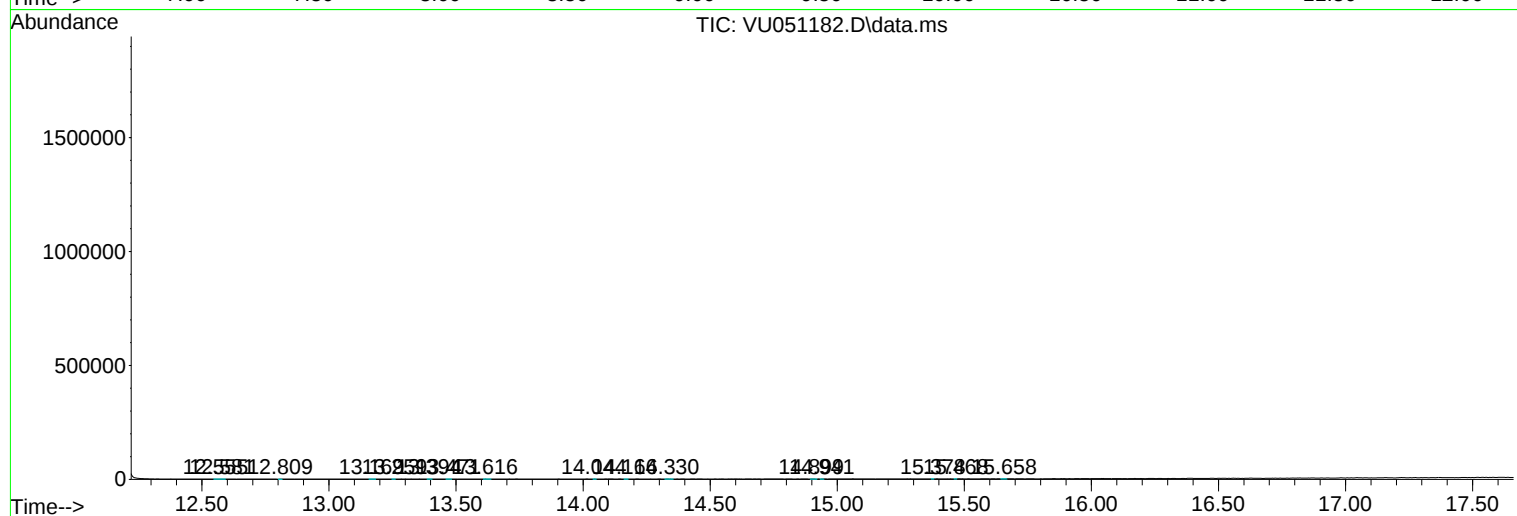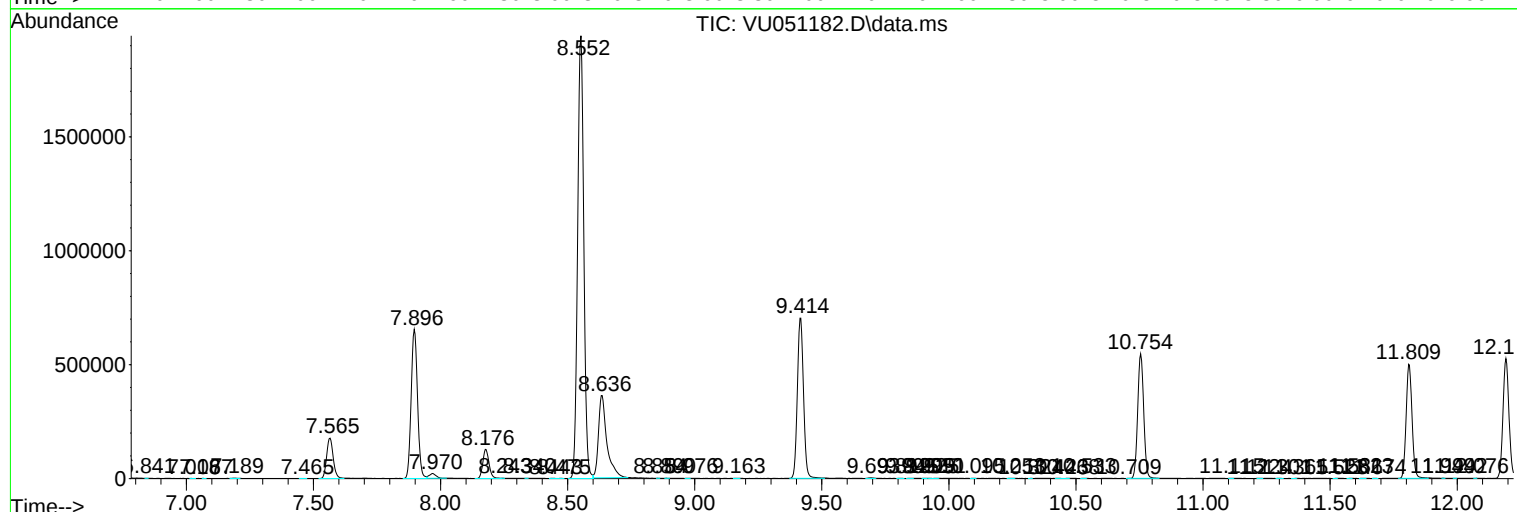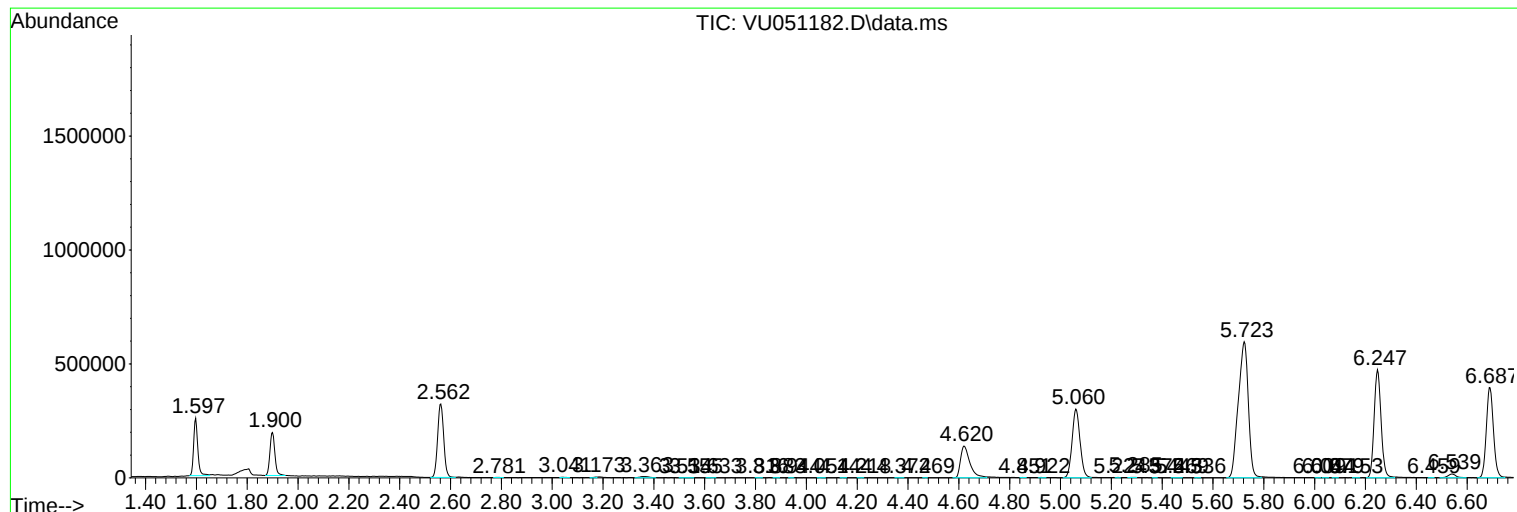

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051182.D
Acq On : 06 Oct 2022 19:19
Operator : JC/MD
Sample : N4893-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051182.D
Acq On : 06 Oct 2022 19:19
Operator : JC/MD
Sample : N4893-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc