

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051183.D
 Acq On : 06 Oct 2022 19:42
 Operator : JC/MD
 Sample : N4893-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	225144	255166	11.76%	2.007%
2	1.900	167	174	199	rVB	174385	241704	11.14%	1.901%
3	2.562	368	380	396	rBV	293558	478872	22.08%	3.766%
4	3.182	563	573	581	rBV	3943	8025	0.37%	0.063%
5	3.295	605	608	611	rBV2	391	316	0.01%	0.002%
6	3.363	618	629	647	rVB3	6135	12368	0.57%	0.097%
7	3.498	667	671	673	rBV2	267	220	0.01%	0.002%
8	3.514	673	676	678	rVV2	268	171	0.01%	0.001%
9	3.552	685	688	690	rVB	261	121	0.01%	0.001%
10	3.636	710	714	717	rBV2	437	270	0.01%	0.002%
11	3.797	762	764	766	rBV2	208	90	0.00%	0.001%
12	3.932	800	806	809	rBV2	326	340	0.02%	0.003%
13	3.973	813	819	821	rBV	428	392	0.02%	0.003%
14	4.141	867	871	873	rBV2	241	183	0.01%	0.001%
15	4.153	873	875	878	rVV2	214	137	0.01%	0.001%
16	4.189	883	886	888	rBV	254	128	0.01%	0.001%
17	4.202	888	890	891	rBV	180	69	0.00%	0.001%
18	4.260	906	908	909	rBV	148	43	0.00%	0.000%
19	4.285	914	916	919	rVB2	345	168	0.01%	0.001%
20	4.308	919	923	926	rBV2	503	366	0.02%	0.003%
21	4.350	933	936	941	rBV2	222	237	0.01%	0.002%
22	4.507	983	985	989	rVB2	267	154	0.01%	0.001%
23	4.565	998	1003	1006	rBV	525	507	0.02%	0.004%
24	4.620	1009	1020	1046	rBV2	126563	322123	14.85%	2.533%
25	5.060	1142	1157	1182	rVB	275099	599188	27.62%	4.712%
26	5.288	1219	1228	1231	rBV4	1522	2036	0.09%	0.016%
27	5.385	1255	1258	1261	rBV3	627	352	0.02%	0.003%
28	5.452	1275	1279	1286	rVB2	510	536	0.02%	0.004%
29	5.488	1287	1290	1294	rBV2	231	226	0.01%	0.002%
30	5.533	1302	1304	1306	rBV2	243	112	0.01%	0.001%
31	5.597	1318	1324	1327	rBV2	416	437	0.02%	0.003%
32	5.642	1335	1338	1339	rBV	191	101	0.00%	0.001%
33	5.723	1339	1363	1388	rBV2	547661	1489907	68.69%	11.716%
34	5.932	1424	1428	1434	rBV5	768	696	0.03%	0.005%
35	6.089	1473	1477	1478	rBV	185	147	0.01%	0.001%
36	6.147	1492	1495	1500	rVB	327	230	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051183.D
 Acq On : 06 Oct 2022 19:42
 Operator : JC/MD
 Sample : N4893-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.247	1512	1526	1546	rBV	416782	790675	36.45%	6.218%
38	6.542	1607	1618	1633	rVB4	22653	45050	2.08%	0.354%
39	6.597	1633	1635	1638	rBV2	433	250	0.01%	0.002%
40	6.690	1649	1664	1684	rBV	358154	699832	32.26%	5.503%
41	6.858	1713	1716	1718	rBV	425	249	0.01%	0.002%
42	6.951	1743	1745	1748	rBV2	398	218	0.01%	0.002%
43	7.025	1765	1768	1771	rVB	371	238	0.01%	0.002%
44	7.041	1771	1773	1776	rBV	202	91	0.00%	0.001%
45	7.057	1776	1778	1780	rBV	117	45	0.00%	0.000%
46	7.073	1780	1783	1788	rBV3	165	180	0.01%	0.001%
47	7.124	1797	1799	1805	rVB3	551	506	0.02%	0.004%
48	7.153	1805	1808	1810	rBV	230	166	0.01%	0.001%
49	7.179	1810	1816	1817	rBV3	836	772	0.04%	0.006%
50	7.250	1834	1838	1839	rBV	163	124	0.01%	0.001%
51	7.321	1858	1860	1868	rBV	398	382	0.02%	0.003%
52	7.356	1869	1871	1873	rVV2	196	73	0.00%	0.001%
53	7.375	1874	1877	1881	rVB2	371	250	0.01%	0.002%
54	7.462	1902	1904	1906	rBV	144	76	0.00%	0.001%
55	7.507	1915	1918	1920	rBV	231	154	0.01%	0.001%
56	7.565	1924	1936	1957	rVV	160066	282437	13.02%	2.221%
57	7.755	1993	1995	1999	rVB2	293	109	0.01%	0.001%
58	7.896	2026	2039	2054	rBV	587996	1013525	46.72%	7.970%
59	8.179	2115	2127	2146	rBV	113300	192599	8.88%	1.515%
60	8.501	2225	2227	2229	rVB	275	87	0.00%	0.001%
61	8.552	2229	2243	2258	rBV	1285509	2169136	100.00%	17.058%
62	8.632	2259	2268	2306	rVB3	314815	741264	34.17%	5.829%
63	9.173	2433	2436	2437	rBV	438	239	0.01%	0.002%
64	9.243	2453	2458	2461	rBV3	436	404	0.02%	0.003%
65	9.259	2461	2463	2468	rVB3	422	244	0.01%	0.002%
66	9.288	2468	2472	2475	rBV2	382	336	0.02%	0.003%
67	9.337	2483	2487	2492	rBV2	269	285	0.01%	0.002%
68	9.417	2497	2512	2546	rBV	620756	1036516	47.78%	8.151%
69	9.613	2568	2573	2576	rBV3	557	531	0.02%	0.004%
70	9.697	2593	2599	2607	rVB4	2021	3041	0.14%	0.024%
71	9.928	2666	2671	2677	rBV2	419	628	0.03%	0.005%
72	9.992	2688	2691	2696	rVB3	511	365	0.02%	0.003%
73	10.128	2731	2733	2735	rBV2	306	129	0.01%	0.001%
74	10.166	2743	2745	2747	rBV2	402	123	0.01%	0.001%
75	10.243	2767	2769	2770	rVB2	171	50	0.00%	0.000%
76	10.256	2770	2773	2775	rBV2	249	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051183.D
 Acq On : 06 Oct 2022 19:42
 Operator : JC/MD
 Sample : N4893-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.272	2775	2778	2780	rBV2	282	194	0.01%	0.002%
78	10.388	2812	2814	2819	rVB	291	209	0.01%	0.002%
79	10.449	2828	2833	2834	rBV2	414	315	0.01%	0.002%
80	10.501	2846	2849	2853	rBV3	269	265	0.01%	0.002%
81	10.581	2871	2874	2878	rVB	400	217	0.01%	0.002%
82	10.600	2878	2880	2882	rBV2	309	149	0.01%	0.001%
83	10.616	2882	2885	2890	rBV	410	311	0.01%	0.002%
84	10.755	2915	2928	2947	rBV	506554	812903	37.48%	6.393%
85	11.214	3067	3071	3073	rBV2	387	325	0.01%	0.003%
86	11.423	3134	3136	3138	rVB	211	83	0.00%	0.001%
87	11.581	3183	3185	3188	rBV2	347	226	0.01%	0.002%
88	11.648	3203	3206	3209	rBV2	378	277	0.01%	0.002%
89	11.809	3244	3256	3283	rBV	437931	712959	32.87%	5.607%
90	12.192	3362	3375	3396	rBV	482740	788959	36.37%	6.204%
91	12.899	3591	3595	3597	rBV	994	776	0.04%	0.006%
92	13.272	3708	3711	3712	rBV2	389	238	0.01%	0.002%
93	14.153	3983	3985	3986	rBV	623	278	0.01%	0.002%




Sum of corrected areas: 12716343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051183.D
Acq On : 06 Oct 2022 19:42
Operator : JC/MD
Sample : N4893-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

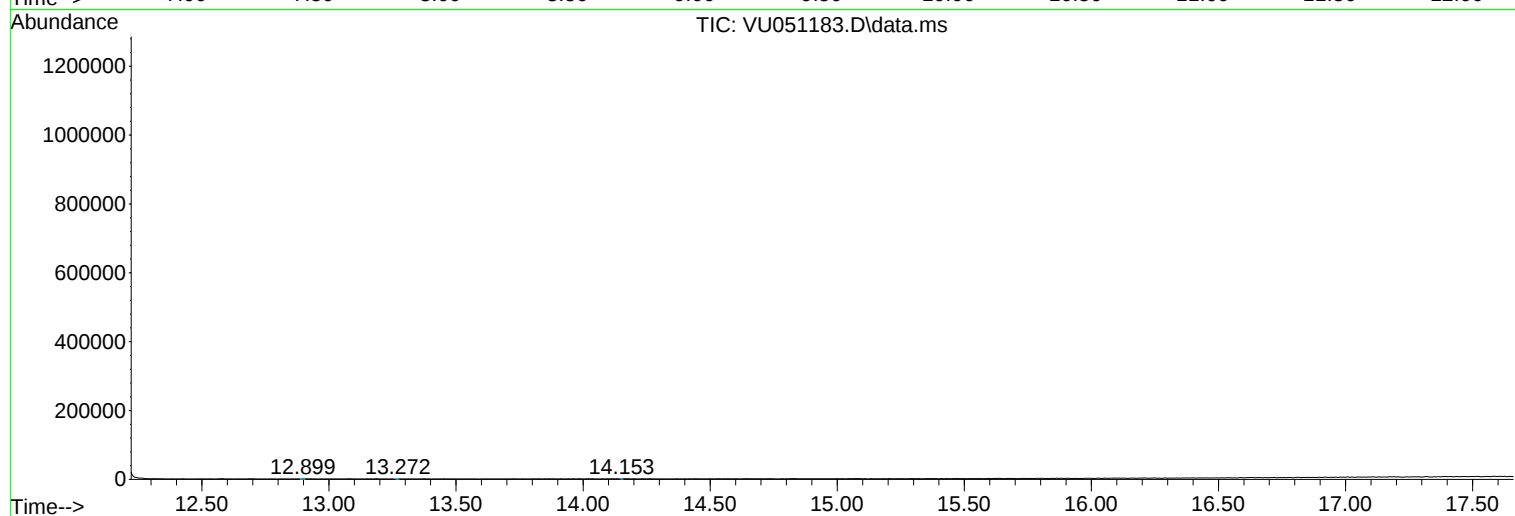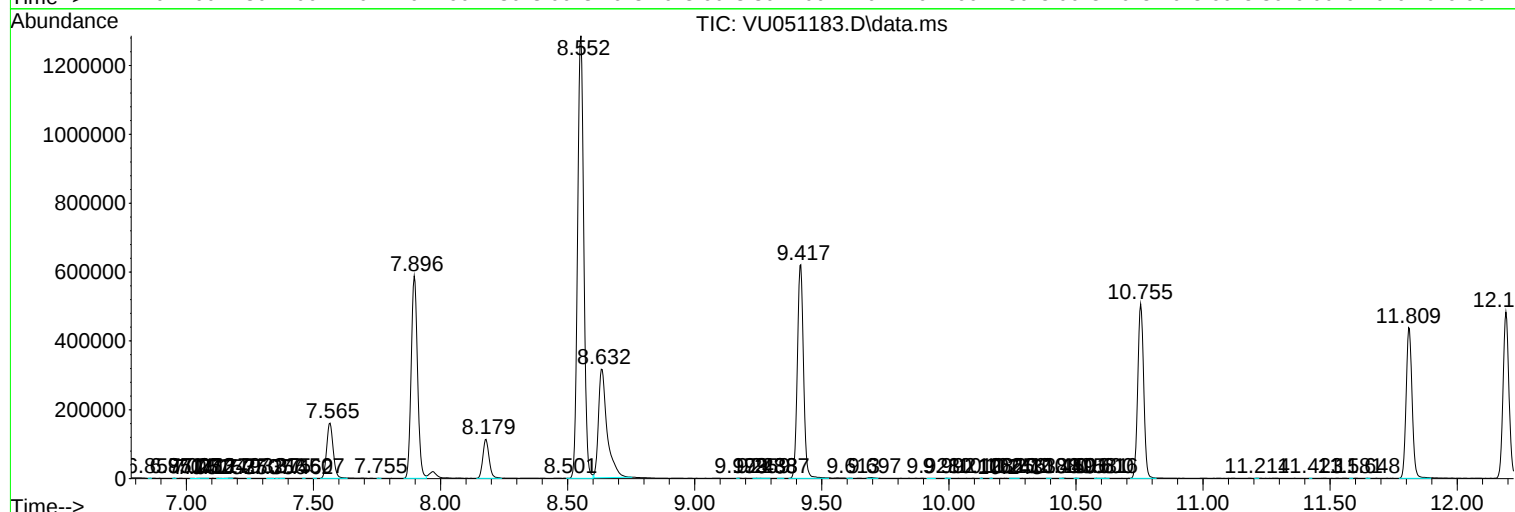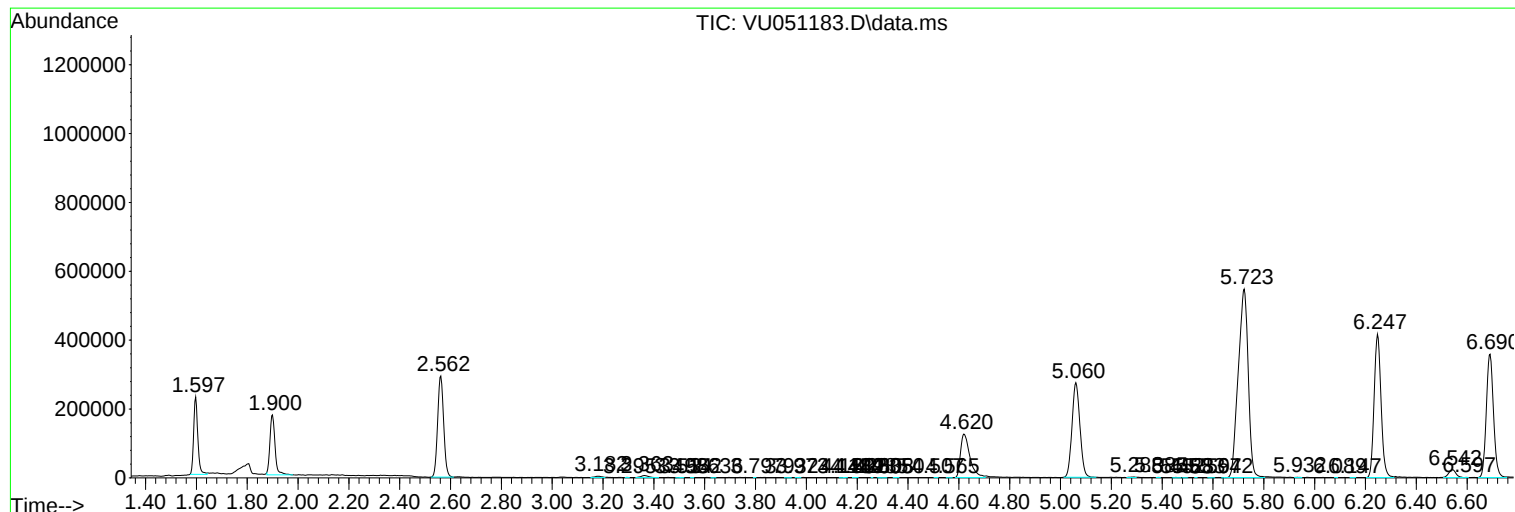

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051183.D
Acq On : 06 Oct 2022 19:42
Operator : JC/MD
Sample : N4893-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051183.D
Acq On : 06 Oct 2022 19:42
Operator : JC/MD
Sample : N4893-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------