

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051184.D
 Acq On : 06 Oct 2022 20:06
 Operator : JC/MD
 Sample : N4893-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051184.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rBV	232858	267106	6.95%	1.781%
2	1.900	166	174	194	rVB	179593	243712	6.34%	1.625%
3	2.562	367	380	397	rBV	302155	492933	12.82%	3.287%
4	2.726	429	431	438	rVB3	611	544	0.01%	0.004%
5	2.787	447	450	452	rBV	427	278	0.01%	0.002%
6	2.871	472	476	477	rBV	491	281	0.01%	0.002%
7	2.932	492	495	498	rVB2	479	298	0.01%	0.002%
8	2.961	498	504	507	rBV3	460	530	0.01%	0.004%
9	3.041	524	529	537	rVB3	1324	1693	0.04%	0.011%
10	3.118	551	553	559	rVB3	515	429	0.01%	0.003%
11	3.179	560	572	585	rVV5	2606	6019	0.16%	0.040%
12	3.231	585	588	591	rVB3	502	345	0.01%	0.002%
13	3.250	591	594	598	rVB2	491	313	0.01%	0.002%
14	3.363	615	629	648	rVB2	17272	39978	1.04%	0.267%
15	3.517	672	677	684	rVB3	556	786	0.02%	0.005%
16	3.610	702	706	709	rBV2	365	277	0.01%	0.002%
17	3.658	718	721	728	rVB2	347	356	0.01%	0.002%
18	3.797	761	764	769	rVB2	293	288	0.01%	0.002%
19	4.105	856	860	866	rBV2	472	616	0.02%	0.004%
20	4.202	887	890	892	rBV	463	297	0.01%	0.002%
21	4.343	928	934	939	rBV2	355	473	0.01%	0.003%
22	4.430	955	961	966	rBV2	482	629	0.02%	0.004%
23	4.620	1006	1020	1055	rBV	133241	341629	8.88%	2.278%
24	4.822	1080	1083	1086	rVB	646	340	0.01%	0.002%
25	4.848	1086	1091	1095	rBV4	558	693	0.02%	0.005%
26	4.938	1115	1119	1124	rBV2	482	456	0.01%	0.003%
27	5.060	1139	1157	1180	rBV	280361	620428	16.13%	4.138%
28	5.170	1188	1191	1194	rVB3	524	312	0.01%	0.002%
29	5.276	1219	1224	1225	rBV3	1253	923	0.02%	0.006%
30	5.372	1251	1254	1255	rBV2	501	319	0.01%	0.002%
31	5.526	1299	1302	1308	rVV4	360	367	0.01%	0.002%
32	5.584	1316	1320	1326	rVV2	315	388	0.01%	0.003%
33	5.723	1341	1363	1387	rBV2	557972	1515270	39.40%	10.105%
34	5.919	1419	1424	1428	rBV2	594	556	0.01%	0.004%
35	6.044	1459	1463	1466	rBV2	317	298	0.01%	0.002%
36	6.108	1479	1483	1489	rBV4	543	709	0.02%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051184.D
 Acq On : 06 Oct 2022 20:06
 Operator : JC/MD
 Sample : N4893-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.247	1509	1526	1550	rBV	454807	859337	22.35%	5.731%
38	6.395	1570	1572	1581	rVB4	969	852	0.02%	0.006%
39	6.481	1597	1599	1605	rVB4	390	452	0.01%	0.003%
40	6.542	1605	1618	1632	rBV2	71375	138001	3.59%	0.920%
41	6.690	1649	1664	1687	rBV	368106	720069	18.73%	4.802%
42	7.179	1808	1816	1817	rBV3	798	887	0.02%	0.006%
43	7.189	1817	1819	1822	rVV3	675	482	0.01%	0.003%
44	7.346	1862	1868	1873	rBV3	285	372	0.01%	0.002%
45	7.504	1915	1917	1922	rVB2	401	313	0.01%	0.002%
46	7.565	1922	1936	1954	rBV2	164547	289568	7.53%	1.931%
47	7.690	1971	1975	1976	rBV2	626	445	0.01%	0.003%
48	7.755	1993	1995	2001	rVB3	412	312	0.01%	0.002%
49	7.896	2026	2039	2054	rVV	608871	1037111	26.97%	6.916%
50	7.970	2055	2062	2078	rVB	19001	34535	0.90%	0.230%
51	8.086	2095	2098	2103	rVB4	779	591	0.02%	0.004%
52	8.131	2109	2112	2116	rBV3	390	286	0.01%	0.002%
53	8.179	2116	2127	2146	rBV	119190	201410	5.24%	1.343%
54	8.459	2211	2214	2216	rVB2	614	387	0.01%	0.003%
55	8.552	2229	2243	2258	rBV	2301909	3845478	100.00%	25.645%
56	8.632	2258	2268	2306	rVB3	332935	781557	20.32%	5.212%
57	8.877	2341	2344	2347	rBV3	755	444	0.01%	0.003%
58	9.214	2443	2449	2451	rBV3	452	458	0.01%	0.003%
59	9.237	2451	2456	2461	rVB3	439	521	0.01%	0.003%
60	9.353	2490	2492	2495	rVB2	483	292	0.01%	0.002%
61	9.417	2495	2512	2535	rBV	668341	1116022	29.02%	7.443%
62	9.549	2548	2553	2557	rBV4	1155	1139	0.03%	0.008%
63	9.655	2583	2586	2587	rBV	549	320	0.01%	0.002%
64	9.690	2591	2597	2607	rVV4	2826	4712	0.12%	0.031%
65	9.861	2648	2650	2656	rVB2	435	330	0.01%	0.002%
66	9.893	2656	2660	2663	rBV3	452	326	0.01%	0.002%
67	10.111	2723	2728	2732	rBV4	507	499	0.01%	0.003%
68	10.189	2749	2752	2759	rBV3	268	281	0.01%	0.002%
69	10.279	2776	2780	2784	rBV2	378	347	0.01%	0.002%
70	10.327	2792	2795	2798	rVB3	469	276	0.01%	0.002%
71	10.755	2911	2928	2947	rBV	512222	835784	21.73%	5.574%
72	11.115	3037	3040	3045	rBV4	390	396	0.01%	0.003%
73	11.156	3050	3053	3054	rBV	490	290	0.01%	0.002%
74	11.291	3092	3095	3099	rVB2	564	449	0.01%	0.003%
75	11.362	3115	3117	3123	rVB	564	557	0.01%	0.004%
76	11.410	3128	3132	3134	rBV2	646	443	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051184.D
 Acq On : 06 Oct 2022 20:06
 Operator : JC/MD
 Sample : N4893-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J15

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.562	3173	3179	3181	rBV	573	593	0.02%	0.004%
78	11.629	3196	3200	3203	rBV2	408	332	0.01%	0.002%
79	11.709	3221	3225	3227	rBV2	427	384	0.01%	0.003%
80	11.812	3244	3257	3278	rBV	473110	760096	19.77%	5.069%
81	12.025	3320	3323	3324	rBV	613	301	0.01%	0.002%
82	12.092	3341	3344	3347	rBV	417	278	0.01%	0.002%
83	12.192	3362	3375	3396	rBV	490711	806160	20.96%	5.376%
84	12.381	3431	3434	3435	rBV	623	306	0.01%	0.002%
85	12.603	3500	3503	3509	rBV4	542	601	0.02%	0.004%
86	12.687	3524	3529	3535	rBV3	494	690	0.02%	0.005%
87	12.854	3578	3581	3584	rBV4	463	330	0.01%	0.002%
88	12.906	3592	3597	3599	rBV4	445	443	0.01%	0.003%
89	13.076	3647	3650	3652	rBV2	502	379	0.01%	0.003%
90	13.330	3725	3729	3731	rBV4	553	419	0.01%	0.003%
91	13.385	3741	3746	3750	rBV3	567	549	0.01%	0.004%
92	13.568	3800	3803	3809	rVB2	656	557	0.01%	0.004%
93	13.825	3880	3883	3888	rBV3	570	486	0.01%	0.003%
94	14.163	3986	3988	3993	rVB3	772	661	0.02%	0.004%
95	14.188	3993	3996	4001	rBV2	497	296	0.01%	0.002%
96	14.233	4006	4010	4012	rBV	496	409	0.01%	0.003%
97	14.928	4222	4226	4230	rVB2	696	654	0.02%	0.004%
98	14.957	4230	4235	4238	rBV2	529	641	0.02%	0.004%
99	15.340	4348	4354	4359	rVB5	1142	1231	0.03%	0.008%
100	15.809	4497	4500	4503	rBV3	991	811	0.02%	0.005%




Sum of corrected areas: 14994807

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051184.D
Acq On : 06 Oct 2022 20:06
Operator : JC/MD
Sample : N4893-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

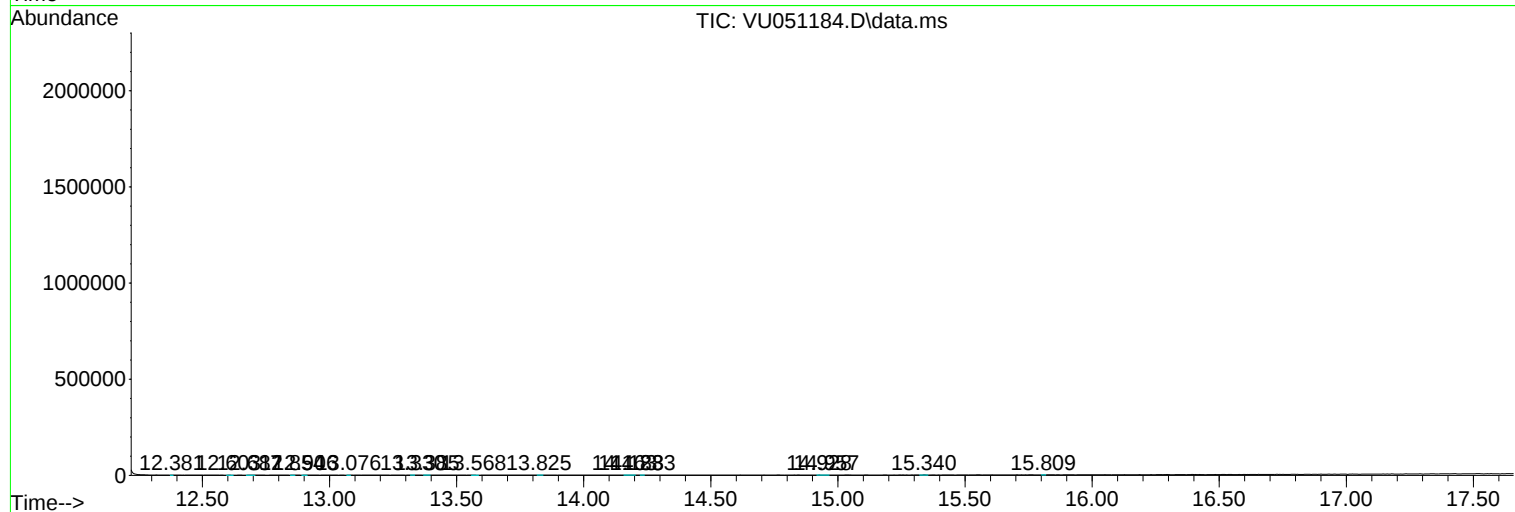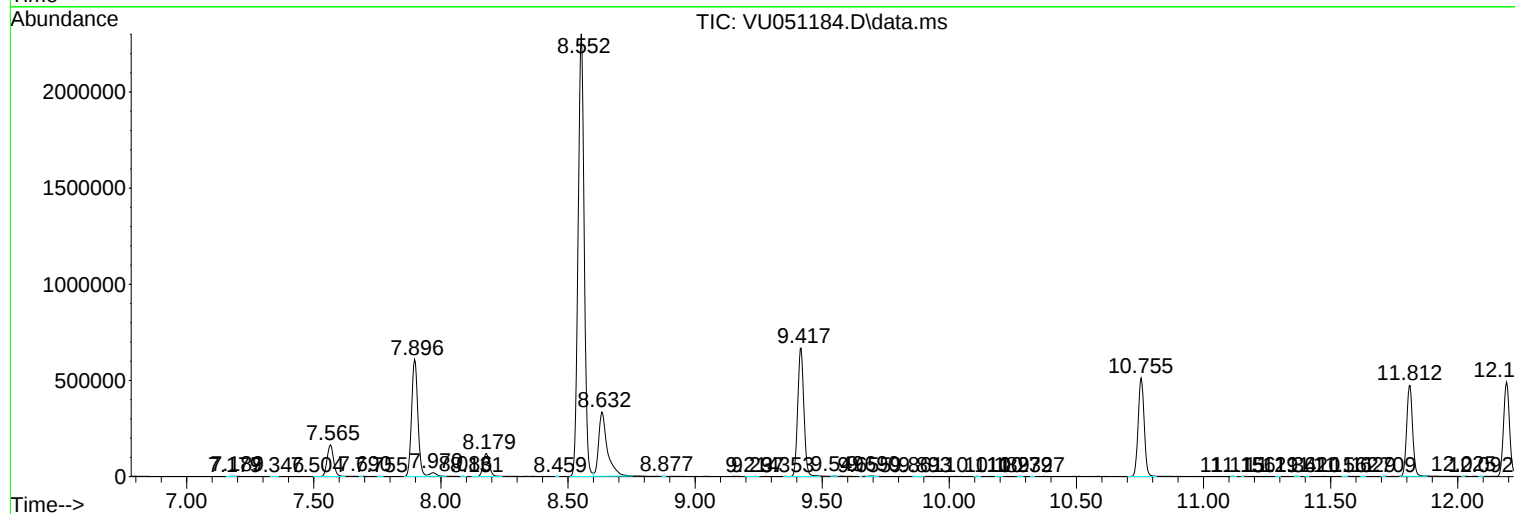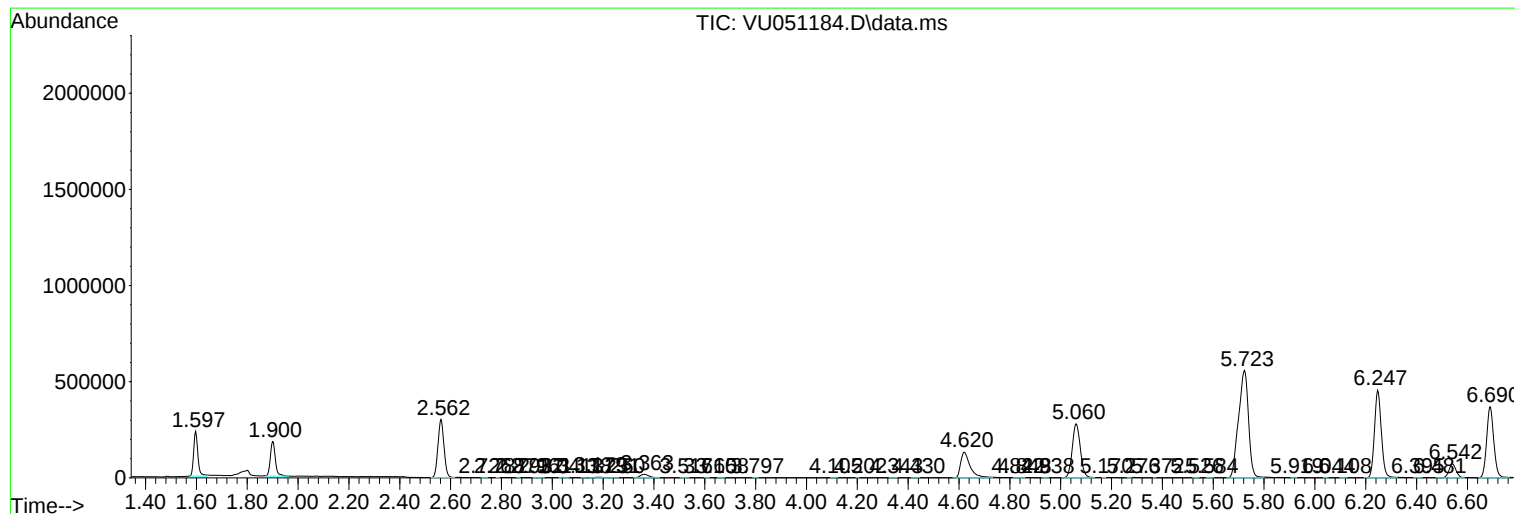

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051184.D
Acq On : 06 Oct 2022 20:06
Operator : JC/MD
Sample : N4893-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051184.D
Acq On : 06 Oct 2022 20:06
Operator : JC/MD
Sample : N4893-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J15

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------