

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051188.D
 Acq On : 06 Oct 2022 22:05
 Operator : JC/MD
 Sample : VU1006WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	263363	293389	17.24%	2.401%
2	1.899	167	174	198	rVB	206817	279298	16.41%	2.285%
3	2.562	368	380	401	rBV	350314	575882	33.84%	4.712%
4	2.977	506	509	514	rBV	517	505	0.03%	0.004%
5	3.041	520	529	540	rBV3	4269	7574	0.45%	0.062%
6	3.182	561	573	583	rBV4	2977	7054	0.41%	0.058%
7	3.260	594	597	599	rBV	372	190	0.01%	0.002%
8	3.305	608	611	616	rBV	396	325	0.02%	0.003%
9	3.343	619	623	624	rBV2	779	524	0.03%	0.004%
10	3.530	678	681	683	rBV2	278	214	0.01%	0.002%
11	3.684	727	729	732	rVB2	417	217	0.01%	0.002%
12	3.880	787	790	794	rBV	241	190	0.01%	0.002%
13	3.932	801	806	808	rBV	544	473	0.03%	0.004%
14	3.944	808	810	813	rVB	276	154	0.01%	0.001%
15	3.973	816	819	821	rBV2	384	212	0.01%	0.002%
16	4.031	835	837	840	rVV	298	148	0.01%	0.001%
17	4.050	840	843	850	rVV2	492	562	0.03%	0.005%
18	4.096	854	857	862	rBV2	237	216	0.01%	0.002%
19	4.147	871	873	877	rVB2	253	121	0.01%	0.001%
20	4.211	890	893	896	rBV2	438	287	0.02%	0.002%
21	4.327	926	929	933	rVB	318	217	0.01%	0.002%
22	4.346	933	935	942	rBV	298	226	0.01%	0.002%
23	4.433	959	962	964	rBV2	282	181	0.01%	0.001%
24	4.494	978	981	986	rBV2	218	199	0.01%	0.002%
25	4.620	1008	1020	1059	rBV	143466	376050	22.10%	3.077%
26	5.060	1141	1157	1180	rBV	313650	686410	40.34%	5.617%
27	5.285	1220	1227	1231	rBV4	897	1305	0.08%	0.011%
28	5.369	1247	1253	1256	rBV4	512	661	0.04%	0.005%
29	5.388	1256	1259	1263	rVB2	687	451	0.03%	0.004%
30	5.478	1284	1287	1290	rBV	185	159	0.01%	0.001%
31	5.520	1296	1300	1304	rBV3	537	490	0.03%	0.004%
32	5.568	1312	1315	1319	rBV2	203	156	0.01%	0.001%
33	5.600	1319	1325	1326	rBV	350	293	0.02%	0.002%
34	5.722	1341	1363	1383	rBV2	632122	1701610	100.00%	13.924%
35	6.015	1452	1454	1455	rBV	250	124	0.01%	0.001%
36	6.044	1460	1463	1468	rVV3	545	550	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051188.D
 Acq On : 06 Oct 2022 22:05
 Operator : JC/MD
 Sample : VU1006WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.086	1472	1476	1479	rBV	408	286	0.02%	0.002%
38	6.105	1479	1482	1484	rBV2	611	352	0.02%	0.003%
39	6.160	1494	1499	1501	rBV2	379	326	0.02%	0.003%
40	6.247	1512	1526	1552	rBV	513599	977882	57.47%	8.002%
41	6.536	1605	1616	1626	rBV8	5201	10380	0.61%	0.085%
42	6.687	1649	1663	1682	rBV	405286	790986	46.48%	6.472%
43	6.893	1724	1727	1729	rBV3	360	228	0.01%	0.002%
44	6.954	1743	1746	1750	rVB2	344	192	0.01%	0.002%
45	7.012	1760	1764	1766	rBV	177	131	0.01%	0.001%
46	7.057	1775	1778	1780	rBB	220	122	0.01%	0.001%
47	7.070	1780	1782	1785	rBV	242	114	0.01%	0.001%
48	7.131	1798	1801	1804	rBV2	315	196	0.01%	0.002%
49	7.150	1804	1807	1810	rBV	357	254	0.01%	0.002%
50	7.256	1838	1840	1844	rVB2	264	144	0.01%	0.001%
51	7.288	1844	1850	1852	rBV2	336	331	0.02%	0.003%
52	7.337	1862	1865	1868	rVB2	513	361	0.02%	0.003%
53	7.388	1879	1881	1885	rVB2	324	219	0.01%	0.002%
54	7.410	1886	1888	1892	rBV2	249	145	0.01%	0.001%
55	7.455	1898	1902	1906	rVB3	379	320	0.02%	0.003%
56	7.565	1923	1936	1957	rBV	179526	322130	18.93%	2.636%
57	7.690	1972	1975	1976	rBV2	672	396	0.02%	0.003%
58	7.896	2025	2039	2054	rBV	694618	1193175	70.12%	9.763%
59	8.176	2115	2126	2146	rVV	127381	222009	13.05%	1.817%
60	8.500	2223	2227	2229	rBV3	294	216	0.01%	0.002%
61	8.513	2229	2231	2233	rVB2	367	125	0.01%	0.001%
62	8.552	2233	2243	2257	rBV2	14440	24373	1.43%	0.199%
63	8.636	2257	2269	2308	rBV3	342296	796125	46.79%	6.515%
64	8.909	2351	2354	2355	rBV2	483	276	0.02%	0.002%
65	8.967	2369	2372	2373	rBV	477	206	0.01%	0.002%
66	8.992	2377	2380	2385	rVV3	710	541	0.03%	0.004%
67	9.021	2388	2389	2393	rVB	557	198	0.01%	0.002%
68	9.050	2395	2398	2402	rBV2	527	416	0.02%	0.003%
69	9.160	2429	2432	2434	rBV3	510	354	0.02%	0.003%
70	9.266	2462	2465	2468	rBV2	313	172	0.01%	0.001%
71	9.285	2468	2471	2474	rBV2	317	251	0.01%	0.002%
72	9.417	2498	2512	2542	rBV	743936	1241039	72.93%	10.155%
73	9.693	2592	2598	2609	rVB6	3404	5688	0.33%	0.047%
74	9.761	2616	2619	2621	rBV2	360	188	0.01%	0.002%
75	9.783	2623	2626	2630	rVV2	449	363	0.02%	0.003%
76	9.877	2653	2655	2659	rBV	218	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051188.D
 Acq On : 06 Oct 2022 22:05
 Operator : JC/MD
 Sample : VU1006WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	9.909	2662	2665	2666	rBV	315	161	0.01%	0.001%
78	9.963	2679	2682	2684	rVB	515	231	0.01%	0.002%
79	9.976	2684	2686	2689	rBV2	184	124	0.01%	0.001%
80	10.115	2721	2729	2736	rBV7	1643	2909	0.17%	0.024%
81	10.330	2792	2796	2800	rBV2	396	314	0.02%	0.003%
82	10.356	2802	2804	2807	rBV	261	174	0.01%	0.001%
83	10.391	2813	2815	2818	rBV	333	162	0.01%	0.001%
84	10.488	2837	2845	2854	rVB2	1535	2041	0.12%	0.017%
85	10.623	2884	2887	2892	rVB2	543	352	0.02%	0.003%
86	10.754	2914	2928	2944	rBV	556112	896693	52.70%	7.337%
87	11.253	3079	3083	3089	rVB2	316	312	0.02%	0.003%
88	11.288	3090	3094	3096	rBV	327	288	0.02%	0.002%
89	11.471	3143	3151	3160	rBV4	2572	3569	0.21%	0.029%
90	11.603	3189	3192	3195	rBV	310	177	0.01%	0.001%
91	11.716	3221	3227	3229	rBV	495	502	0.03%	0.004%
92	11.809	3244	3256	3282	rBV	516184	841039	49.43%	6.882%
93	12.192	3362	3375	3397	rBV	530206	880079	51.72%	7.201%
94	12.870	3583	3586	3588	rBV2	436	291	0.02%	0.002%
95	12.995	3620	3625	3626	rBV2	995	788	0.05%	0.006%
96	13.102	3655	3658	3661	rVB2	684	433	0.03%	0.004%
97	13.227	3689	3697	3707	rVB5	4638	7524	0.44%	0.062%
98	13.844	3883	3889	3901	rVB4	7227	10536	0.62%	0.086%
99	14.092	3957	3966	3984	rVB2	14482	28290	1.66%	0.231%
100	14.333	4033	4041	4058	rVB4	8897	15809	0.93%	0.129%




Sum of corrected areas: 12220778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051188.D
Acq On : 06 Oct 2022 22:05
Operator : JC/MD
Sample : VU1006WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

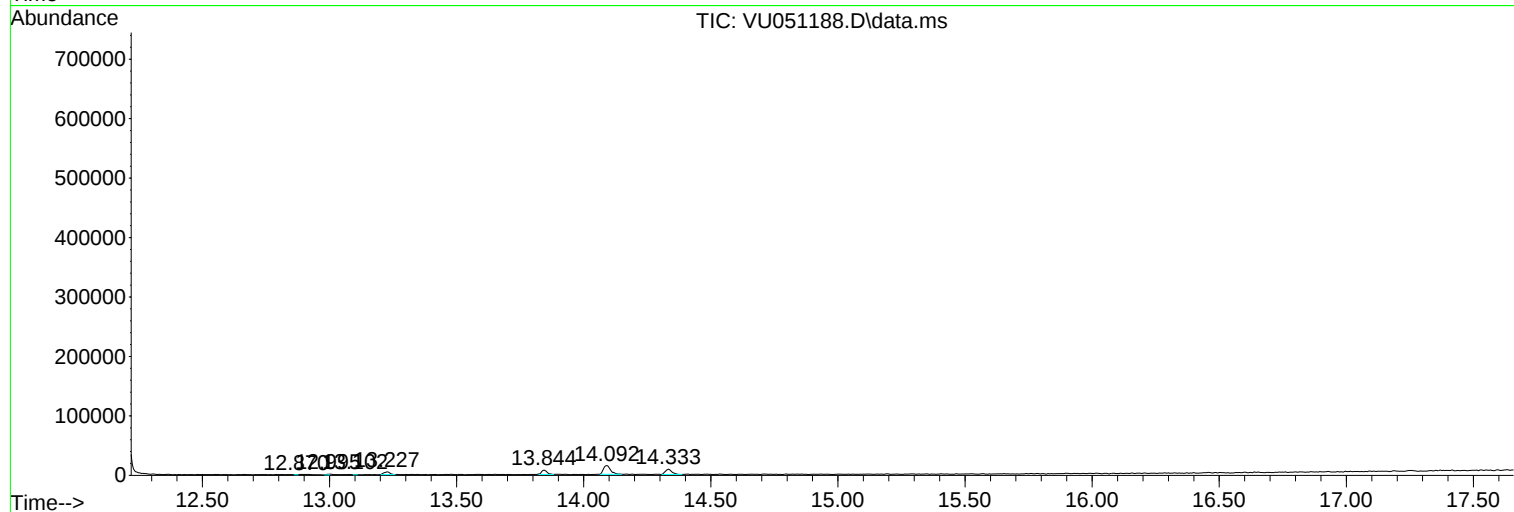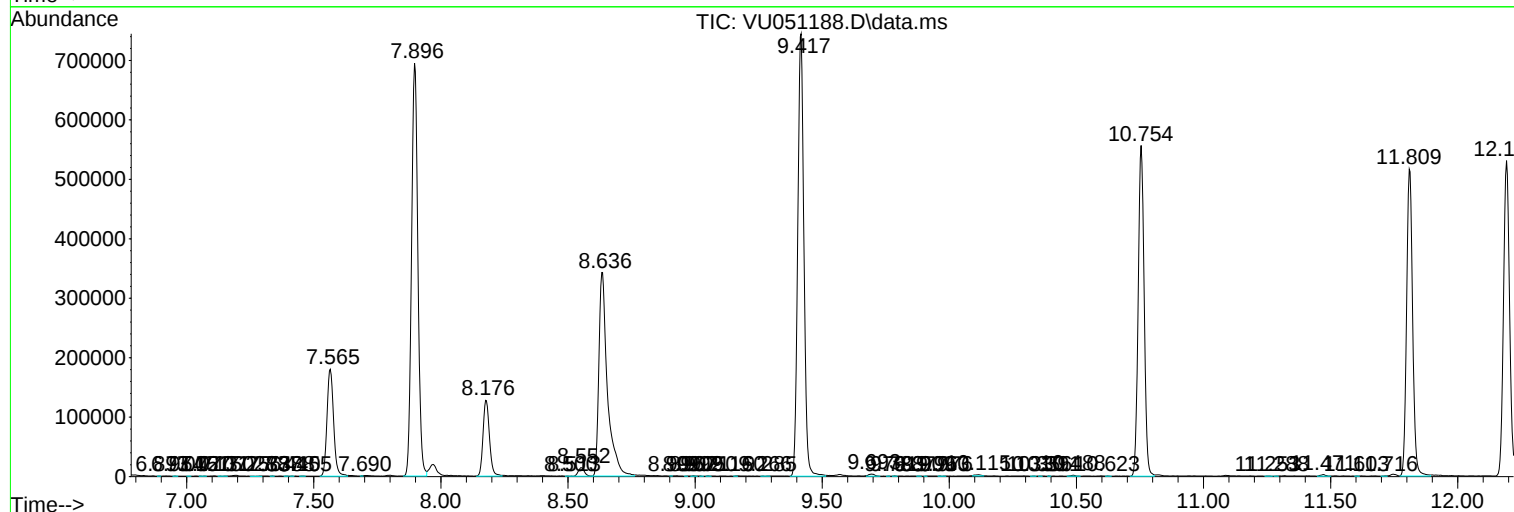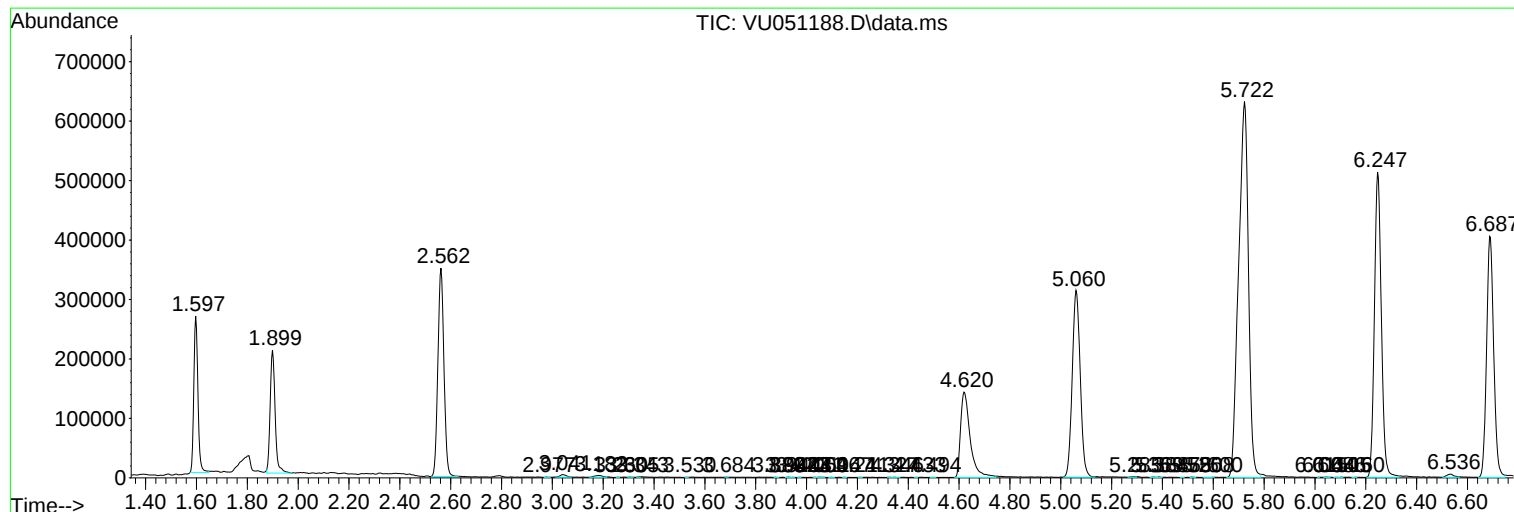

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051188.D
Acq On : 06 Oct 2022 22:05
Operator : JC/MD
Sample : VU1006WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051188.D
Acq On : 06 Oct 2022 22:05
Operator : JC/MD
Sample : VU1006WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------