

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051189.D
 Acq On : 06 Oct 2022 22:29
 Operator : JC/MD
 Sample : N4893-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	182624	201565	0.31%	0.267%
2	1.903	167	175	196	rVB	155688	209910	0.33%	0.278%
3	2.562	368	380	397	rBV	248389	404737	0.63%	0.536%
4	2.787	446	450	460	rVB3	1820	2828	0.00%	0.004%
5	2.977	506	509	512	rBV2	476	283	0.00%	0.000%
6	3.041	522	529	542	rVB5	2008	3576	0.01%	0.005%
7	3.182	560	573	589	rVB2	6677	14948	0.02%	0.020%
8	3.260	595	597	604	rVB2	432	343	0.00%	0.000%
9	3.363	612	629	653	rBV	153934	360602	0.56%	0.477%
10	3.510	672	675	677	rBV	380	270	0.00%	0.000%
11	3.768	751	755	759	rVB2	382	339	0.00%	0.000%
12	3.848	777	780	783	rBV2	547	373	0.00%	0.000%
13	3.980	818	821	824	rVB	434	287	0.00%	0.000%
14	4.060	841	846	850	rVB	433	486	0.00%	0.001%
15	4.157	873	876	883	rVB2	454	432	0.00%	0.001%
16	4.263	904	909	911	rVV2	412	301	0.00%	0.000%
17	4.356	934	938	943	rVB3	309	296	0.00%	0.000%
18	4.395	943	950	954	rBV3	343	500	0.00%	0.001%
19	4.488	974	979	982	rBV2	314	283	0.00%	0.000%
20	4.507	982	985	990	rBV	306	288	0.00%	0.000%
21	4.623	1007	1021	1060	rBV	135343	387478	0.60%	0.513%
22	4.938	1115	1119	1123	rVB2	494	303	0.00%	0.000%
23	5.060	1140	1157	1178	rBV	252746	560697	0.87%	0.742%
24	5.186	1191	1196	1199	rBV3	381	325	0.00%	0.000%
25	5.205	1199	1202	1205	rVB3	381	269	0.00%	0.000%
26	5.288	1219	1228	1236	rBV6	1289	2366	0.00%	0.003%
27	5.526	1299	1302	1309	rVB3	380	414	0.00%	0.001%
28	5.559	1309	1312	1314	rBV2	430	304	0.00%	0.000%
29	5.571	1314	1316	1323	rVB2	457	357	0.00%	0.000%
30	5.723	1342	1363	1390	rBV2	508163	1394297	2.17%	1.845%
31	5.941	1420	1431	1440	rBV5	3716	7026	0.01%	0.009%
32	6.153	1494	1497	1503	rVB2	613	477	0.00%	0.001%
33	6.195	1505	1510	1512	rBV	422	386	0.00%	0.001%
34	6.247	1512	1526	1547	rBV	402718	770016	1.20%	1.019%
35	6.539	1603	1617	1634	rBV2	268124	507239	0.79%	0.671%
36	6.690	1649	1664	1681	rBV	338361	660642	1.03%	0.874%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051189.D
 Acq On : 06 Oct 2022 22:29
 Operator : JC/MD
 Sample : N4893-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.108	1782	1794	1802	rBV4	1496	2437	0.00%	0.003%
38	7.192	1813	1820	1821	rBV4	907	1011	0.00%	0.001%
39	7.356	1864	1871	1874	rBV3	579	598	0.00%	0.001%
40	7.388	1878	1881	1885	rBV2	436	299	0.00%	0.000%
41	7.565	1923	1936	1953	rBV	158308	278333	0.43%	0.368%
42	7.649	1960	1962	1968	rVB3	625	517	0.00%	0.001%
43	7.684	1971	1973	1975	rBV3	542	320	0.00%	0.000%
44	7.796	2002	2008	2013	rBV2	1138	1221	0.00%	0.002%
45	7.896	2025	2039	2054	rBV	547047	946230	1.48%	1.252%
46	7.967	2056	2061	2074	rVB2	19946	33270	0.05%	0.044%
47	8.050	2083	2087	2091	rVB2	649	630	0.00%	0.001%
48	8.128	2107	2111	2115	rVB3	525	537	0.00%	0.001%
49	8.179	2115	2127	2143	rBV2	110069	188883	0.29%	0.250%
50	8.330	2171	2174	2176	rBV	564	341	0.00%	0.000%
51	8.369	2183	2186	2190	rBV2	297	267	0.00%	0.000%
52	8.462	2211	2215	2218	rVB2	394	306	0.00%	0.000%
53	8.555	2226	2244	2260	rBV	38605660	64116161	100.00%	84.848%
54	8.632	2262	2268	2308	rVB3	411800	999980	1.56%	1.323%
55	9.060	2398	2401	2407	rBV3	592	521	0.00%	0.001%
56	9.163	2427	2433	2437	rBV4	1079	1115	0.00%	0.001%
57	9.417	2498	2512	2537	rBV	636119	1060039	1.65%	1.403%
58	9.571	2553	2560	2570	rVB4	2921	4513	0.01%	0.006%
59	9.697	2591	2599	2607	rVB2	4727	6832	0.01%	0.009%
60	9.771	2620	2622	2626	rVB3	551	343	0.00%	0.000%
61	9.803	2626	2632	2633	rBV3	350	310	0.00%	0.000%
62	10.108	2717	2727	2736	rBV7	1850	3250	0.01%	0.004%
63	10.189	2747	2752	2759	rBV2	307	438	0.00%	0.001%
64	10.320	2787	2793	2796	rBV4	485	542	0.00%	0.001%
65	10.385	2808	2813	2815	rBV3	422	390	0.00%	0.001%
66	10.427	2822	2826	2832	rBV3	305	277	0.00%	0.000%
67	10.481	2839	2843	2850	rVB4	1027	1319	0.00%	0.002%
68	10.584	2867	2875	2879	rBV3	517	695	0.00%	0.001%
69	10.687	2902	2907	2909	rBV3	296	307	0.00%	0.000%
70	10.755	2912	2928	2945	rBV	498661	798667	1.25%	1.057%
71	11.005	3001	3006	3008	rBV3	559	435	0.00%	0.001%
72	11.089	3028	3032	3037	rBV3	1366	1239	0.00%	0.002%
73	11.134	3043	3046	3051	rVB2	541	477	0.00%	0.001%
74	11.208	3067	3069	3072	rVB2	530	289	0.00%	0.000%
75	11.301	3094	3098	3105	rBV3	295	360	0.00%	0.000%
76	11.468	3144	3150	3158	rBV3	1363	1802	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051189.D
 Acq On : 06 Oct 2022 22:29
 Operator : JC/MD
 Sample : N4893-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.748	3230	3237	3244	rBV4	3206	4609	0.01%	0.006%
78	11.809	3244	3256	3274	rBV	473434	765737	1.19%	1.013%
79	12.192	3362	3375	3398	rBV	485031	809405	1.26%	1.071%
80	12.645	3510	3516	3519	rBV3	775	860	0.00%	0.001%
81	12.761	3547	3552	3555	rBV3	662	678	0.00%	0.001%
82	12.893	3590	3593	3595	rBV3	374	290	0.00%	0.000%
83	13.008	3626	3629	3633	rBV3	410	313	0.00%	0.000%
84	13.105	3656	3659	3662	rBV3	621	390	0.00%	0.001%
85	13.224	3690	3696	3706	rBV7	3151	4998	0.01%	0.007%
86	13.359	3733	3738	3740	rBV	354	388	0.00%	0.001%
87	13.648	3826	3828	3832	rBV2	560	402	0.00%	0.001%
88	13.716	3847	3849	3853	rBV3	425	366	0.00%	0.000%
89	13.770	3863	3866	3870	rBV2	695	536	0.00%	0.001%
90	13.848	3883	3890	3898	rVB4	3790	5098	0.01%	0.007%
91	14.092	3958	3966	3975	rBV2	6472	10786	0.02%	0.014%
92	14.156	3984	3986	3992	rBV3	373	292	0.00%	0.000%
93	14.227	4005	4008	4013	rBV3	425	351	0.00%	0.000%
94	14.333	4034	4041	4047	rBV4	4261	5729	0.01%	0.008%
95	14.732	4163	4165	4175	rBV4	511	703	0.00%	0.001%
96	15.295	4338	4340	4343	rBV2	569	415	0.00%	0.001%
97	15.520	4405	4410	4413	rBV5	797	865	0.00%	0.001%
98	15.667	4454	4456	4459	rBV2	646	405	0.00%	0.001%
99	15.706	4465	4468	4473	rVB3	1258	1175	0.00%	0.002%
100	15.732	4473	4476	4479	rBV3	911	679	0.00%	0.001%




Sum of corrected areas: 75566214

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051189.D
Acq On : 06 Oct 2022 22:29
Operator : JC/MD
Sample : N4893-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

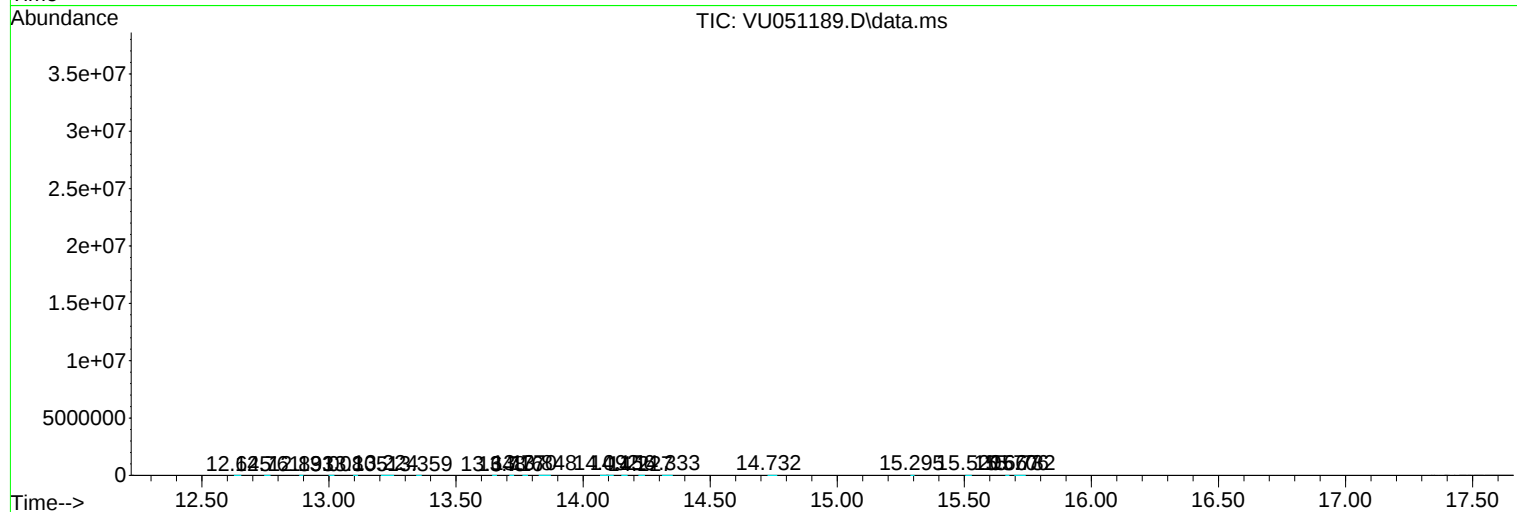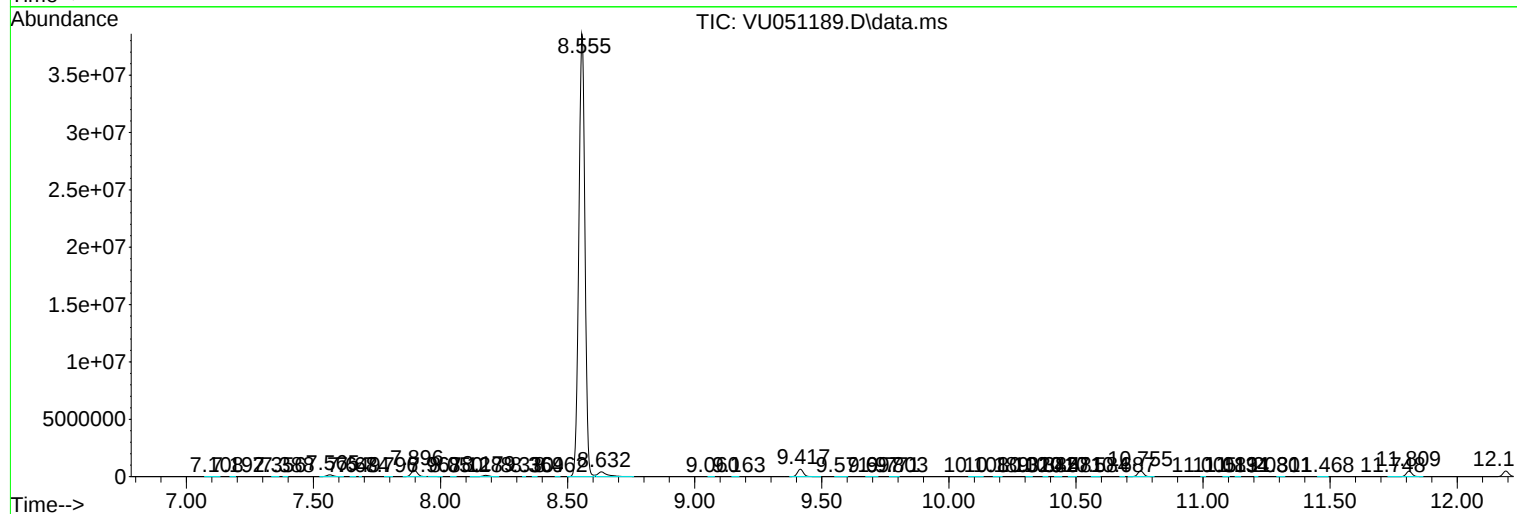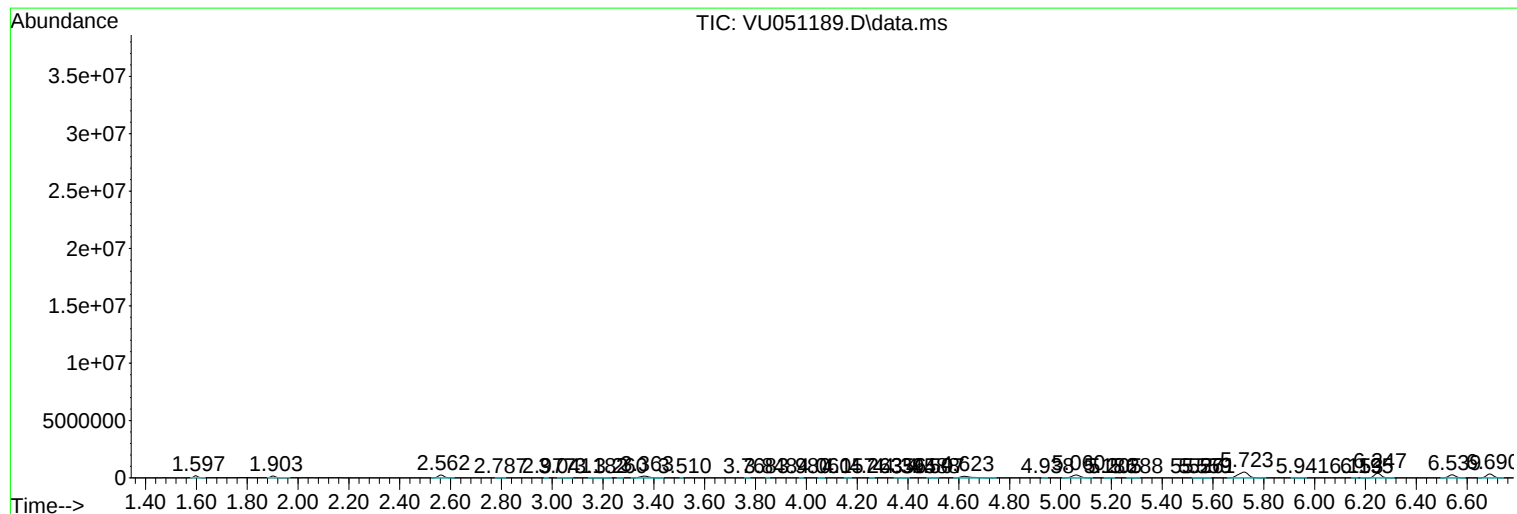

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051189.D
Acq On : 06 Oct 2022 22:29
Operator : JC/MD
Sample : N4893-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051189.D
Acq On : 06 Oct 2022 22:29
Operator : JC/MD
Sample : N4893-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc