

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051190.D
 Acq On : 06 Oct 2022 22:52
 Operator : JC/MD
 Sample : N4893-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051190.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	37	42	51	rBV4	4970	6860	0.14%	0.043%
2	1.597	73	80	91	rBV	219991	245900	5.02%	1.533%
3	1.903	166	175	193	rVB	173214	238203	4.87%	1.485%
4	2.562	368	380	393	rBV	292309	479430	9.80%	2.989%
5	2.626	394	400	417	rVB	14091	24456	0.50%	0.152%
6	2.781	443	448	451	rBV3	1585	1725	0.04%	0.011%
7	2.871	473	476	481	rBV4	444	384	0.01%	0.002%
8	3.044	521	530	533	rVV5	1236	1743	0.04%	0.011%
9	3.183	560	573	587	rVB2	4790	11362	0.23%	0.071%
10	3.363	615	629	642	rBV3	11747	26447	0.54%	0.165%
11	3.562	686	691	697	rBV3	395	404	0.01%	0.003%
12	3.716	736	739	745	rVB2	390	377	0.01%	0.002%
13	3.777	754	758	761	rBV3	1066	996	0.02%	0.006%
14	3.932	802	806	810	rVB2	397	352	0.01%	0.002%
15	3.964	810	816	818	rBV2	465	486	0.01%	0.003%
16	4.620	1008	1020	1058	rBV	133619	348975	7.13%	2.176%
17	4.945	1117	1121	1126	rBB3	414	429	0.01%	0.003%
18	5.060	1140	1157	1177	rBV	282590	624461	12.76%	3.894%
19	5.266	1218	1221	1223	rBV3	625	399	0.01%	0.002%
20	5.285	1224	1227	1237	rVB5	1320	1931	0.04%	0.012%
21	5.346	1243	1246	1248	rBV2	354	295	0.01%	0.002%
22	5.385	1254	1258	1261	rBV2	571	356	0.01%	0.002%
23	5.433	1270	1273	1277	rBV2	388	308	0.01%	0.002%
24	5.520	1297	1300	1304	rVB2	469	283	0.01%	0.002%
25	5.549	1304	1309	1313	rBV2	516	377	0.01%	0.002%
26	5.575	1313	1317	1321	rBV3	423	420	0.01%	0.003%
27	5.600	1322	1325	1331	rVB3	387	391	0.01%	0.002%
28	5.723	1341	1363	1383	rBV2	561599	1532238	31.31%	9.554%
29	5.990	1442	1446	1450	rVB4	633	570	0.01%	0.004%
30	6.012	1450	1453	1456	rVB2	507	340	0.01%	0.002%
31	6.041	1456	1462	1466	rBV4	690	858	0.02%	0.005%
32	6.076	1468	1473	1478	rVB4	386	411	0.01%	0.003%
33	6.115	1479	1485	1488	rBV3	598	634	0.01%	0.004%
34	6.247	1512	1526	1552	rBV	433230	832816	17.02%	5.193%
35	6.385	1566	1569	1575	rBV4	900	639	0.01%	0.004%
36	6.543	1605	1618	1630	rBV5	38801	75581	1.54%	0.471%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051190.D
 Acq On : 06 Oct 2022 22:52
 Operator : JC/MD
 Sample : N4893-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1649	1663	1684	rBV	368777	724975	14.81%	4.520%
38	6.928	1735	1738	1744	rVB2	583	445	0.01%	0.003%
39	7.018	1760	1766	1769	rBV3	487	413	0.01%	0.003%
40	7.121	1795	1798	1802	rVB	491	351	0.01%	0.002%
41	7.186	1812	1818	1823	rBV4	1432	1560	0.03%	0.010%
42	7.565	1921	1936	1960	rBV	164167	298232	6.09%	1.860%
43	7.694	1971	1976	1977	rBV2	663	604	0.01%	0.004%
44	7.787	2000	2005	2007	rBV2	819	645	0.01%	0.004%
45	7.896	2025	2039	2054	rBV	614580	1057993	21.62%	6.597%
46	7.970	2057	2062	2073	rVB3	16548	25523	0.52%	0.159%
47	8.179	2115	2127	2141	rBV	118467	202322	4.13%	1.262%
48	8.391	2190	2193	2199	rBV3	595	554	0.01%	0.003%
49	8.552	2225	2243	2258	rBV	2938986	4893575	100.00%	30.513%
50	8.633	2259	2268	2301	rVB3	343651	805164	16.45%	5.020%
51	8.832	2328	2330	2335	rVB4	879	782	0.02%	0.005%
52	8.928	2357	2360	2365	rVB4	485	420	0.01%	0.003%
53	9.034	2391	2393	2397	rVB2	458	309	0.01%	0.002%
54	9.166	2430	2434	2438	rVV3	472	544	0.01%	0.003%
55	9.195	2438	2443	2448	rVB3	348	394	0.01%	0.002%
56	9.414	2495	2511	2531	rBV	657935	1087534	22.22%	6.781%
57	9.565	2555	2558	2566	rBV5	1364	1722	0.04%	0.011%
58	9.694	2592	2598	2611	rVB3	3432	5232	0.11%	0.033%
59	9.748	2611	2615	2618	rBV	351	311	0.01%	0.002%
60	10.099	2718	2724	2725	rBV4	1058	966	0.02%	0.006%
61	10.108	2725	2727	2730	rVB3	750	475	0.01%	0.003%
62	10.292	2776	2784	2791	rBV3	550	971	0.02%	0.006%
63	10.369	2803	2808	2813	rVB2	321	361	0.01%	0.002%
64	10.485	2837	2844	2850	rVB4	769	1094	0.02%	0.007%
65	10.575	2864	2872	2875	rBV3	629	598	0.01%	0.004%
66	10.603	2875	2881	2887	rBV2	499	609	0.01%	0.004%
67	10.649	2892	2895	2901	rVB2	465	509	0.01%	0.003%
68	10.684	2901	2906	2910	rBV2	453	492	0.01%	0.003%
69	10.755	2910	2928	2947	rBV	526497	852087	17.41%	5.313%
70	11.266	3084	3087	3090	rBV2	440	327	0.01%	0.002%
71	11.475	3148	3152	3156	rVB3	824	774	0.02%	0.005%
72	11.571	3179	3182	3185	rBV2	376	305	0.01%	0.002%
73	11.587	3185	3187	3193	rVB	531	402	0.01%	0.003%
74	11.639	3198	3203	3207	rBB2	573	515	0.01%	0.003%
75	11.713	3222	3226	3231	rBV2	335	386	0.01%	0.002%
76	11.745	3231	3236	3243	rBV6	1766	2448	0.05%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051190.D
 Acq On : 06 Oct 2022 22:52
 Operator : JC/MD
 Sample : N4893-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.809	3243	3256	3279	rBV	467775	749094	15.31%	4.671%
78	12.192	3361	3375	3399	rBV	503839	832491	17.01%	5.191%
79	12.324	3412	3416	3418	rVB3	492	320	0.01%	0.002%
80	12.340	3418	3421	3425	rVB	944	708	0.01%	0.004%
81	12.365	3425	3429	3432	rBV2	624	445	0.01%	0.003%
82	12.462	3456	3459	3465	rBV2	622	522	0.01%	0.003%
83	12.645	3514	3516	3525	rVB4	608	649	0.01%	0.004%
84	12.767	3551	3554	3558	rVB3	437	381	0.01%	0.002%
85	12.867	3581	3585	3589	rVV2	396	372	0.01%	0.002%
86	12.976	3614	3619	3624	rVB4	482	551	0.01%	0.003%
87	13.298	3716	3719	3724	rVB2	619	362	0.01%	0.002%
88	13.378	3741	3744	3748	rBV2	366	304	0.01%	0.002%
89	13.462	3767	3770	3773	rBV3	435	343	0.01%	0.002%
90	13.510	3782	3785	3789	rBV2	426	390	0.01%	0.002%
91	13.732	3851	3854	3857	rBV3	761	444	0.01%	0.003%
92	13.783	3868	3870	3880	rVB4	480	463	0.01%	0.003%
93	13.848	3885	3890	3900	rVB4	2435	3260	0.07%	0.020%
94	13.986	3927	3933	3936	rVB4	627	742	0.02%	0.005%
95	14.092	3958	3966	3975	rBV5	3627	6258	0.13%	0.039%
96	14.259	4015	4018	4020	rBV	555	335	0.01%	0.002%
97	14.304	4028	4032	4034	rBV3	547	402	0.01%	0.003%
98	14.336	4034	4042	4047	rVV7	2175	3321	0.07%	0.021%
99	14.433	4069	4072	4075	rBV	495	385	0.01%	0.002%
100	15.079	4270	4273	4275	rBV3	468	303	0.01%	0.002%




Sum of corrected areas: 16037605

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051190.D
Acq On : 06 Oct 2022 22:52
Operator : JC/MD
Sample : N4893-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

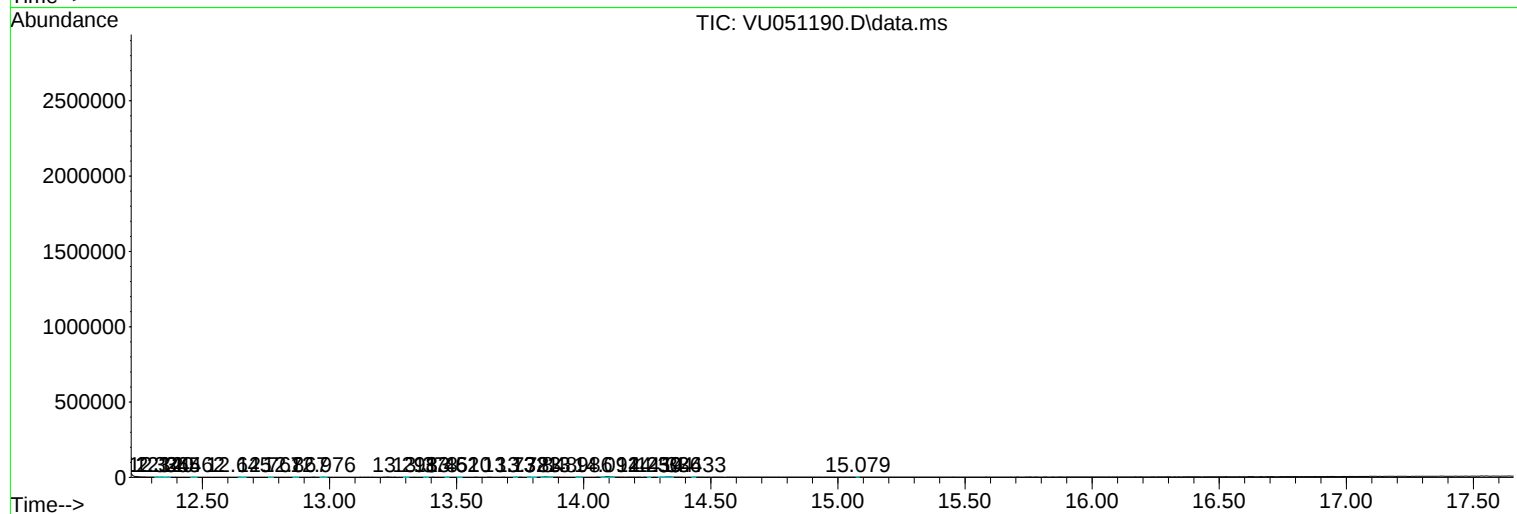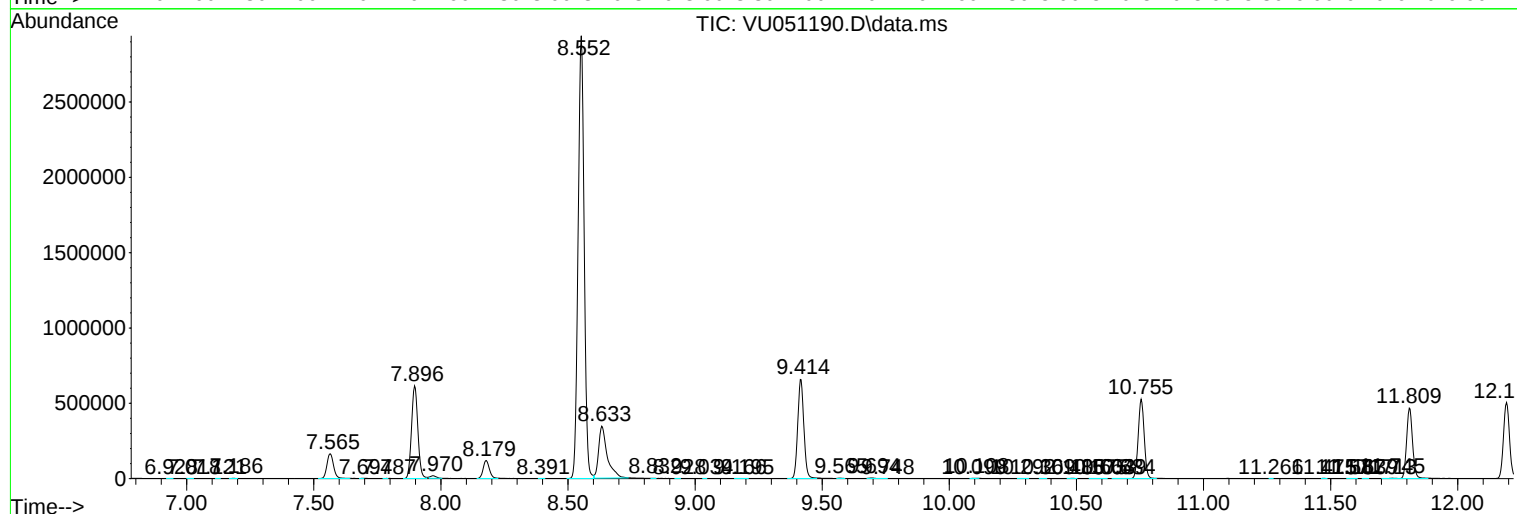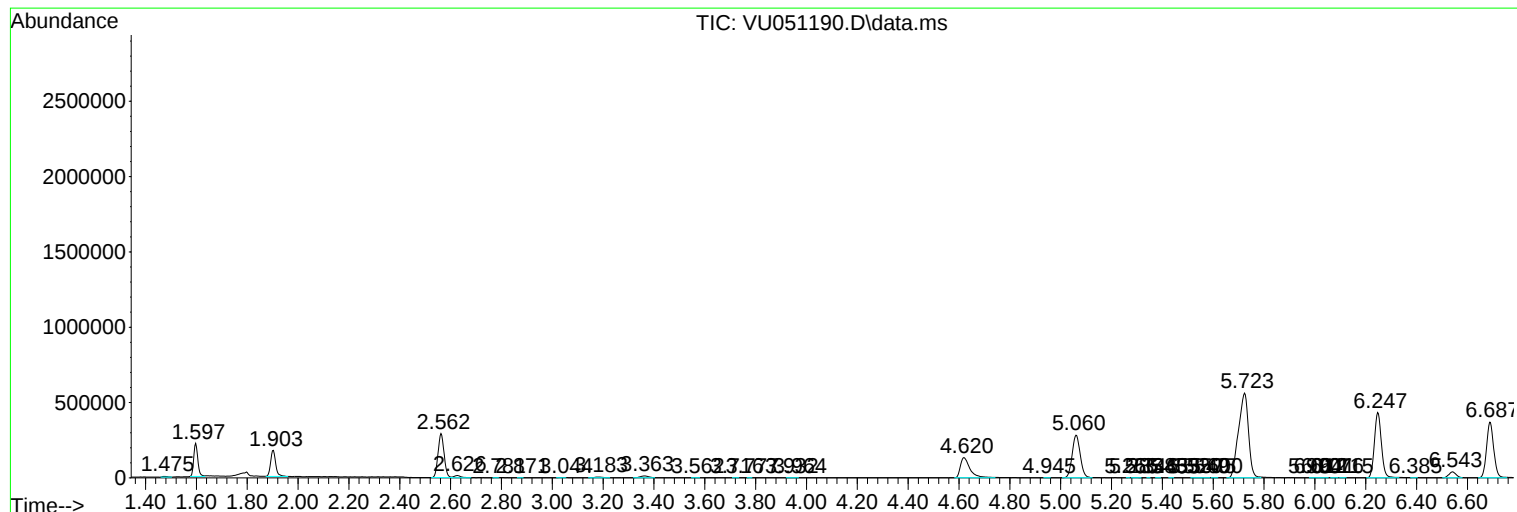

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051190.D
Acq On : 06 Oct 2022 22:52
Operator : JC/MD
Sample : N4893-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051190.D
Acq On : 06 Oct 2022 22:52
Operator : JC/MD
Sample : N4893-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------