

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051191.D
 Acq On : 06 Oct 2022 23:16
 Operator : JC/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	39	44	52	rBV	29467	29732	1.93%	0.262%
2	1.597	73	80	95	rBV	218495	243950	15.80%	2.151%
3	1.899	167	174	191	rVB	176256	234400	15.18%	2.067%
4	2.562	368	380	392	rBV	292615	474975	30.77%	4.189%
5	3.462	657	660	662	rBV2	401	251	0.02%	0.002%
6	3.530	677	681	685	rVB2	403	321	0.02%	0.003%
7	3.559	688	690	692	rBV	257	109	0.01%	0.001%
8	3.575	693	695	697	rBV2	460	273	0.02%	0.002%
9	3.681	725	728	733	rBV2	392	286	0.02%	0.003%
10	3.732	741	744	747	rBV2	319	303	0.02%	0.003%
11	3.813	766	769	772	rBV2	253	198	0.01%	0.002%
12	3.980	819	821	823	rBV	256	156	0.01%	0.001%
13	4.015	829	832	835	rBV2	208	169	0.01%	0.001%
14	4.067	845	848	849	rBV	197	116	0.01%	0.001%
15	4.134	865	869	871	rBV2	196	119	0.01%	0.001%
16	4.176	880	882	887	rVB2	401	261	0.02%	0.002%
17	4.202	887	890	892	rBV	212	129	0.01%	0.001%
18	4.221	892	896	898	rBV	449	282	0.02%	0.002%
19	4.324	923	928	929	rBV	311	257	0.02%	0.002%
20	4.353	934	937	938	rBV	414	243	0.02%	0.002%
21	4.411	952	955	957	rBV	137	78	0.01%	0.001%
22	4.433	960	962	966	rVV	258	119	0.01%	0.001%
23	4.475	970	975	977	rBV2	281	245	0.02%	0.002%
24	4.513	985	987	989	rBV	194	114	0.01%	0.001%
25	4.542	994	996	997	rBV2	157	76	0.00%	0.001%
26	4.620	1008	1020	1043	rBV	138012	348879	22.60%	3.077%
27	4.915	1109	1112	1118	rBV4	483	563	0.04%	0.005%
28	4.986	1130	1134	1136	rBV4	448	403	0.03%	0.004%
29	5.060	1141	1157	1183	rVV	298692	657180	42.57%	5.795%
30	5.378	1249	1256	1259	rBV3	906	914	0.06%	0.008%
31	5.401	1261	1263	1264	rBV3	332	130	0.01%	0.001%
32	5.513	1295	1298	1302	rVB2	194	146	0.01%	0.001%
33	5.536	1302	1305	1309	rBV3	340	241	0.02%	0.002%
34	5.558	1309	1312	1315	rBV3	407	279	0.02%	0.002%
35	5.578	1315	1318	1321	rBV2	225	151	0.01%	0.001%
36	5.722	1340	1363	1392	rBV2	568317	1543655	100.00%	13.613%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051191.D
 Acq On : 06 Oct 2022 23:16
 Operator : JC/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.105	1480	1482	1484	rVB3	319	164	0.01%	0.001%
38	6.121	1484	1487	1490	rVB2	665	433	0.03%	0.004%
39	6.140	1490	1493	1494	rBV	285	141	0.01%	0.001%
40	6.182	1504	1506	1508	rBV2	276	128	0.01%	0.001%
41	6.247	1512	1526	1548	rBV	466001	888448	57.55%	7.835%
42	6.533	1607	1615	1623	rBV8	4743	7890	0.51%	0.070%
43	6.629	1643	1645	1648	rVB	410	158	0.01%	0.001%
44	6.690	1649	1664	1688	rBV	370677	727181	47.11%	6.413%
45	6.870	1717	1720	1723	rVB4	686	428	0.03%	0.004%
46	6.886	1723	1725	1726	rBV	308	133	0.01%	0.001%
47	6.925	1735	1737	1740	rBV	290	159	0.01%	0.001%
48	6.941	1740	1742	1746	rBV2	231	113	0.01%	0.001%
49	6.960	1746	1748	1753	rBV	250	205	0.01%	0.002%
50	6.996	1757	1759	1765	rVB2	352	228	0.01%	0.002%
51	7.041	1769	1773	1776	rBV2	247	156	0.01%	0.001%
52	7.060	1776	1779	1780	rBV	336	183	0.01%	0.002%
53	7.134	1799	1802	1805	rBV2	222	182	0.01%	0.002%
54	7.189	1813	1819	1822	rBV7	1200	1329	0.09%	0.012%
55	7.230	1830	1832	1833	rBV	256	135	0.01%	0.001%
56	7.365	1871	1874	1877	rBV2	282	219	0.01%	0.002%
57	7.488	1908	1912	1916	rBV2	389	260	0.02%	0.002%
58	7.565	1922	1936	1958	rBV	166750	294310	19.07%	2.595%
59	7.796	1996	2008	2018	rBV5	3331	6225	0.40%	0.055%
60	7.838	2018	2021	2023	rBV2	357	209	0.01%	0.002%
61	7.896	2023	2039	2054	rBV	612032	1048304	67.91%	9.245%
62	8.179	2112	2127	2150	rBV	123506	222348	14.40%	1.961%
63	8.343	2175	2178	2180	rBV3	548	255	0.02%	0.002%
64	8.552	2230	2243	2256	rBV2	104393	178749	11.58%	1.576%
65	8.635	2257	2269	2307	rVV3	315833	763615	49.47%	6.734%
66	8.893	2348	2349	2351	rBV2	410	215	0.01%	0.002%
67	8.934	2359	2362	2364	rBV2	604	360	0.02%	0.003%
68	8.947	2364	2366	2370	rVB	354	268	0.02%	0.002%
69	9.005	2383	2384	2385	rBV	333	114	0.01%	0.001%
70	9.037	2390	2394	2396	rBV2	315	288	0.02%	0.003%
71	9.079	2403	2407	2410	rBV3	316	311	0.02%	0.003%
72	9.127	2420	2422	2423	rBV	167	73	0.00%	0.001%
73	9.137	2423	2425	2427	rVV	238	101	0.01%	0.001%
74	9.205	2442	2446	2450	rBV	408	337	0.02%	0.003%
75	9.237	2453	2456	2458	rVV2	239	125	0.01%	0.001%
76	9.324	2481	2483	2485	rBV	198	83	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051191.D
 Acq On : 06 Oct 2022 23:16
 Operator : JC/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	9.343	2485	2489	2491	rBV2	326	260	0.02%	0.002%
78	9.417	2498	2512	2534	rBV	687532	1150219	74.51%	10.143%
79	9.697	2593	2599	2609	rVB7	2957	4231	0.27%	0.037%
80	9.783	2617	2626	2637	rBV5	2235	4299	0.28%	0.038%
81	9.973	2683	2685	2689	rVB	313	134	0.01%	0.001%
82	9.992	2689	2691	2692	rBV	187	83	0.01%	0.001%
83	10.066	2710	2714	2715	rBV	306	189	0.01%	0.002%
84	10.160	2741	2743	2746	rBV2	273	138	0.01%	0.001%
85	10.369	2803	2808	2811	rBV2	478	360	0.02%	0.003%
86	10.401	2814	2818	2822	rBV2	279	223	0.01%	0.002%
87	10.475	2840	2841	2842	rBV	243	88	0.01%	0.001%
88	10.484	2842	2844	2849	rVB3	665	542	0.04%	0.005%
89	10.510	2849	2852	2855	rBV3	475	302	0.02%	0.003%
90	10.754	2914	2928	2950	rBV	532332	856781	55.50%	7.556%
91	11.143	3047	3049	3053	rVB	355	229	0.01%	0.002%
92	11.166	3053	3056	3058	rBV	471	302	0.02%	0.003%
93	11.327	3102	3106	3110	rBV2	295	330	0.02%	0.003%
94	11.574	3180	3183	3184	rBV	485	259	0.02%	0.002%
95	11.809	3244	3256	3280	rBV	480876	776880	50.33%	6.851%
96	12.063	3326	3335	3348	rBV2	18765	33810	2.19%	0.298%
97	12.192	3363	3375	3396	rBV	500148	822226	53.26%	7.251%
98	12.532	3475	3481	3490	rBV5	1935	2626	0.17%	0.023%
99	12.979	3618	3620	3623	rBV2	674	427	0.03%	0.004%
100	13.484	3774	3777	3779	rBV	688	460	0.03%	0.004%




Sum of corrected areas: 11339664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051191.D
Acq On : 06 Oct 2022 23:16
Operator : JC/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

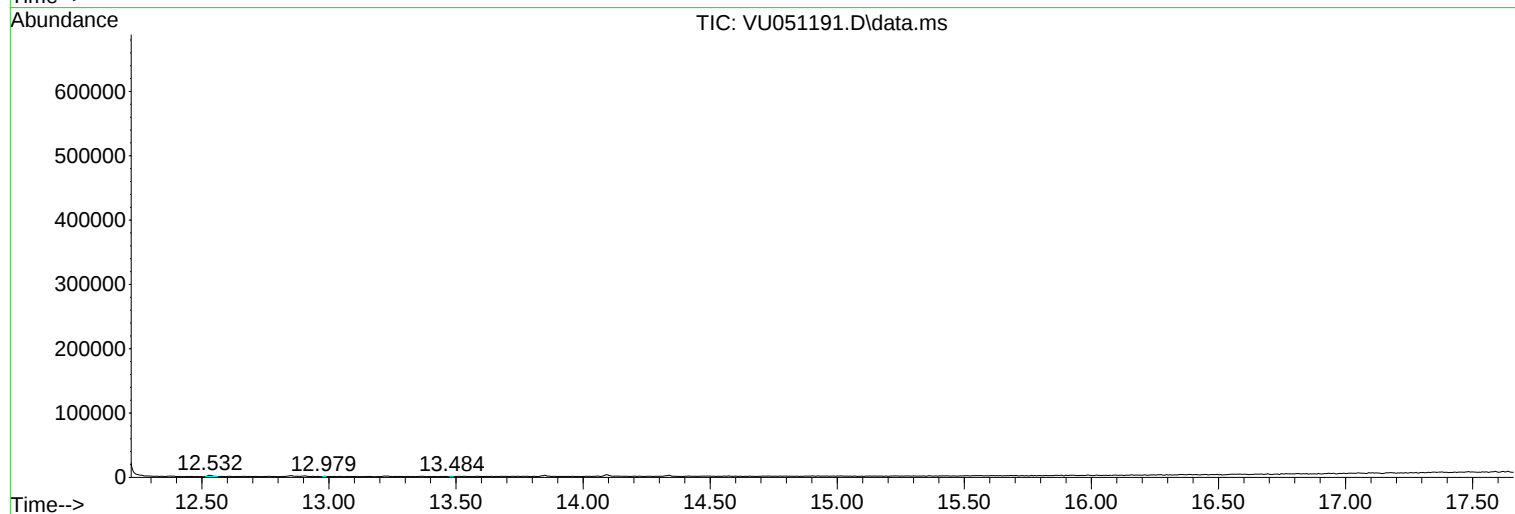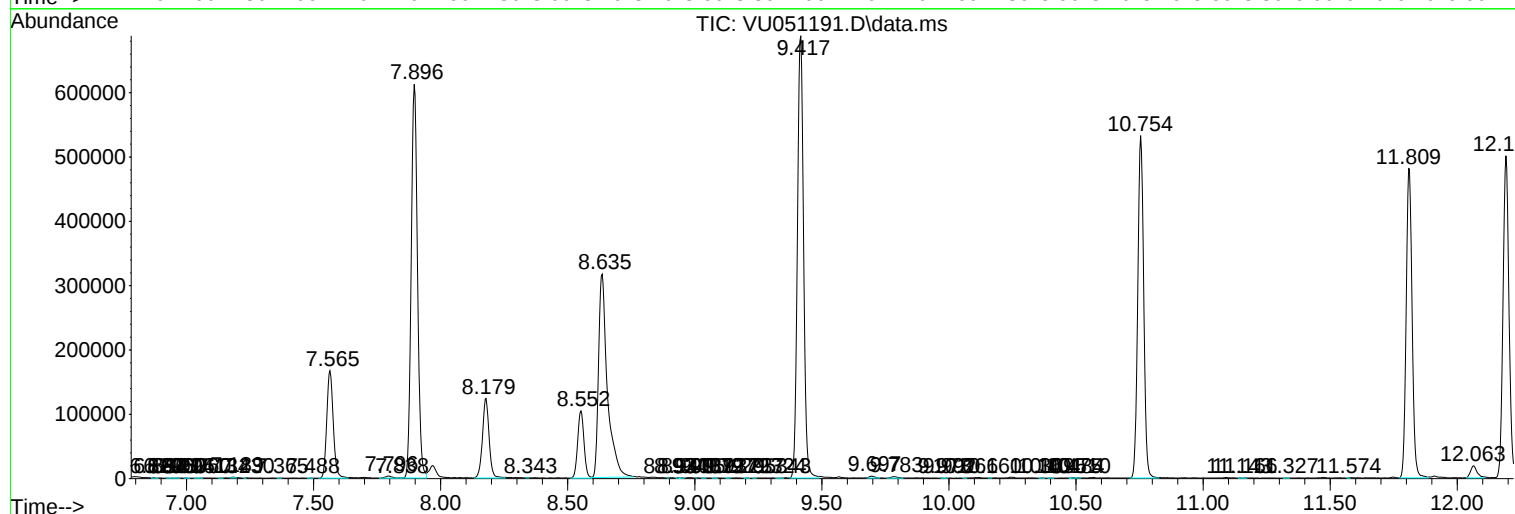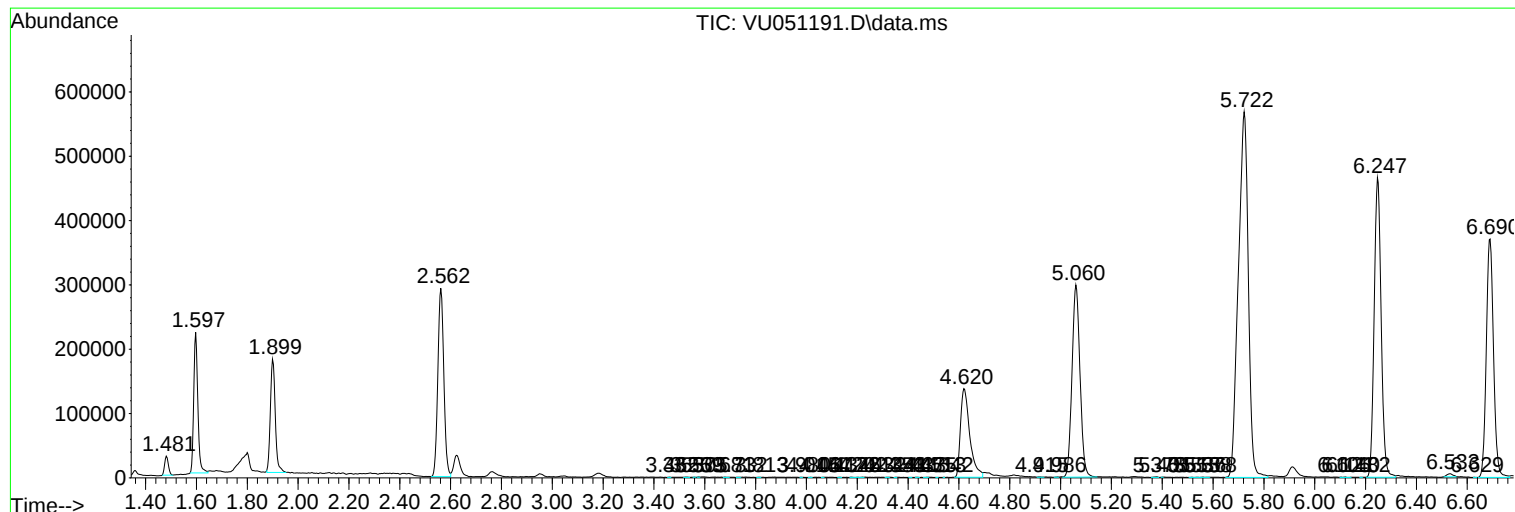

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051191.D
Acq On : 06 Oct 2022 23:16
Operator : JC/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051191.D
Acq On : 06 Oct 2022 23:16
Operator : JC/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc