

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051192.D
 Acq On : 06 Oct 2022 23:40
 Operator : JC/MD
 Sample : N4890-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	223478	245110	15.82%	2.223%
2	1.900	167	174	193	rVB	177964	240719	15.54%	2.183%
3	2.562	369	380	396	rBV	296044	476103	30.74%	4.318%
4	3.044	521	530	537	rVB3	1673	2939	0.19%	0.027%
5	3.356	622	627	630	rBV4	520	512	0.03%	0.005%
6	3.472	656	663	665	rBV	559	523	0.03%	0.005%
7	3.623	706	710	713	rBV	291	221	0.01%	0.002%
8	3.694	728	732	734	rBV	288	236	0.02%	0.002%
9	3.736	742	745	747	rBV	91	72	0.00%	0.001%
10	3.752	747	750	752	rBV2	216	170	0.01%	0.002%
11	3.887	790	792	795	rBV	224	134	0.01%	0.001%
12	3.912	797	800	802	rVV2	273	171	0.01%	0.002%
13	4.012	827	831	834	rBV2	318	316	0.02%	0.003%
14	4.047	841	842	844	rVB	158	58	0.00%	0.001%
15	4.064	844	847	851	rVB	489	311	0.02%	0.003%
16	4.096	853	857	860	rBV	278	237	0.02%	0.002%
17	4.208	889	892	894	rBV2	211	141	0.01%	0.001%
18	4.221	894	896	898	rVV	316	181	0.01%	0.002%
19	4.250	902	905	906	rVV2	311	185	0.01%	0.002%
20	4.260	906	908	911	rVB	389	209	0.01%	0.002%
21	4.298	918	920	922	rBV	145	85	0.01%	0.001%
22	4.318	922	926	929	rVV3	348	304	0.02%	0.003%
23	4.337	930	932	935	rVB	239	92	0.01%	0.001%
24	4.369	935	942	944	rBV	386	332	0.02%	0.003%
25	4.388	945	948	952	rVV2	347	292	0.02%	0.003%
26	4.420	955	958	962	rVB2	235	172	0.01%	0.002%
27	4.443	962	965	968	rBV2	226	148	0.01%	0.001%
28	4.568	1002	1004	1007	rBV	146	75	0.00%	0.001%
29	4.620	1007	1020	1048	rBV	133722	337992	21.82%	3.065%
30	5.060	1141	1157	1180	rBV	287617	627356	40.50%	5.690%
31	5.327	1238	1240	1248	rVB2	433	405	0.03%	0.004%
32	5.366	1251	1252	1254	rBV2	262	98	0.01%	0.001%
33	5.385	1254	1258	1262	rVB3	766	533	0.03%	0.005%
34	5.404	1262	1264	1265	rBV	179	74	0.00%	0.001%
35	5.482	1281	1288	1291	rBV3	608	620	0.04%	0.006%
36	5.507	1291	1296	1300	rBV2	979	1026	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051192.D
 Acq On : 06 Oct 2022 23:40
 Operator : JC/MD
 Sample : N4890-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.594	1317	1323	1332	rVB2	598	882	0.06%	0.008%
38	5.629	1332	1334	1336	rBV	332	180	0.01%	0.002%
39	5.723	1342	1363	1393	rBV2	573411	1548943	100.00%	14.047%
40	6.080	1473	1474	1476	rBV2	232	94	0.01%	0.001%
41	6.115	1481	1485	1486	rBV2	441	355	0.02%	0.003%
42	6.195	1506	1510	1512	rBV3	260	200	0.01%	0.002%
43	6.247	1512	1526	1551	rBV	442437	858984	55.46%	7.790%
44	6.440	1582	1586	1589	rBV3	563	513	0.03%	0.005%
45	6.485	1597	1600	1601	rBV2	348	196	0.01%	0.002%
46	6.539	1605	1617	1631	rVV4	13004	28550	1.84%	0.259%
47	6.687	1649	1663	1685	rBV	374976	729610	47.10%	6.617%
48	6.871	1718	1720	1723	rBV3	282	154	0.01%	0.001%
49	6.887	1723	1725	1730	rVB	752	427	0.03%	0.004%
50	6.999	1755	1760	1761	rBV	321	287	0.02%	0.003%
51	7.047	1770	1775	1777	rBV2	308	266	0.02%	0.002%
52	7.105	1788	1793	1797	rBV3	566	613	0.04%	0.006%
53	7.163	1810	1811	1812	rBV3	342	121	0.01%	0.001%
54	7.237	1830	1834	1838	rBV3	454	431	0.03%	0.004%
55	7.375	1875	1877	1880	rBV2	346	173	0.01%	0.002%
56	7.424	1890	1892	1895	rBV	320	151	0.01%	0.001%
57	7.498	1912	1915	1918	rBV	335	239	0.02%	0.002%
58	7.565	1923	1936	1959	rVV	162481	293789	18.97%	2.664%
59	7.764	1994	1998	2004	rBV3	361	438	0.03%	0.004%
60	7.829	2015	2018	2022	rBV	316	225	0.01%	0.002%
61	7.896	2026	2039	2054	rBV	598636	1043251	67.35%	9.461%
62	8.176	2111	2126	2146	rBV	119040	202849	13.10%	1.840%
63	8.552	2232	2243	2256	rVB2	55989	94965	6.13%	0.861%
64	8.633	2256	2268	2308	rBV3	307182	753290	48.63%	6.832%
65	8.922	2355	2358	2361	rVB3	567	353	0.02%	0.003%
66	8.948	2361	2366	2369	rBV3	677	670	0.04%	0.006%
67	9.028	2389	2391	2393	rVB	256	104	0.01%	0.001%
68	9.044	2393	2396	2402	rBV3	342	414	0.03%	0.004%
69	9.099	2409	2413	2423	rVB	480	536	0.03%	0.005%
70	9.137	2423	2425	2426	rBV	206	73	0.00%	0.001%
71	9.221	2448	2451	2453	rBV2	389	221	0.01%	0.002%
72	9.321	2478	2482	2484	rBV	287	227	0.01%	0.002%
73	9.417	2498	2512	2529	rBV	665821	1103448	71.24%	10.007%
74	9.694	2592	2598	2606	rVB3	2643	3419	0.22%	0.031%
75	9.858	2645	2649	2651	rBV	298	221	0.01%	0.002%
76	9.938	2671	2674	2678	rBV	540	325	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051192.D
 Acq On : 06 Oct 2022 23:40
 Operator : JC/MD
 Sample : N4890-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.205	2753	2757	2759	rBV3	352	281	0.02%	0.003%
78	10.372	2806	2809	2813	rBV	311	191	0.01%	0.002%
79	10.430	2825	2827	2828	rBV	168	87	0.01%	0.001%
80	10.671	2900	2902	2905	rVB2	307	171	0.01%	0.002%
81	10.755	2915	2928	2948	rBV	537318	850020	54.88%	7.709%
82	10.944	2984	2987	2991	rBV2	432	360	0.02%	0.003%
83	11.028	3011	3013	3018	rVB2	314	188	0.01%	0.002%
84	11.050	3018	3020	3021	rBV	280	105	0.01%	0.001%
85	11.140	3045	3048	3055	rBV	339	316	0.02%	0.003%
86	11.375	3113	3121	3123	rBV2	496	625	0.04%	0.006%
87	11.391	3123	3126	3128	rBV2	284	191	0.01%	0.002%
88	11.607	3189	3193	3196	rBV2	442	286	0.02%	0.003%
89	11.626	3196	3199	3203	rVV	322	299	0.02%	0.003%
90	11.722	3227	3229	3231	rBV	397	215	0.01%	0.002%
91	11.809	3243	3256	3275	rBV	468232	747713	48.27%	6.781%
92	12.066	3328	3336	3353	rBV3	6648	12466	0.80%	0.113%
93	12.192	3362	3375	3393	rBV	494877	803606	51.88%	7.288%
94	12.726	3538	3541	3544	rBV	586	491	0.03%	0.004%
95	13.385	3742	3746	3749	rBV	655	570	0.04%	0.005%




Sum of corrected areas: 11026520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051192.D
Acq On : 06 Oct 2022 23:40
Operator : JC/MD
Sample : N4890-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

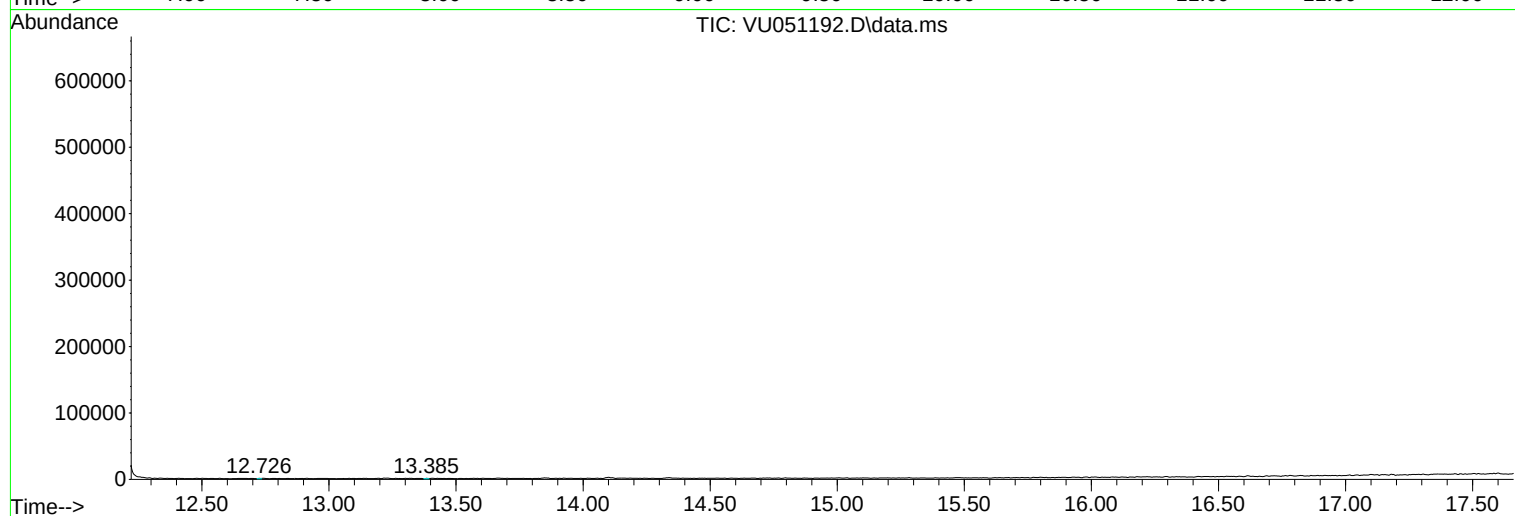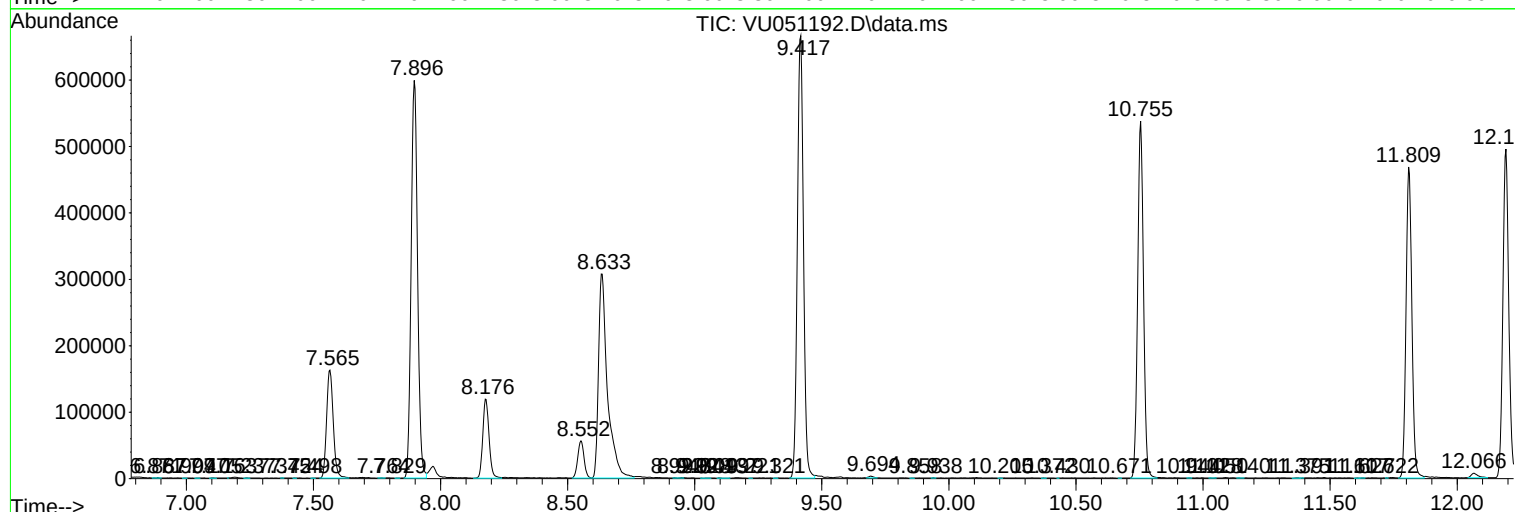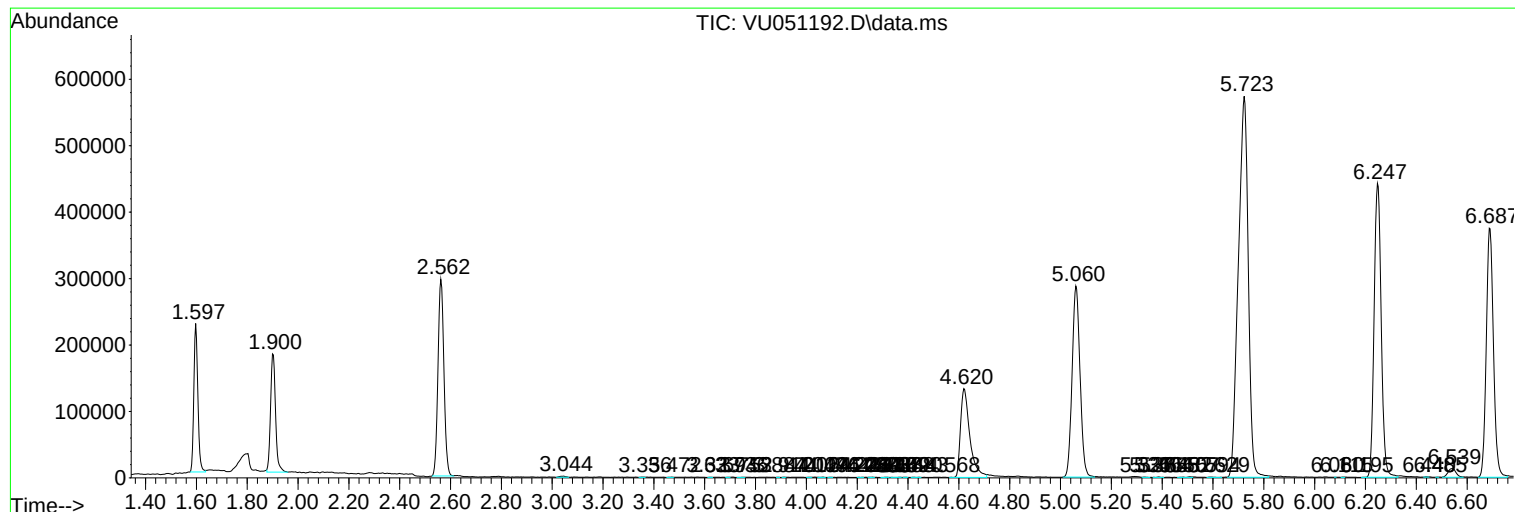

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051192.D
Acq On : 06 Oct 2022 23:40
Operator : JC/MD
Sample : N4890-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051192.D
Acq On : 06 Oct 2022 23:40
Operator : JC/MD
Sample : N4890-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc