

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051193.D
 Acq On : 07 Oct 2022 00:03
 Operator : JC/MD
 Sample : N4890-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	205430	226830	15.51%	2.067%
2	1.899	166	174	194	rVB	163092	224116	15.32%	2.042%
3	2.562	368	380	396	rBV	273865	444739	30.40%	4.052%
4	2.681	414	417	419	rBV3	547	288	0.02%	0.003%
5	2.742	434	436	442	rBV2	516	418	0.03%	0.004%
6	3.034	520	527	528	rBV3	1307	1206	0.08%	0.011%
7	3.112	548	551	555	rVB3	445	387	0.03%	0.004%
8	3.337	618	621	626	rVB2	282	292	0.02%	0.003%
9	3.440	650	653	656	rVV	408	285	0.02%	0.003%
10	3.465	658	661	665	rVB3	416	342	0.02%	0.003%
11	3.674	722	726	731	rBV3	330	418	0.03%	0.004%
12	3.767	749	755	759	rVB3	419	491	0.03%	0.004%
13	3.796	759	764	767	rBV2	520	453	0.03%	0.004%
14	3.858	780	783	787	rVB2	434	365	0.02%	0.003%
15	3.890	787	793	797	rBV3	349	478	0.03%	0.004%
16	3.964	811	816	820	rBV	360	400	0.03%	0.004%
17	4.002	826	828	833	rVB3	490	354	0.02%	0.003%
18	4.034	833	838	843	rBV3	419	486	0.03%	0.004%
19	4.369	940	942	947	rVB	395	360	0.02%	0.003%
20	4.414	953	956	960	rBV2	389	384	0.03%	0.003%
21	4.620	1007	1020	1051	rBV	129651	335488	22.93%	3.057%
22	5.060	1140	1157	1181	rBV	275419	599615	40.99%	5.463%
23	5.240	1211	1213	1216	rVB3	515	300	0.02%	0.003%
24	5.292	1220	1229	1235	rBV4	1100	1938	0.13%	0.018%
25	5.365	1247	1252	1254	rBV2	513	489	0.03%	0.004%
26	5.378	1254	1256	1259	rVV2	649	353	0.02%	0.003%
27	5.517	1296	1299	1304	rVB2	410	309	0.02%	0.003%
28	5.722	1342	1363	1393	rBV2	537600	1462897	100.00%	13.329%
29	5.902	1414	1419	1422	rBV3	658	604	0.04%	0.006%
30	5.986	1442	1445	1449	rBV3	605	385	0.03%	0.004%
31	6.041	1459	1462	1468	rVB3	515	404	0.03%	0.004%
32	6.121	1483	1487	1491	rVB3	523	433	0.03%	0.004%
33	6.246	1511	1526	1545	rBV	429183	820637	56.10%	7.477%
34	6.539	1603	1617	1640	rBV	219215	418773	28.63%	3.816%
35	6.690	1649	1664	1684	rBV	357755	699243	47.80%	6.371%
36	6.841	1708	1711	1718	rVB5	733	653	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051193.D
 Acq On : 07 Oct 2022 00:03
 Operator : JC/MD
 Sample : N4890-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.996	1754	1759	1763	rBV2	394	368	0.03%	0.003%
38	7.063	1775	1780	1784	rBV2	420	380	0.03%	0.003%
39	7.089	1784	1788	1792	rVV3	363	362	0.02%	0.003%
40	7.160	1804	1810	1813	rBV3	280	302	0.02%	0.003%
41	7.185	1813	1818	1821	rBV3	1359	1236	0.08%	0.011%
42	7.234	1829	1833	1835	rBV	446	310	0.02%	0.003%
43	7.468	1903	1906	1909	rBV2	367	304	0.02%	0.003%
44	7.565	1924	1936	1954	rBV2	157538	282113	19.28%	2.570%
45	7.674	1968	1970	1974	rBV4	381	309	0.02%	0.003%
46	7.693	1974	1976	1980	rVV3	403	312	0.02%	0.003%
47	7.767	1997	1999	2004	rVB2	490	322	0.02%	0.003%
48	7.796	2004	2008	2009	rBV2	441	289	0.02%	0.003%
49	7.809	2009	2012	2018	rVB2	479	440	0.03%	0.004%
50	7.841	2018	2022	2025	rVB2	453	302	0.02%	0.003%
51	7.896	2025	2039	2054	rBV	574564	986630	67.44%	8.990%
52	7.970	2057	2062	2072	rVB2	14513	23191	1.59%	0.211%
53	8.179	2115	2127	2142	rBV	111008	189890	12.98%	1.730%
54	8.336	2173	2176	2182	rBV3	412	426	0.03%	0.004%
55	8.471	2214	2218	2220	rVB3	486	287	0.02%	0.003%
56	8.488	2220	2223	2227	rBV2	460	304	0.02%	0.003%
57	8.552	2230	2243	2256	rVB2	38048	64781	4.43%	0.590%
58	8.635	2256	2269	2305	rBV4	296387	731334	49.99%	6.664%
59	8.848	2331	2335	2339	rBV2	828	884	0.06%	0.008%
60	9.037	2390	2394	2398	rVV	458	376	0.03%	0.003%
61	9.172	2431	2436	2438	rBV3	657	612	0.04%	0.006%
62	9.417	2498	2512	2537	rBV	645165	1084385	74.13%	9.880%
63	9.574	2554	2561	2566	rVB5	1272	1689	0.12%	0.015%
64	9.619	2571	2575	2576	rBV2	405	283	0.02%	0.003%
65	9.632	2576	2579	2587	rVB4	714	700	0.05%	0.006%
66	9.697	2588	2599	2605	rBV4	2352	3736	0.26%	0.034%
67	10.102	2721	2725	2728	rVB3	464	398	0.03%	0.004%
68	10.211	2753	2759	2762	rBV2	559	522	0.04%	0.005%
69	10.388	2810	2814	2818	rBV2	367	322	0.02%	0.003%
70	10.484	2839	2844	2846	rBV2	378	343	0.02%	0.003%
71	10.590	2873	2877	2884	rBV3	322	372	0.03%	0.003%
72	10.754	2915	2928	2947	rBV	512340	824973	56.39%	7.517%
73	10.989	2995	3001	3004	rBV2	436	413	0.03%	0.004%
74	11.311	3097	3101	3104	rBV2	478	327	0.02%	0.003%
75	11.468	3145	3150	3158	rVB4	792	1072	0.07%	0.010%
76	11.741	3232	3235	3239	rBV2	740	724	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051193.D
 Acq On : 07 Oct 2022 00:03
 Operator : JC/MD
 Sample : N4890-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.809	3244	3256	3279	rBV	440032	726067	49.63%	6.616%
78	12.066	3328	3336	3347	rBV4	7715	13851	0.95%	0.126%
79	12.140	3356	3359	3362	rVB3	507	348	0.02%	0.003%
80	12.192	3362	3375	3396	rBV	462997	773963	52.91%	7.052%
81	12.391	3434	3437	3440	rBV3	467	407	0.03%	0.004%
82	12.574	3491	3494	3497	rVB2	511	301	0.02%	0.003%
83	12.867	3581	3585	3589	rBV2	311	344	0.02%	0.003%
84	12.886	3589	3591	3596	rVB3	468	341	0.02%	0.003%
85	12.938	3603	3607	3611	rVB3	345	389	0.03%	0.004%
86	13.057	3642	3644	3651	rVB3	799	657	0.04%	0.006%
87	13.092	3651	3655	3657	rBV2	375	311	0.02%	0.003%
88	13.137	3667	3669	3672	rBV2	376	294	0.02%	0.003%
89	13.224	3692	3696	3698	rBV3	637	502	0.03%	0.005%
90	13.365	3737	3740	3742	rBV2	454	293	0.02%	0.003%
91	13.404	3749	3752	3757	rBV2	330	320	0.02%	0.003%
92	13.819	3878	3881	3883	rBV2	677	520	0.04%	0.005%
93	13.992	3929	3935	3937	rBV2	546	576	0.04%	0.005%
94	14.060	3952	3956	3958	rBV2	424	320	0.02%	0.003%
95	14.323	4035	4038	4041	rBV2	1229	949	0.06%	0.009%
96	14.709	4154	4158	4162	rBV3	563	440	0.03%	0.004%
97	15.275	4331	4334	4338	rBV2	710	531	0.04%	0.005%
98	15.294	4338	4340	4344	rVV4	776	507	0.03%	0.005%
99	15.314	4344	4346	4352	rVB5	631	529	0.04%	0.005%
100	15.359	4357	4360	4362	rBV2	482	367	0.03%	0.003%




Sum of corrected areas: 10975063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051193.D
Acq On : 07 Oct 2022 00:03
Operator : JC/MD
Sample : N4890-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

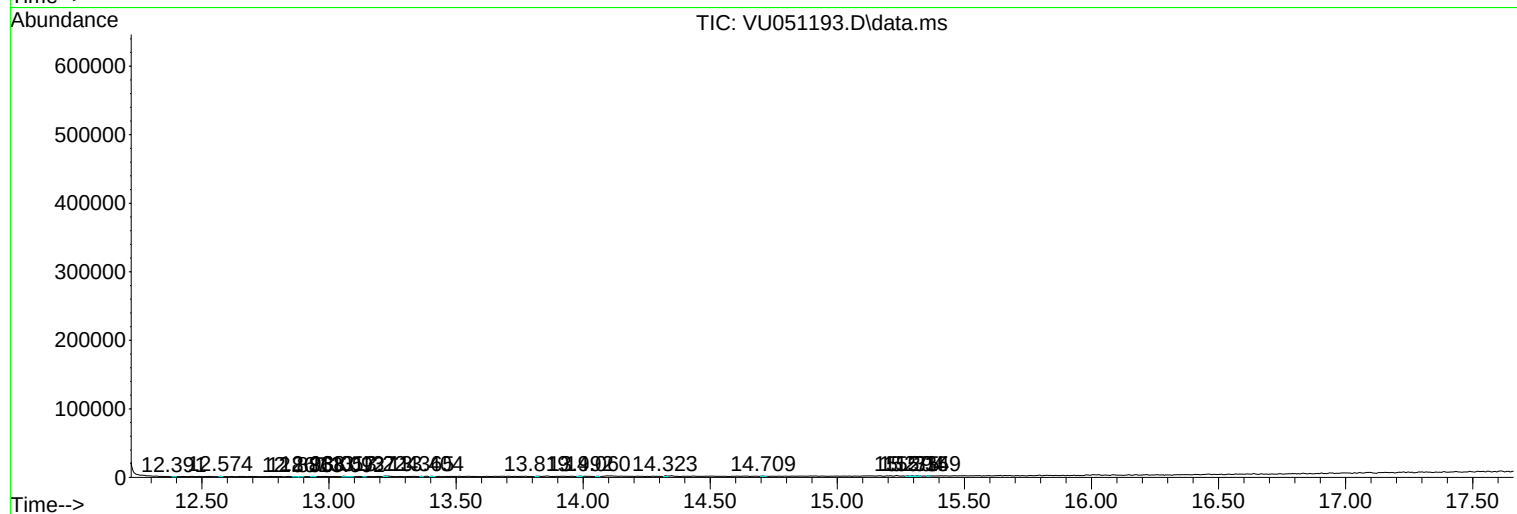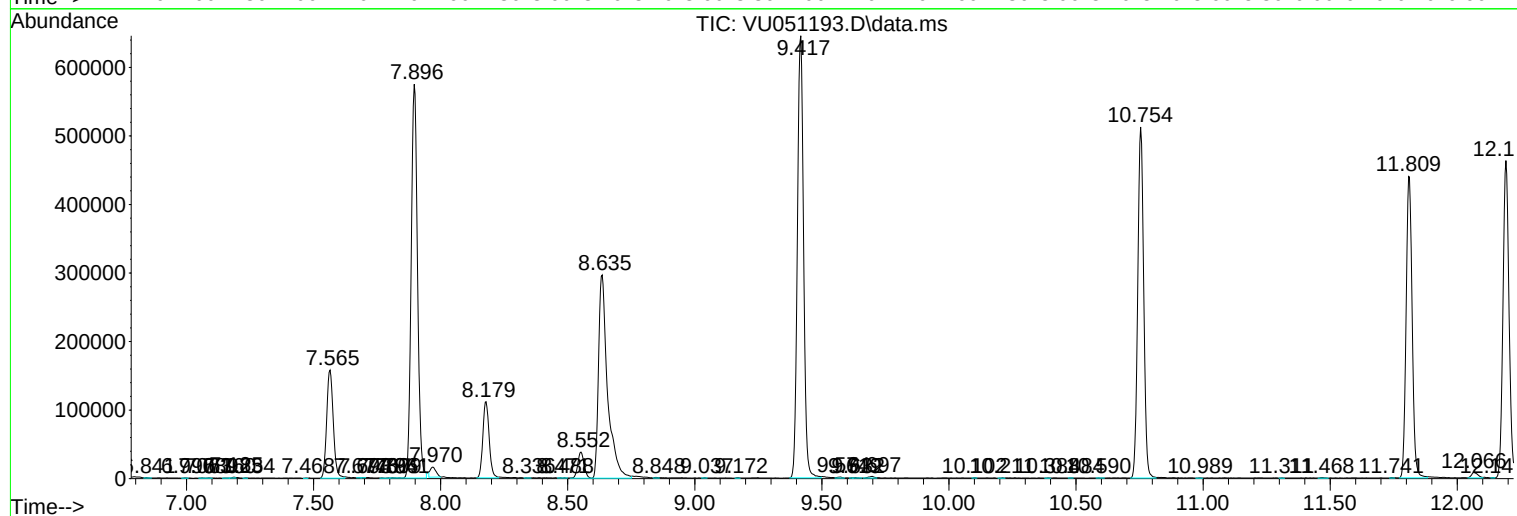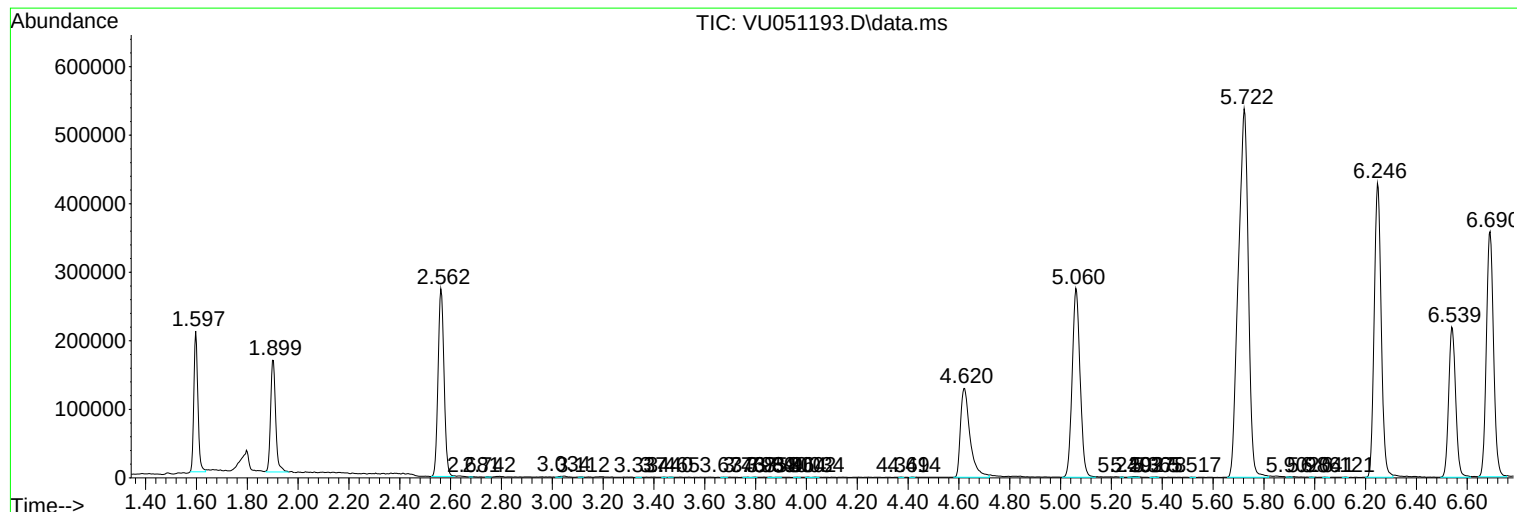

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051193.D
Acq On : 07 Oct 2022 00:03
Operator : JC/MD
Sample : N4890-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051193.D
Acq On : 07 Oct 2022 00:03
Operator : JC/MD
Sample : N4890-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc