

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051194.D
 Acq On : 07 Oct 2022 00:27
 Operator : JC/MD
 Sample : N4890-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	198675	222943	15.46%	2.134%
2	1.899	166	174	194	rVB	164492	222006	15.40%	2.125%
3	2.562	368	380	395	rBV	273340	445266	30.88%	4.262%
4	3.041	515	529	539	rVB3	7026	12095	0.84%	0.116%
5	3.189	564	575	578	rVV2	803	1151	0.08%	0.011%
6	3.292	602	607	614	rVB2	397	561	0.04%	0.005%
7	3.333	614	620	622	rBV2	548	595	0.04%	0.006%
8	3.430	646	650	653	rBV2	515	454	0.03%	0.004%
9	3.517	675	677	685	rVB3	297	329	0.02%	0.003%
10	3.581	692	697	699	rVV3	282	318	0.02%	0.003%
11	3.729	740	743	748	rVB2	372	292	0.02%	0.003%
12	3.758	748	752	754	rBV2	327	263	0.02%	0.003%
13	3.813	764	769	773	rVB2	280	329	0.02%	0.003%
14	3.858	780	783	791	rBV3	523	653	0.05%	0.006%
15	3.967	811	817	824	rBV2	466	719	0.05%	0.007%
16	4.237	893	901	904	rBV	350	375	0.03%	0.004%
17	4.620	1008	1020	1043	rBV	127507	322212	22.35%	3.084%
18	4.951	1120	1123	1125	rBV2	410	287	0.02%	0.003%
19	5.060	1141	1157	1179	rBV	270348	591131	41.00%	5.658%
20	5.205	1199	1202	1207	rBV5	604	451	0.03%	0.004%
21	5.288	1222	1228	1236	rVV5	926	1562	0.11%	0.015%
22	5.321	1236	1238	1240	rVB2	610	264	0.02%	0.003%
23	5.369	1250	1253	1259	rVB2	618	487	0.03%	0.005%
24	5.481	1284	1288	1293	rVB2	336	301	0.02%	0.003%
25	5.510	1293	1297	1301	rBV2	304	253	0.02%	0.002%
26	5.610	1322	1328	1336	rBV2	313	494	0.03%	0.005%
27	5.722	1336	1363	1389	rBV2	529780	1441698	100.00%	13.799%
28	5.964	1433	1438	1442	rBV4	503	518	0.04%	0.005%
29	6.070	1468	1471	1476	rVB3	507	466	0.03%	0.004%
30	6.099	1476	1480	1481	rBV	441	273	0.02%	0.003%
31	6.189	1502	1508	1510	rBV2	385	355	0.02%	0.003%
32	6.247	1512	1526	1548	rBV	431142	824202	57.17%	7.889%
33	6.372	1562	1565	1572	rVB5	854	729	0.05%	0.007%
34	6.501	1598	1605	1606	rBV4	589	559	0.04%	0.005%
35	6.533	1606	1615	1629	rVB8	4450	9603	0.67%	0.092%
36	6.584	1629	1631	1633	rBV2	643	379	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051194.D
 Acq On : 07 Oct 2022 00:27
 Operator : JC/MD
 Sample : N4890-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.690	1648	1664	1682	rBV	351681	682369	47.33%	6.531%
38	6.970	1749	1751	1755	rVV2	364	346	0.02%	0.003%
39	7.115	1790	1796	1802	rBV3	510	597	0.04%	0.006%
40	7.189	1809	1819	1820	rBV3	1012	1360	0.09%	0.013%
41	7.565	1924	1936	1954	rBV2	156101	271459	18.83%	2.598%
42	7.674	1967	1970	1972	rBV2	580	363	0.03%	0.003%
43	7.806	2004	2011	2013	rBV4	385	470	0.03%	0.004%
44	7.896	2025	2039	2054	rBV	568366	967403	67.10%	9.259%
45	8.176	2115	2126	2143	rBV	110330	188114	13.05%	1.800%
46	8.356	2176	2182	2184	rBV2	290	321	0.02%	0.003%
47	8.552	2233	2243	2256	rBV4	33586	58005	4.02%	0.555%
48	8.632	2256	2268	2312	rBV2	296022	718942	49.87%	6.881%
49	8.906	2348	2353	2355	rBV3	447	407	0.03%	0.004%
50	9.005	2381	2384	2387	rBV2	813	682	0.05%	0.007%
51	9.330	2481	2485	2488	rBV3	381	319	0.02%	0.003%
52	9.417	2496	2512	2539	rBV	649691	1094166	75.89%	10.473%
53	9.568	2557	2559	2568	rVB4	1114	1251	0.09%	0.012%
54	9.697	2591	2599	2607	rBV6	2349	3931	0.27%	0.038%
55	9.777	2619	2624	2626	rBV2	484	429	0.03%	0.004%
56	9.899	2657	2662	2667	rBV2	338	365	0.03%	0.003%
57	10.066	2709	2714	2716	rBV2	364	312	0.02%	0.003%
58	10.089	2716	2721	2722	rVV2	300	277	0.02%	0.003%
59	10.098	2722	2724	2726	rVV2	483	280	0.02%	0.003%
60	10.134	2733	2735	2739	rVB2	477	331	0.02%	0.003%
61	10.443	2826	2831	2833	rBV	322	294	0.02%	0.003%
62	10.484	2840	2844	2848	rVB2	520	400	0.03%	0.004%
63	10.648	2893	2895	2898	rBV2	427	270	0.02%	0.003%
64	10.754	2912	2928	2947	rBV	506083	816340	56.62%	7.813%
65	10.883	2965	2968	2970	rBV2	403	270	0.02%	0.003%
66	11.005	3001	3006	3011	rBV2	471	630	0.04%	0.006%
67	11.057	3019	3022	3025	rBV	396	275	0.02%	0.003%
68	11.111	3032	3039	3042	rVB	372	382	0.03%	0.004%
69	11.320	3100	3104	3105	rVV	379	255	0.02%	0.002%
70	11.471	3147	3151	3155	rBV3	741	565	0.04%	0.005%
71	11.533	3165	3170	3172	rBV	333	328	0.02%	0.003%
72	11.584	3182	3186	3189	rBV3	437	394	0.03%	0.004%
73	11.623	3195	3198	3201	rBV	345	309	0.02%	0.003%
74	11.674	3209	3214	3217	rBV2	435	404	0.03%	0.004%
75	11.748	3234	3237	3243	rVB3	940	952	0.07%	0.009%
76	11.809	3243	3256	3278	rBV	457975	735561	51.02%	7.040%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051194.D
 Acq On : 07 Oct 2022 00:27
 Operator : JC/MD
 Sample : N4890-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.934	3291	3295	3301	rBV2	849	754	0.05%	0.007%
78	12.066	3329	3336	3349	rBV5	6077	10942	0.76%	0.105%
79	12.192	3363	3375	3402	rVV	469400	770683	53.46%	7.376%
80	12.639	3512	3514	3519	rVB3	494	336	0.02%	0.003%
81	12.995	3622	3625	3628	rBV3	605	408	0.03%	0.004%
82	13.098	3654	3657	3661	rBV3	618	527	0.04%	0.005%
83	13.314	3720	3724	3730	rBV4	764	893	0.06%	0.009%
84	13.442	3758	3764	3769	rVB3	839	927	0.06%	0.009%
85	13.481	3769	3776	3779	rBV2	634	768	0.05%	0.007%
86	13.539	3791	3794	3798	rBV	372	305	0.02%	0.003%
87	13.754	3857	3861	3864	rBV	635	555	0.04%	0.005%
88	13.793	3869	3873	3876	rBV2	688	641	0.04%	0.006%
89	13.848	3887	3890	3893	rBV3	598	437	0.03%	0.004%
90	13.957	3920	3924	3926	rBV3	518	392	0.03%	0.004%
91	14.028	3940	3946	3949	rBV3	483	594	0.04%	0.006%
92	14.320	4033	4037	4038	rBV	710	458	0.03%	0.004%
93	14.365	4048	4051	4053	rBV	538	367	0.03%	0.004%
94	14.430	4069	4071	4075	rVB3	485	270	0.02%	0.003%
95	14.796	4182	4185	4191	rVB2	616	505	0.04%	0.005%
96	14.921	4222	4224	4227	rBV2	464	248	0.02%	0.002%
97	15.021	4253	4255	4259	rBV2	666	371	0.03%	0.004%
98	15.249	4324	4326	4330	rVB	793	455	0.03%	0.004%
99	15.613	4437	4439	4443	rBV4	1049	617	0.04%	0.006%
100	15.767	4483	4487	4489	rBV4	994	764	0.05%	0.007%




Sum of corrected areas: 10447918

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051194.D
Acq On : 07 Oct 2022 00:27
Operator : JC/MD
Sample : N4890-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

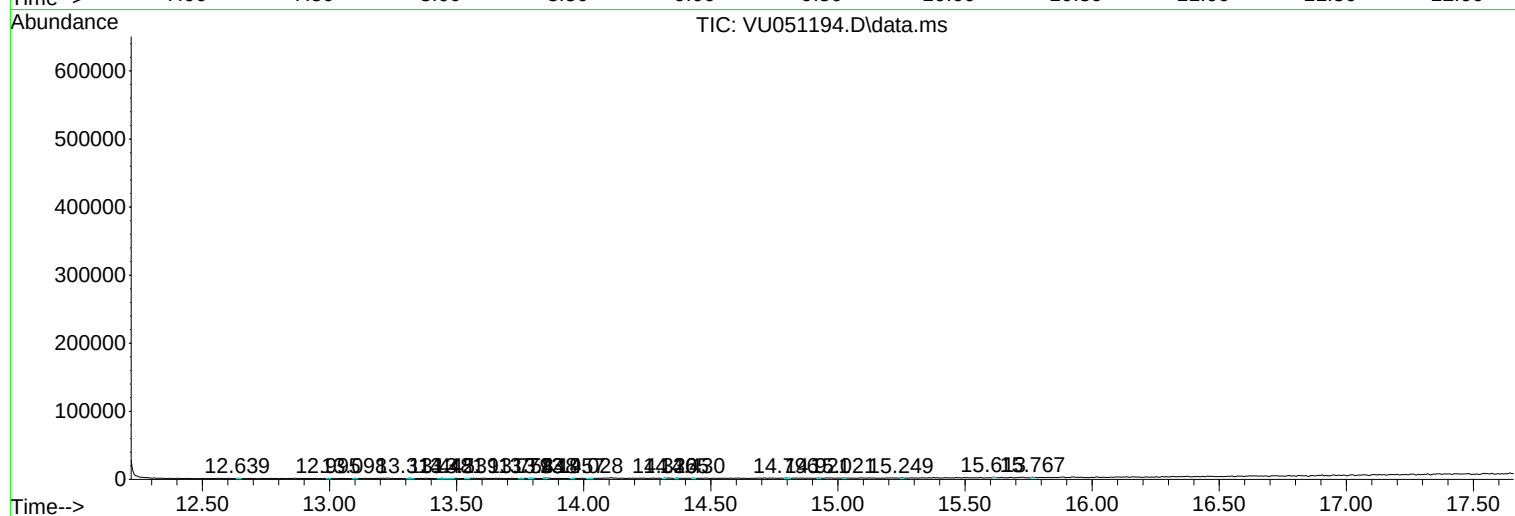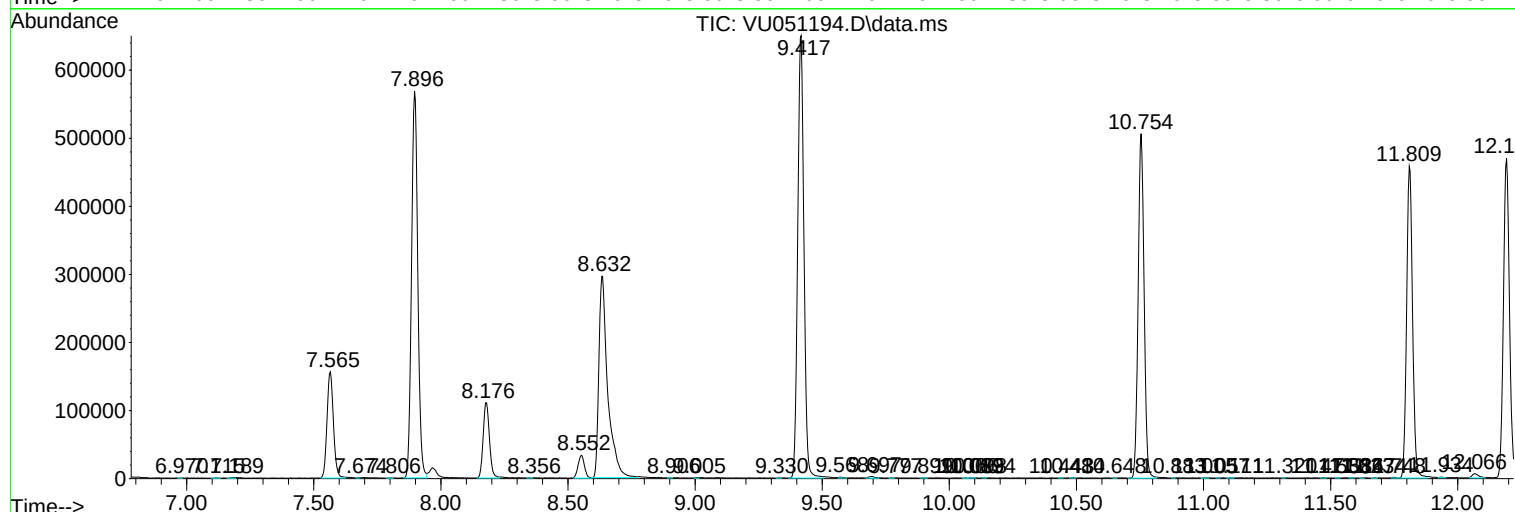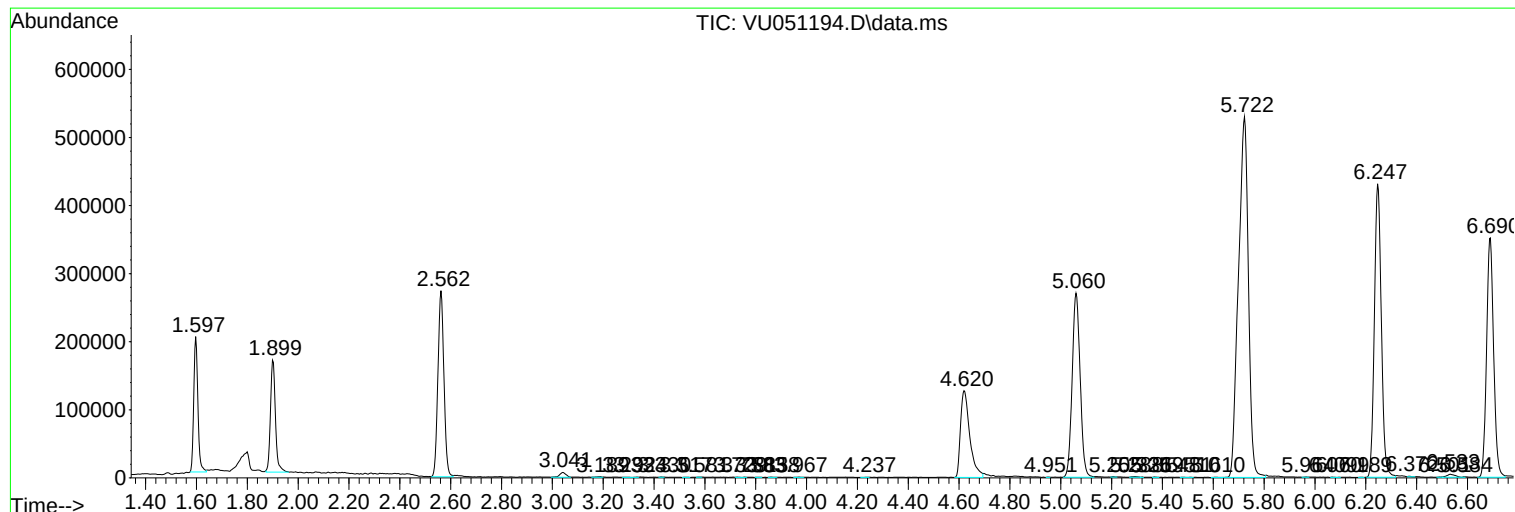

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051194.D
Acq On : 07 Oct 2022 00:27
Operator : JC/MD
Sample : N4890-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051194.D
Acq On : 07 Oct 2022 00:27
Operator : JC/MD
Sample : N4890-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------