

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051196.D
 Acq On : 07 Oct 2022 01:14
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	220307	243968	15.97%	2.199%
2	1.903	166	175	193	rVB	177758	240783	15.77%	2.171%
3	2.562	368	380	392	rBV	301013	485852	31.81%	4.380%
4	2.623	392	399	414	rVB2	29833	50827	3.33%	0.458%
5	2.793	449	452	459	rVB4	1225	1381	0.09%	0.012%
6	2.871	474	476	480	rBV	467	290	0.02%	0.003%
7	3.038	524	528	529	rBV3	997	644	0.04%	0.006%
8	3.179	563	572	587	rBV5	1896	4137	0.27%	0.037%
9	3.240	587	591	595	rVB2	491	417	0.03%	0.004%
10	3.353	620	626	630	rBV2	404	500	0.03%	0.005%
11	3.395	637	639	644	rVB3	392	300	0.02%	0.003%
12	3.430	644	650	654	rBV3	400	430	0.03%	0.004%
13	3.533	679	682	685	rVV2	478	325	0.02%	0.003%
14	3.552	685	688	692	rVB2	480	329	0.02%	0.003%
15	3.575	692	695	698	rBV2	422	295	0.02%	0.003%
16	3.601	698	703	707	rVV2	513	486	0.03%	0.004%
17	3.797	760	764	767	rBV2	353	299	0.02%	0.003%
18	4.227	895	898	901	rBV2	362	280	0.02%	0.003%
19	4.436	956	963	967	rBV4	378	560	0.04%	0.005%
20	4.510	981	986	991	rBV2	332	433	0.03%	0.004%
21	4.620	1008	1020	1060	rBV	127564	344085	22.53%	3.102%
22	5.060	1140	1157	1184	rBV	284452	625235	40.94%	5.636%
23	5.160	1185	1188	1190	rVB3	517	283	0.02%	0.003%
24	5.205	1200	1202	1207	rVB2	422	318	0.02%	0.003%
25	5.292	1220	1229	1230	rBV4	821	1018	0.07%	0.009%
26	5.356	1242	1249	1250	rBV3	353	284	0.02%	0.003%
27	5.385	1256	1258	1261	rVV2	393	284	0.02%	0.003%
28	5.723	1342	1363	1388	rBV2	557985	1527257	100.00%	13.768%
29	5.880	1410	1412	1419	rVB4	904	858	0.06%	0.008%
30	5.912	1419	1422	1435	rVB5	579	856	0.06%	0.008%
31	5.983	1441	1444	1449	rVB2	805	562	0.04%	0.005%
32	6.044	1459	1463	1470	rVB3	735	957	0.06%	0.009%
33	6.247	1507	1526	1557	rBV	470704	895705	58.65%	8.074%
34	6.443	1584	1587	1588	rBV3	551	339	0.02%	0.003%
35	6.533	1605	1615	1627	rBV9	4934	10851	0.71%	0.098%
36	6.610	1636	1639	1643	rBV3	511	370	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051196.D
 Acq On : 07 Oct 2022 01:14
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1684	rBV	364134	720242	47.16%	6.493%
38	6.887	1722	1725	1729	rBV2	584	389	0.03%	0.004%
39	6.912	1729	1733	1735	rBV3	423	358	0.02%	0.003%
40	6.944	1740	1743	1746	rBV	499	285	0.02%	0.003%
41	7.018	1758	1766	1767	rBV2	389	478	0.03%	0.004%
42	7.102	1787	1792	1795	rBV3	344	287	0.02%	0.003%
43	7.128	1795	1800	1803	rBV3	402	491	0.03%	0.004%
44	7.182	1814	1817	1826	rVB5	1179	1693	0.11%	0.015%
45	7.224	1827	1830	1834	rVV3	461	281	0.02%	0.003%
46	7.292	1844	1851	1855	rBV2	366	496	0.03%	0.004%
47	7.340	1863	1866	1871	rBV2	407	384	0.03%	0.003%
48	7.395	1880	1883	1889	rVB2	349	361	0.02%	0.003%
49	7.565	1923	1936	1959	rBV	159961	285328	18.68%	2.572%
50	7.684	1971	1973	1975	rBV2	568	356	0.02%	0.003%
51	7.793	2003	2007	2009	rBV2	669	543	0.04%	0.005%
52	7.842	2016	2022	2025	rBV3	490	417	0.03%	0.004%
53	7.896	2025	2039	2056	rBV	599394	1042605	68.27%	9.399%
54	8.179	2115	2127	2148	rBV	115184	198473	13.00%	1.789%
55	8.401	2193	2196	2198	rBV2	387	315	0.02%	0.003%
56	8.430	2202	2205	2209	rVB2	373	301	0.02%	0.003%
57	8.456	2209	2213	2216	rBV3	373	394	0.03%	0.004%
58	8.552	2234	2243	2254	rVB4	17916	30287	1.98%	0.273%
59	8.636	2254	2269	2306	rBV4	295833	740726	48.50%	6.677%
60	8.877	2341	2344	2348	rVB5	677	445	0.03%	0.004%
61	8.922	2355	2358	2362	rVB3	373	287	0.02%	0.003%
62	9.047	2392	2397	2401	rBV2	322	329	0.02%	0.003%
63	9.076	2401	2406	2411	rVB2	715	636	0.04%	0.006%
64	9.102	2411	2414	2417	rBV3	454	360	0.02%	0.003%
65	9.414	2498	2511	2535	rBV	702887	1165922	76.34%	10.510%
66	9.626	2573	2577	2579	rBV2	777	496	0.03%	0.004%
67	9.658	2584	2587	2590	rVV3	507	331	0.02%	0.003%
68	9.690	2594	2597	2608	rVV4	1530	2362	0.15%	0.021%
69	9.915	2663	2667	2673	rVB2	379	390	0.03%	0.004%
70	9.948	2673	2677	2681	rVB	454	300	0.02%	0.003%
71	10.047	2702	2708	2716	rBV2	526	726	0.05%	0.007%
72	10.185	2747	2751	2755	rBV2	477	353	0.02%	0.003%
73	10.221	2758	2762	2765	rVB3	514	415	0.03%	0.004%
74	10.237	2765	2767	2769	rBV	693	415	0.03%	0.004%
75	10.481	2839	2843	2846	rBV2	410	342	0.02%	0.003%
76	10.591	2873	2877	2880	rBV	466	347	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051196.D
 Acq On : 07 Oct 2022 01:14
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.623	2884	2887	2890	rVV2	599	412	0.03%	0.004%
78	10.755	2915	2928	2951	rBV	513862	830354	54.37%	7.485%
79	11.060	3021	3023	3027	rVB2	456	326	0.02%	0.003%
80	11.166	3051	3056	3059	rBV2	944	934	0.06%	0.008%
81	11.208	3067	3069	3076	rVB2	421	350	0.02%	0.003%
82	11.301	3096	3098	3103	rVB3	420	302	0.02%	0.003%
83	11.562	3175	3179	3181	rBV	371	278	0.02%	0.003%
84	11.809	3243	3256	3276	rBV	482975	781118	51.15%	7.041%
85	12.063	3327	3335	3357	rVV3	13336	25967	1.70%	0.234%
86	12.192	3362	3375	3396	rBV	488953	804531	52.68%	7.252%
87	12.353	3423	3425	3429	rVB3	525	286	0.02%	0.003%
88	12.475	3460	3463	3467	rVB3	499	394	0.03%	0.004%
89	12.642	3512	3515	3521	rBV3	569	452	0.03%	0.004%
90	13.224	3692	3696	3701	rBV4	633	658	0.04%	0.006%
91	13.330	3724	3729	3733	rBV2	408	528	0.03%	0.005%
92	13.452	3763	3767	3771	rBV3	558	553	0.04%	0.005%
93	13.533	3786	3792	3799	rBV4	540	820	0.05%	0.007%
94	13.565	3799	3802	3805	rVV3	364	298	0.02%	0.003%
95	13.841	3885	3888	3891	rBV2	507	367	0.02%	0.003%
96	13.989	3932	3934	3940	rVB2	709	600	0.04%	0.005%
97	14.253	4013	4016	4020	rBV3	568	513	0.03%	0.005%
98	14.793	4181	4184	4186	rBV2	657	338	0.02%	0.003%
99	15.240	4321	4323	4325	rBV2	532	300	0.02%	0.003%
100	15.934	4536	4539	4543	rBV2	1195	780	0.05%	0.007%




Sum of corrected areas: 11093203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051196.D
Acq On : 07 Oct 2022 01:14
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

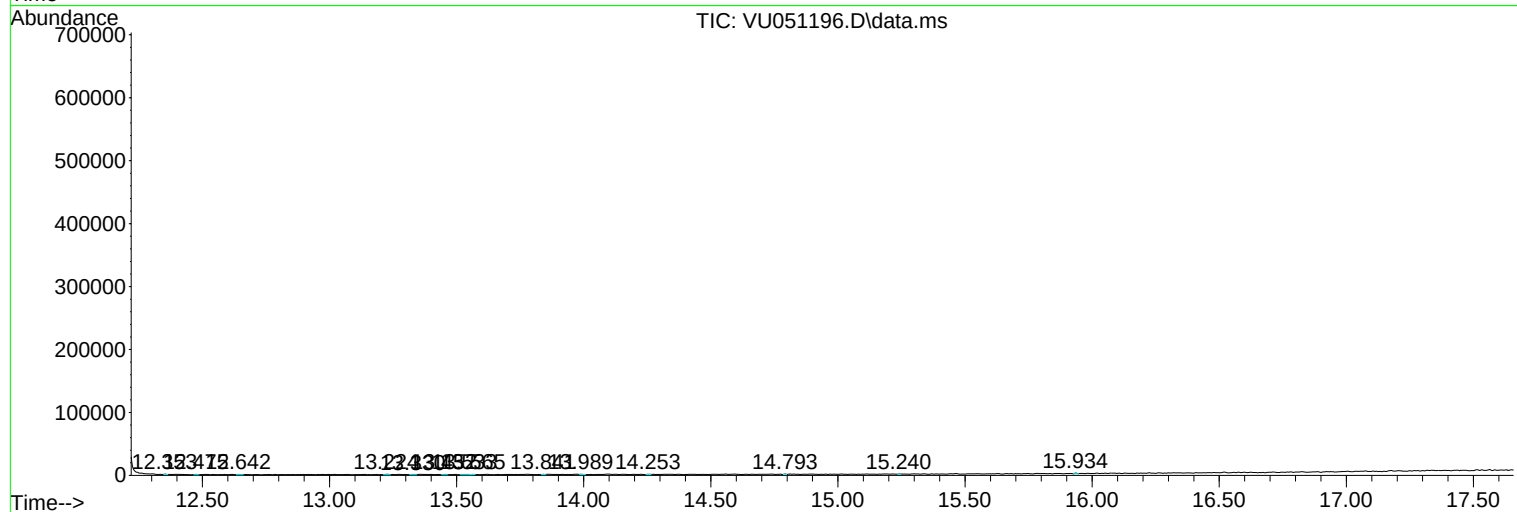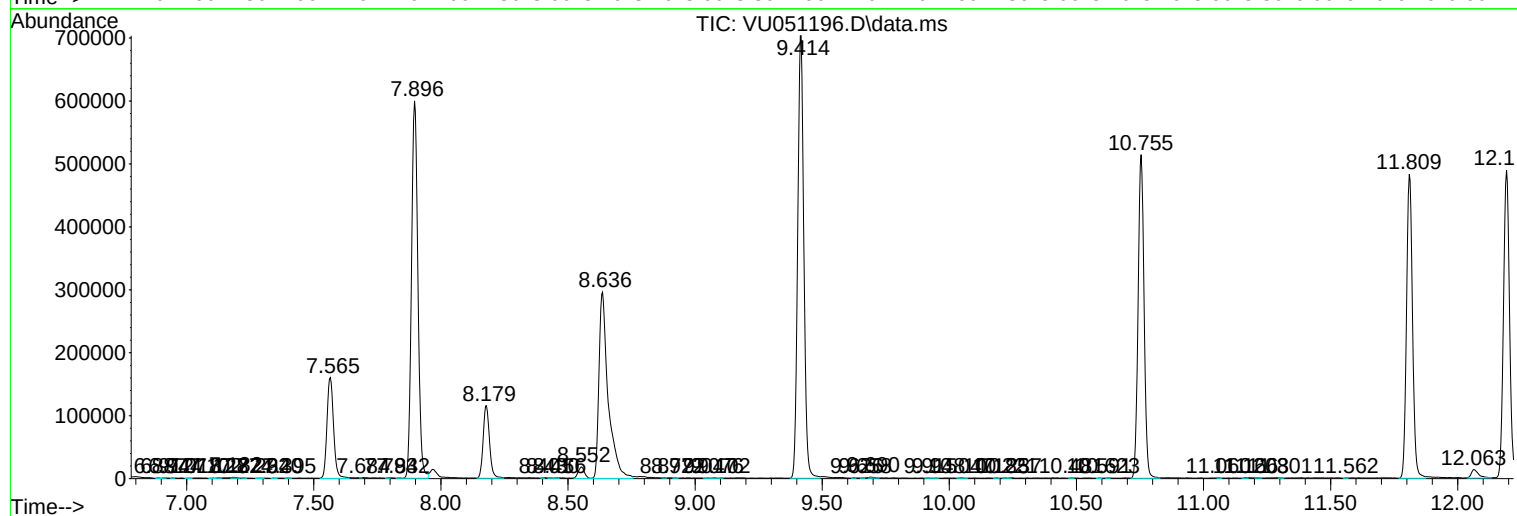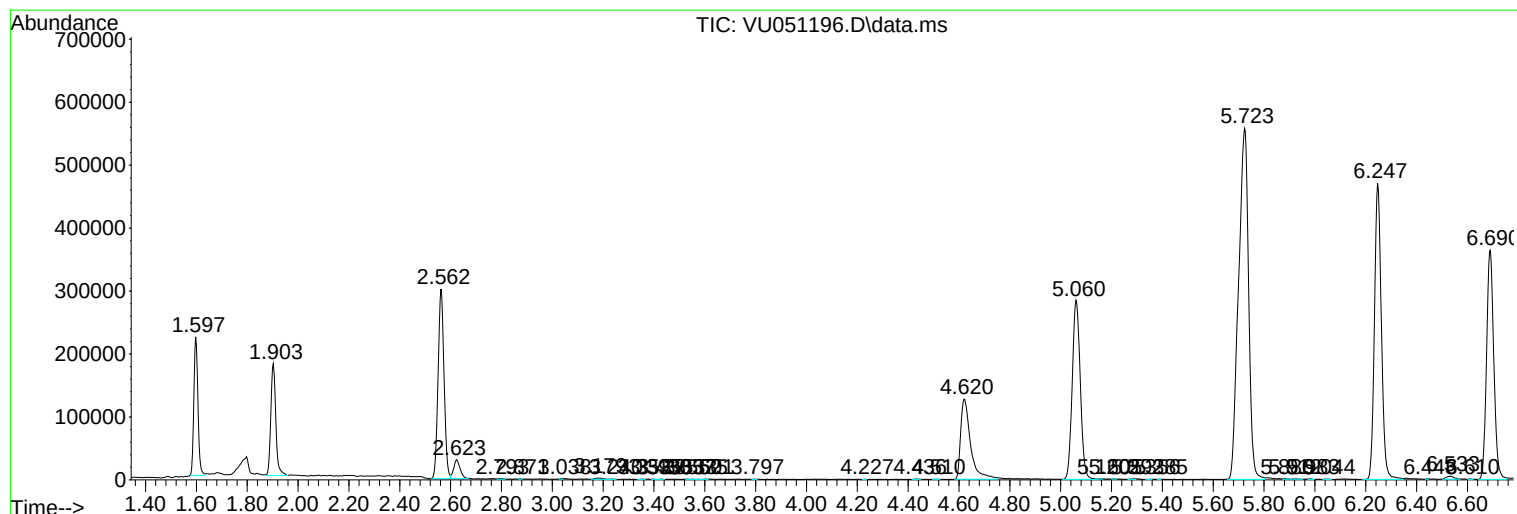

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051196.D
Acq On : 07 Oct 2022 01:14
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051196.D
Acq On : 07 Oct 2022 01:14
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc