

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051197.D
 Acq On : 07 Oct 2022 01:38
 Operator : JC/MD
 Sample : N4890-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	215861	238513	15.97%	2.201%
2	1.903	167	175	191	rVB	175510	233773	15.65%	2.157%
3	2.562	368	380	397	rBV	291639	476096	31.88%	4.394%
4	2.777	444	447	457	rVB6	846	1417	0.09%	0.013%
5	2.961	500	504	508	rVB2	255	247	0.02%	0.002%
6	2.986	508	512	514	rBV3	357	281	0.02%	0.003%
7	3.044	522	530	540	rVB8	1251	2231	0.15%	0.021%
8	3.092	540	545	548	rVB	367	278	0.02%	0.003%
9	3.199	574	578	586	rVB2	928	997	0.07%	0.009%
10	3.253	589	595	597	rBV2	404	385	0.03%	0.004%
11	3.645	711	717	721	rBV3	447	510	0.03%	0.005%
12	3.777	754	758	762	rBV2	312	321	0.02%	0.003%
13	4.112	856	862	865	rBV2	419	350	0.02%	0.003%
14	4.170	876	880	885	rVV3	370	331	0.02%	0.003%
15	4.250	901	905	908	rBV	781	677	0.05%	0.006%
16	4.366	937	941	945	rVB3	449	424	0.03%	0.004%
17	4.465	965	972	974	rBV2	296	280	0.02%	0.003%
18	4.562	998	1002	1005	rBV2	334	287	0.02%	0.003%
19	4.620	1005	1020	1051	rBV	130021	334665	22.41%	3.089%
20	4.954	1121	1124	1127	rBV2	465	278	0.02%	0.003%
21	4.986	1130	1134	1141	rVB4	467	688	0.05%	0.006%
22	5.060	1141	1157	1182	rBV	278589	612968	41.04%	5.657%
23	5.202	1197	1201	1203	rBV	514	386	0.03%	0.004%
24	5.372	1251	1254	1255	rBV2	454	239	0.02%	0.002%
25	5.526	1298	1302	1303	rBV	498	292	0.02%	0.003%
26	5.578	1312	1318	1320	rBV2	568	467	0.03%	0.004%
27	5.620	1329	1331	1336	rVB	364	251	0.02%	0.002%
28	5.723	1341	1363	1389	rBV2	550154	1493489	100.00%	13.783%
29	5.960	1433	1437	1441	rBV3	589	645	0.04%	0.006%
30	6.015	1445	1454	1455	rBV2	585	643	0.04%	0.006%
31	6.044	1461	1463	1467	rVB	412	272	0.02%	0.003%
32	6.067	1467	1470	1478	rVB3	314	360	0.02%	0.003%
33	6.124	1485	1488	1493	rVB3	334	262	0.02%	0.002%
34	6.247	1509	1526	1547	rBV	446253	858119	57.46%	7.919%
35	6.539	1603	1617	1636	rBV4	73497	141982	9.51%	1.310%
36	6.690	1649	1664	1683	rBV	365154	707385	47.36%	6.528%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051197.D
 Acq On : 07 Oct 2022 01:38
 Operator : JC/MD
 Sample : N4890-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.845	1709	1712	1717	rVV5	398	320	0.02%	0.003%
38	6.915	1728	1734	1736	rBV2	418	374	0.03%	0.003%
39	7.176	1813	1815	1817	rBV3	664	410	0.03%	0.004%
40	7.266	1837	1843	1849	rVB	548	639	0.04%	0.006%
41	7.565	1924	1936	1957	rBV2	156827	275834	18.47%	2.546%
42	7.697	1973	1977	1982	rVV6	878	983	0.07%	0.009%
43	7.732	1986	1988	1993	rVB2	586	405	0.03%	0.004%
44	7.896	2023	2039	2054	rBV	590578	1012512	67.80%	9.344%
45	8.092	2098	2100	2106	rVB2	632	431	0.03%	0.004%
46	8.131	2107	2112	2113	rBV2	345	244	0.02%	0.002%
47	8.179	2113	2127	2144	rBV	111598	191047	12.79%	1.763%
48	8.308	2163	2167	2171	rBV4	521	527	0.04%	0.005%
49	8.372	2184	2187	2191	rBV2	446	406	0.03%	0.004%
50	8.433	2203	2206	2210	rVB2	424	375	0.03%	0.003%
51	8.462	2210	2215	2218	rBV2	715	735	0.05%	0.007%
52	8.491	2222	2224	2228	rVB	396	267	0.02%	0.002%
53	8.552	2233	2243	2254	rVB4	14329	23908	1.60%	0.221%
54	8.632	2256	2268	2304	rBV3	292557	725668	48.59%	6.697%
55	9.086	2406	2409	2414	rVB2	379	271	0.02%	0.003%
56	9.417	2497	2512	2532	rBV	667100	1108763	74.24%	10.233%
57	9.645	2579	2583	2585	rBV2	634	399	0.03%	0.004%
58	9.697	2591	2599	2606	rBV3	2124	3052	0.20%	0.028%
59	9.771	2618	2622	2627	rBV	435	464	0.03%	0.004%
60	10.166	2742	2745	2748	rBV2	531	375	0.03%	0.003%
61	10.414	2818	2822	2825	rVB2	590	443	0.03%	0.004%
62	10.755	2915	2928	2950	rBV	511869	825565	55.28%	7.619%
63	10.906	2973	2975	2978	rVB2	499	271	0.02%	0.003%
64	11.066	3021	3025	3026	rBV2	399	287	0.02%	0.003%
65	11.076	3026	3028	3034	rVV2	544	479	0.03%	0.004%
66	11.127	3042	3044	3049	rVB	384	252	0.02%	0.002%
67	11.195	3061	3065	3070	rBV2	533	493	0.03%	0.005%
68	11.272	3086	3089	3092	rVB2	426	285	0.02%	0.003%
69	11.362	3113	3117	3124	rBV3	350	412	0.03%	0.004%
70	11.468	3147	3150	3155	rVV4	655	494	0.03%	0.005%
71	11.738	3229	3234	3237	rBV3	540	495	0.03%	0.005%
72	11.809	3243	3256	3276	rBV	462252	745150	49.89%	6.877%
73	11.938	3294	3296	3298	rVB3	605	238	0.02%	0.002%
74	12.063	3330	3335	3337	rBV3	3242	2866	0.19%	0.026%
75	12.192	3361	3375	3401	rBV	474058	785079	52.57%	7.245%
76	12.468	3457	3461	3465	rBV2	793	539	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051197.D
 Acq On : 07 Oct 2022 01:38
 Operator : JC/MD
 Sample : N4890-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.587	3494	3498	3503	rBV3	540	672	0.04%	0.006%
78	12.851	3578	3580	3585	rVB2	485	345	0.02%	0.003%
79	12.909	3593	3598	3601	rVB2	498	466	0.03%	0.004%
80	12.944	3601	3609	3610	rBV3	588	770	0.05%	0.007%
81	13.015	3627	3631	3633	rBV2	460	331	0.02%	0.003%
82	13.047	3639	3641	3645	rVB3	421	246	0.02%	0.002%
83	13.230	3695	3698	3705	rVB3	797	716	0.05%	0.007%
84	13.388	3740	3747	3750	rBV3	670	703	0.05%	0.006%
85	13.446	3759	3765	3767	rBV3	399	459	0.03%	0.004%
86	13.610	3814	3816	3818	rBV2	619	366	0.02%	0.003%
87	13.957	3919	3924	3928	rVB2	659	679	0.05%	0.006%
88	13.983	3928	3932	3935	rBV	630	577	0.04%	0.005%
89	14.037	3947	3949	3953	rBV	440	330	0.02%	0.003%
90	14.057	3953	3955	3960	rVB2	522	345	0.02%	0.003%
91	14.227	4006	4008	4013	rBV3	393	384	0.03%	0.004%
92	14.340	4036	4043	4048	rBV2	777	1081	0.07%	0.010%
93	14.783	4179	4181	4185	rVB2	686	430	0.03%	0.004%
94	14.838	4195	4198	4202	rBV2	683	494	0.03%	0.005%
95	15.076	4269	4272	4276	rVB3	790	502	0.03%	0.005%
96	15.217	4313	4316	4323	rBV4	854	992	0.07%	0.009%
97	15.417	4375	4378	4381	rVB3	768	559	0.04%	0.005%
98	15.471	4392	4395	4398	rBV3	1043	779	0.05%	0.007%
99	15.590	4429	4432	4433	rBV	759	441	0.03%	0.004%
100	15.751	4480	4482	4484	rBV2	741	337	0.02%	0.003%




Sum of corrected areas: 10835550

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051197.D
Acq On : 07 Oct 2022 01:38
Operator : JC/MD
Sample : N4890-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

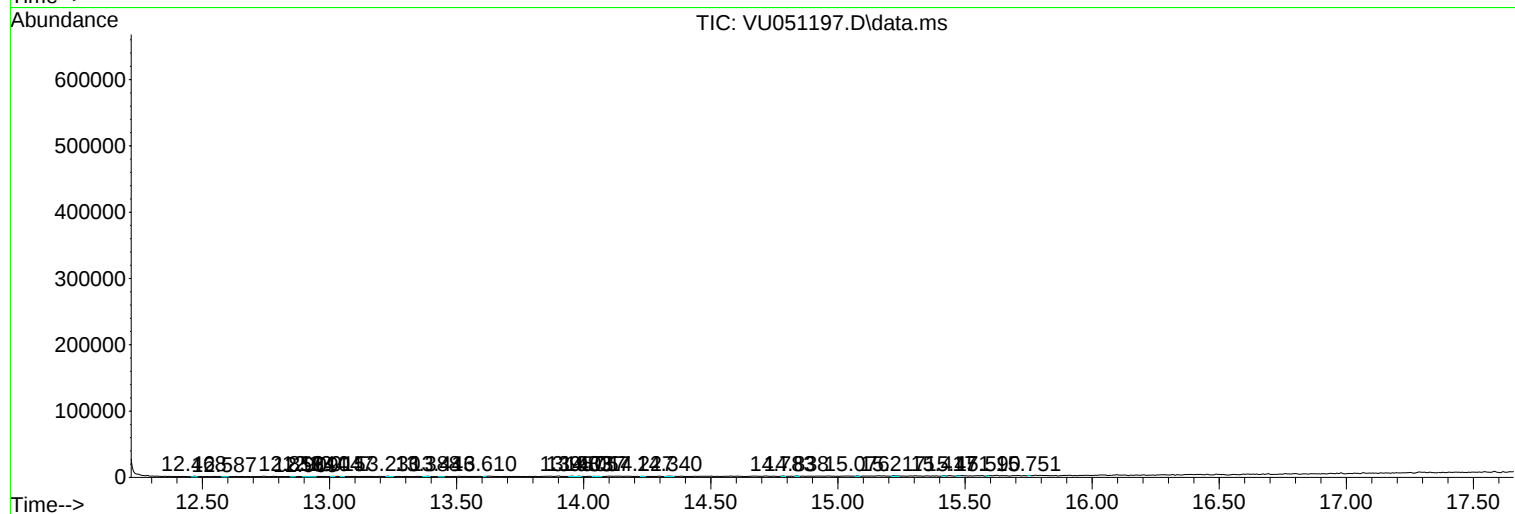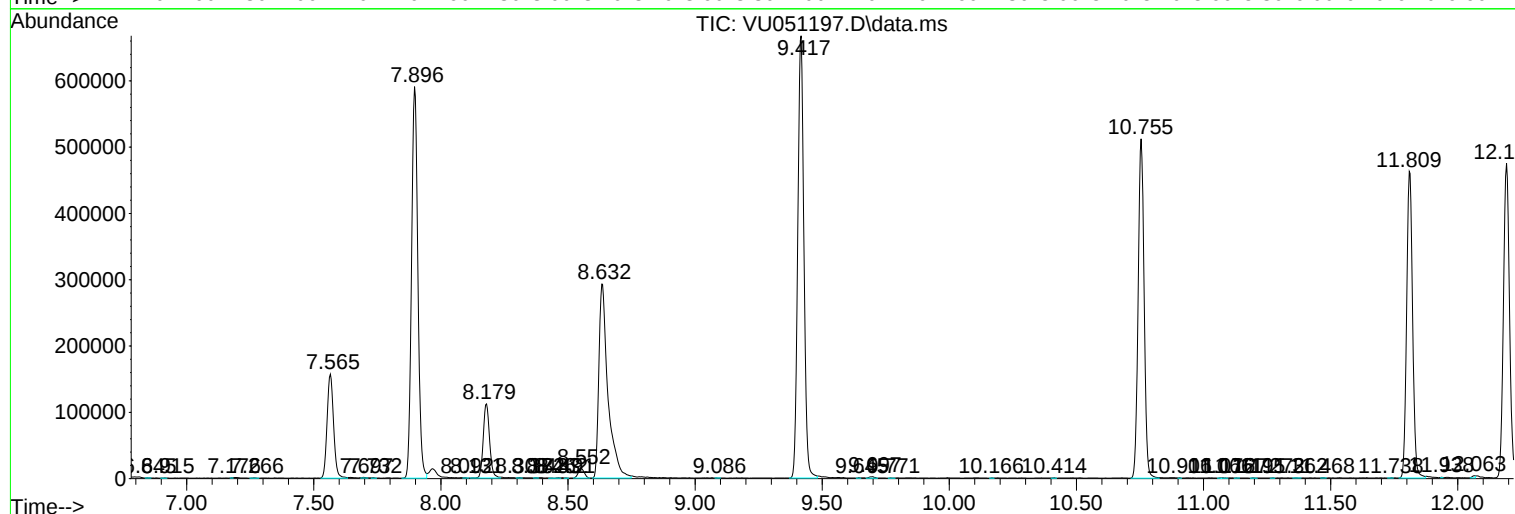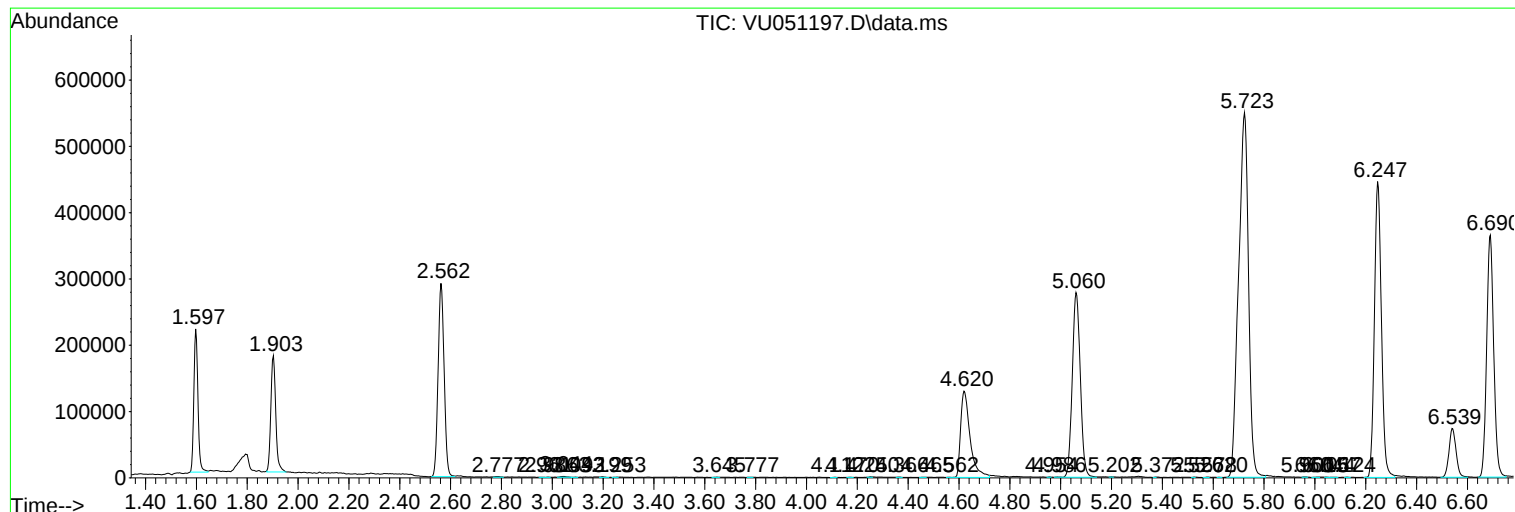

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051197.D
Acq On : 07 Oct 2022 01:38
Operator : JC/MD
Sample : N4890-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051197.D
Acq On : 07 Oct 2022 01:38
Operator : JC/MD
Sample : N4890-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc