

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051198.D
 Acq On : 07 Oct 2022 02:02
 Operator : JC/MD
 Sample : N4890-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	221275	241627	16.12%	2.276%
2	1.899	167	174	197	rVB	173050	238596	15.92%	2.247%
3	2.562	368	380	392	rBV	288094	467821	31.21%	4.407%
4	3.038	521	528	537	rBV6	1712	2937	0.20%	0.028%
5	3.137	555	559	564	rBV3	578	635	0.04%	0.006%
6	3.182	564	573	586	rVB7	1795	4182	0.28%	0.039%
7	3.568	691	693	696	rBV2	262	146	0.01%	0.001%
8	3.620	705	709	712	rBV	358	275	0.02%	0.003%
9	3.649	712	718	721	rBV2	406	502	0.03%	0.005%
10	4.096	855	857	859	rBV	239	130	0.01%	0.001%
11	4.205	888	891	897	rBV	382	422	0.03%	0.004%
12	4.231	897	899	901	rVB	276	103	0.01%	0.001%
13	4.472	972	974	976	rBV	168	55	0.00%	0.001%
14	4.523	987	990	993	rBV	357	244	0.02%	0.002%
15	4.620	1006	1020	1049	rBV	129377	337937	22.54%	3.183%
16	5.060	1142	1157	1178	rBV	279089	610828	40.75%	5.754%
17	5.372	1251	1254	1262	rVB3	625	680	0.05%	0.006%
18	5.407	1263	1265	1267	rBV2	191	93	0.01%	0.001%
19	5.507	1292	1296	1298	rVB	311	223	0.01%	0.002%
20	5.523	1298	1301	1302	rBV	170	112	0.01%	0.001%
21	5.549	1307	1309	1311	rBV	110	64	0.00%	0.001%
22	5.562	1311	1313	1314	rBV	235	100	0.01%	0.001%
23	5.597	1322	1324	1328	rBV2	165	139	0.01%	0.001%
24	5.722	1341	1363	1387	rBV2	551854	1499021	100.00%	14.120%
25	5.986	1443	1445	1448	rBV3	600	345	0.02%	0.003%
26	6.247	1511	1526	1551	rBV	436017	840454	56.07%	7.917%
27	6.530	1605	1614	1615	rBV2	4280	5038	0.34%	0.047%
28	6.629	1643	1645	1647	rBV2	323	105	0.01%	0.001%
29	6.690	1649	1664	1685	rBV	362711	710430	47.39%	6.692%
30	6.864	1714	1718	1722	rVB3	771	595	0.04%	0.006%
31	7.018	1764	1766	1769	rVB3	276	141	0.01%	0.001%
32	7.038	1769	1772	1775	rBV2	222	145	0.01%	0.001%
33	7.124	1793	1799	1800	rBV2	795	667	0.04%	0.006%
34	7.266	1838	1843	1846	rBV2	473	421	0.03%	0.004%
35	7.314	1856	1858	1860	rVB2	202	94	0.01%	0.001%
36	7.330	1861	1863	1866	rVB2	229	109	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051198.D
 Acq On : 07 Oct 2022 02:02
 Operator : JC/MD
 Sample : N4890-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.382	1876	1879	1884	rBV2	315	311	0.02%	0.003%
38	7.407	1885	1887	1889	rVV	236	63	0.00%	0.001%
39	7.565	1922	1936	1958	rBV	156944	277296	18.50%	2.612%
40	7.745	1991	1992	1993	rVB	576	111	0.01%	0.001%
41	7.764	1993	1998	2001	rBV3	527	573	0.04%	0.005%
42	7.796	2005	2008	2012	rVV	516	392	0.03%	0.004%
43	7.896	2026	2039	2054	rBV	584140	1009774	67.36%	9.512%
44	8.179	2115	2127	2148	rBV	112497	192479	12.84%	1.813%
45	8.388	2189	2192	2195	rBV3	380	305	0.02%	0.003%
46	8.552	2233	2243	2254	rBV4	13317	21540	1.44%	0.203%
47	8.636	2257	2269	2309	rBV4	288512	728844	48.62%	6.865%
48	8.925	2356	2359	2365	rBV2	784	834	0.06%	0.008%
49	8.954	2365	2368	2372	rVV4	427	381	0.03%	0.004%
50	9.002	2381	2383	2388	rVB2	262	187	0.01%	0.002%
51	9.028	2389	2391	2394	rVV2	418	187	0.01%	0.002%
52	9.041	2394	2395	2399	rVB	241	152	0.01%	0.001%
53	9.063	2399	2402	2405	rBV2	370	196	0.01%	0.002%
54	9.153	2428	2430	2433	rBV2	409	197	0.01%	0.002%
55	9.320	2479	2482	2484	rBV2	194	164	0.01%	0.002%
56	9.417	2499	2512	2531	rBV	657241	1087105	72.52%	10.240%
57	9.613	2570	2573	2577	rVB2	530	343	0.02%	0.003%
58	9.697	2590	2599	2606	rBV5	1595	2243	0.15%	0.021%
59	9.793	2627	2629	2631	rBV2	277	174	0.01%	0.002%
60	9.893	2658	2660	2663	rBV	184	107	0.01%	0.001%
61	10.008	2692	2696	2701	rBV3	407	461	0.03%	0.004%
62	10.102	2722	2725	2728	rBV3	396	321	0.02%	0.003%
63	10.127	2731	2733	2737	rBV	370	270	0.02%	0.003%
64	10.176	2746	2748	2750	rBV	193	107	0.01%	0.001%
65	10.250	2769	2771	2774	rVB	319	154	0.01%	0.001%
66	10.362	2803	2806	2808	rBV	368	256	0.02%	0.002%
67	10.398	2815	2817	2818	rBV	176	59	0.00%	0.001%
68	10.754	2915	2928	2949	rBV	509923	824066	54.97%	7.762%
69	10.870	2962	2964	2967	rBV	383	246	0.02%	0.002%
70	11.359	3113	3116	3118	rBV2	314	181	0.01%	0.002%
71	11.407	3128	3131	3133	rBV2	309	188	0.01%	0.002%
72	11.471	3144	3151	3156	rVB3	735	824	0.05%	0.008%
73	11.504	3156	3161	3164	rBV2	320	385	0.03%	0.004%
74	11.552	3174	3176	3180	rVB	385	190	0.01%	0.002%
75	11.571	3180	3182	3185	rVB	311	140	0.01%	0.001%
76	11.587	3185	3187	3188	rBV	286	141	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051198.D
Acq On : 07 Oct 2022 02:02
Operator : JC/MD
Sample : N4890-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

77	11.809	3244	3256	3272	rBV	439863	711734	47.48%	6.704%
78	12.024	3319	3323	3327	rBV3	538	675	0.05%	0.006%
79	12.066	3328	3336	3346	rVV5	6086	11287	0.75%	0.106%
80	12.192	3361	3375	3398	rBV	472733	774402	51.66%	7.295%
81	13.233	3695	3699	3701	rBV4	863	745	0.05%	0.007%




Sum of corrected areas: 10616206

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051198.D
Acq On : 07 Oct 2022 02:02
Operator : JC/MD
Sample : N4890-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

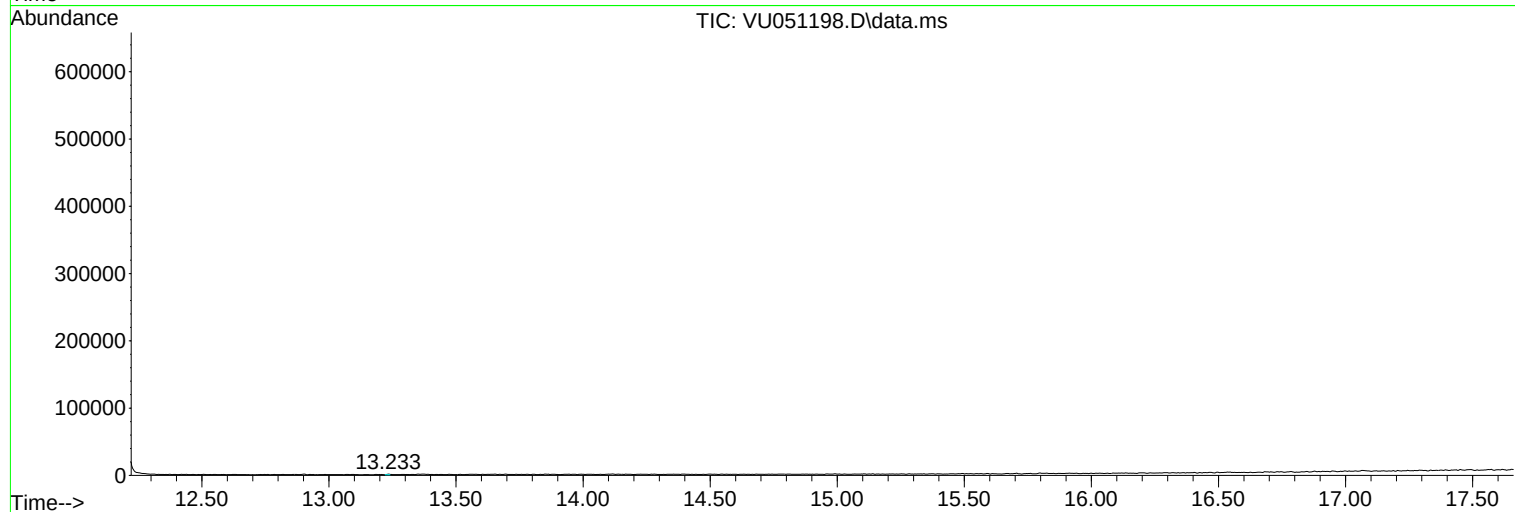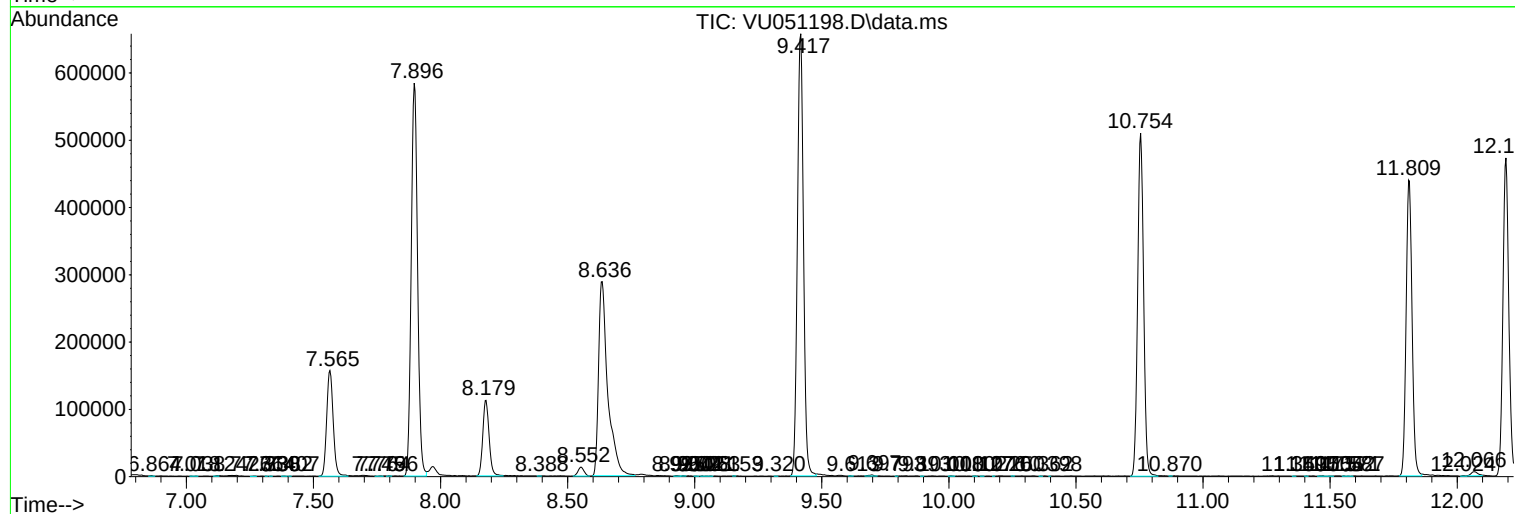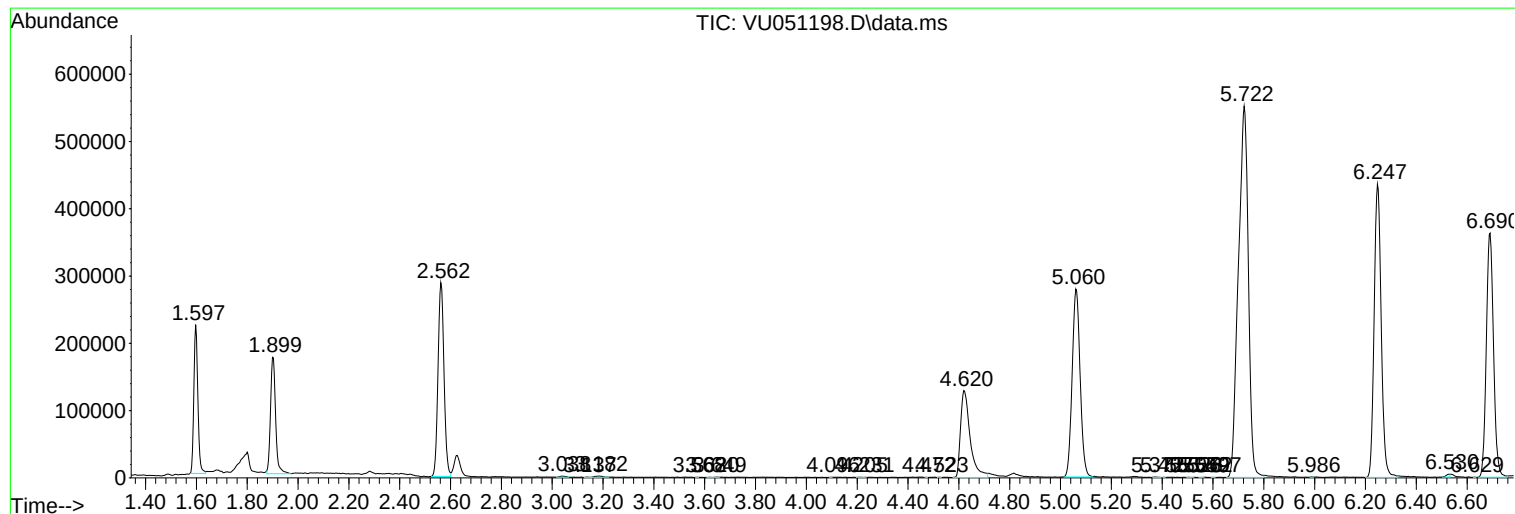

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051198.D
Acq On : 07 Oct 2022 02:02
Operator : JC/MD
Sample : N4890-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051198.D
Acq On : 07 Oct 2022 02:02
Operator : JC/MD
Sample : N4890-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------