

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051200.D
 Acq On : 07 Oct 2022 02:49
 Operator : JC/MD
 Sample : N4890-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051200.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	225033	244888	15.98%	2.148%
2	1.900	167	174	190	rVB	176784	236482	15.43%	2.074%
3	2.562	368	380	395	rBV	291359	475167	31.01%	4.167%
4	3.041	521	529	538	rVB4	1953	3107	0.20%	0.027%
5	3.089	538	544	548	rBV3	518	650	0.04%	0.006%
6	3.144	558	561	565	rBV2	439	265	0.02%	0.002%
7	3.527	677	680	682	rBV2	226	142	0.01%	0.001%
8	3.581	695	697	700	rBV	180	93	0.01%	0.001%
9	3.732	742	744	747	rBV	211	149	0.01%	0.001%
10	3.777	756	758	761	rBV	341	183	0.01%	0.002%
11	3.999	825	827	828	rBV	179	89	0.01%	0.001%
12	4.099	855	858	859	rBV	149	70	0.00%	0.001%
13	4.289	912	917	920	rBV2	220	243	0.02%	0.002%
14	4.314	922	925	929	rVB	327	207	0.01%	0.002%
15	4.363	937	940	942	rVB	302	141	0.01%	0.001%
16	4.395	942	950	952	rBV2	388	502	0.03%	0.004%
17	4.440	962	964	968	rVB	216	96	0.01%	0.001%
18	4.465	968	972	977	rBV2	240	264	0.02%	0.002%
19	4.520	987	989	993	rVB	202	123	0.01%	0.001%
20	4.546	993	997	1001	rBV2	115	115	0.01%	0.001%
21	4.565	1001	1003	1004	rVB	159	59	0.00%	0.001%
22	4.620	1004	1020	1049	rBV2	129714	338439	22.08%	2.968%
23	4.980	1130	1132	1134	rBV	356	219	0.01%	0.002%
24	5.060	1141	1157	1184	rBV	285365	623225	40.67%	5.466%
25	5.256	1216	1218	1221	rBV3	529	336	0.02%	0.003%
26	5.311	1221	1235	1250	rVB8	4657	11886	0.78%	0.104%
27	5.375	1250	1255	1259	rBV2	509	521	0.03%	0.005%
28	5.459	1279	1281	1282	rBV	141	74	0.00%	0.001%
29	5.559	1310	1312	1313	rBV	146	57	0.00%	0.000%
30	5.626	1331	1333	1335	rBV2	195	114	0.01%	0.001%
31	5.723	1342	1363	1389	rBV2	564793	1532470	100.00%	13.440%
32	6.035	1457	1460	1462	rBV2	526	284	0.02%	0.002%
33	6.105	1479	1482	1485	rBV3	259	186	0.01%	0.002%
34	6.125	1485	1488	1493	rVB3	540	385	0.03%	0.003%
35	6.166	1498	1501	1503	rBV2	218	165	0.01%	0.001%
36	6.195	1507	1510	1511	rBV	151	87	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051200.D
 Acq On : 07 Oct 2022 02:49
 Operator : JC/MD
 Sample : N4890-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.247	1511	1526	1548	rBV	452375	860442	56.15%	7.546%
38	6.488	1599	1601	1603	rBV	249	120	0.01%	0.001%
39	6.539	1603	1617	1638	rBV	305666	581022	37.91%	5.096%
40	6.687	1650	1663	1684	rBV	367784	720275	47.00%	6.317%
41	7.031	1765	1770	1774	rBV2	471	427	0.03%	0.004%
42	7.051	1774	1776	1779	rVB2	307	191	0.01%	0.002%
43	7.327	1856	1862	1865	rBV2	229	237	0.02%	0.002%
44	7.346	1865	1868	1870	rBV2	119	56	0.00%	0.000%
45	7.362	1870	1873	1876	rBV3	290	189	0.01%	0.002%
46	7.417	1885	1890	1895	rBV3	416	427	0.03%	0.004%
47	7.456	1898	1902	1906	rBV2	155	173	0.01%	0.002%
48	7.485	1906	1911	1913	rBV2	194	178	0.01%	0.002%
49	7.565	1923	1936	1953	rBV	158919	280624	18.31%	2.461%
50	7.819	2012	2015	2017	rVB2	285	160	0.01%	0.001%
51	7.838	2017	2021	2024	rVB	551	433	0.03%	0.004%
52	7.896	2024	2039	2055	rBV	606332	1035162	67.55%	9.078%
53	8.179	2115	2127	2145	rBV	114177	193950	12.66%	1.701%
54	8.404	2195	2197	2202	rVB2	529	438	0.03%	0.004%
55	8.459	2212	2214	2218	rBV2	371	251	0.02%	0.002%
56	8.552	2234	2243	2253	rVB3	9941	16723	1.09%	0.147%
57	8.636	2257	2269	2313	rBV5	298960	746001	48.68%	6.542%
58	8.980	2374	2376	2377	rBV5	288	127	0.01%	0.001%
59	9.108	2414	2416	2419	rBV2	424	304	0.02%	0.003%
60	9.150	2426	2429	2434	rVB4	619	544	0.04%	0.005%
61	9.369	2494	2497	2499	rVB2	290	142	0.01%	0.001%
62	9.417	2499	2512	2535	rBV	667261	1118064	72.96%	9.805%
63	9.604	2566	2570	2574	rVB3	560	518	0.03%	0.005%
64	9.761	2617	2619	2622	rVB	387	166	0.01%	0.001%
65	9.784	2623	2626	2628	rBV2	290	168	0.01%	0.001%
66	9.816	2635	2636	2637	rBV2	200	74	0.00%	0.001%
67	10.009	2693	2696	2698	rBV	193	95	0.01%	0.001%
68	10.044	2703	2707	2708	rBV	297	252	0.02%	0.002%
69	10.304	2785	2788	2789	rBV	171	108	0.01%	0.001%
70	10.343	2797	2800	2805	rVB3	330	262	0.02%	0.002%
71	10.372	2805	2809	2812	rBV3	323	267	0.02%	0.002%
72	10.391	2812	2815	2817	rVV2	285	164	0.01%	0.001%
73	10.407	2817	2820	2827	rVB2	490	438	0.03%	0.004%
74	10.449	2830	2833	2835	rBV	269	154	0.01%	0.001%
75	10.562	2866	2868	2870	rVB	230	77	0.01%	0.001%
76	10.578	2870	2873	2877	rBV	288	275	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051200.D
 Acq On : 07 Oct 2022 02:49
 Operator : JC/MD
 Sample : N4890-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

77	10.755	2915	2928	2944	rBV	519679	836463	54.58%	7.336%
78	10.941	2983	2986	2989	rBV2	546	336	0.02%	0.003%
79	11.002	3002	3005	3006	rBV	323	181	0.01%	0.002%
80	11.436	3136	3140	3141	rBV	279	209	0.01%	0.002%
81	11.729	3227	3231	3233	rBV2	433	308	0.02%	0.003%
82	11.748	3234	3237	3243	rBV4	686	474	0.03%	0.004%
83	11.809	3244	3256	3276	rBV	462447	747983	48.81%	6.560%
84	12.073	3332	3338	3341	rBV4	1745	2068	0.13%	0.018%
85	12.192	3362	3375	3395	rBV	474486	780480	50.93%	6.845%
86	13.037	3633	3638	3641	rBV2	801	704	0.05%	0.006%
87	13.131	3664	3667	3672	rBV2	572	533	0.03%	0.005%
88	13.240	3695	3701	3704	rBV3	693	885	0.06%	0.008%
89	13.591	3807	3810	3814	rBV	915	816	0.05%	0.007%




Sum of corrected areas: 11402601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051200.D
Acq On : 07 Oct 2022 02:49
Operator : JC/MD
Sample : N4890-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

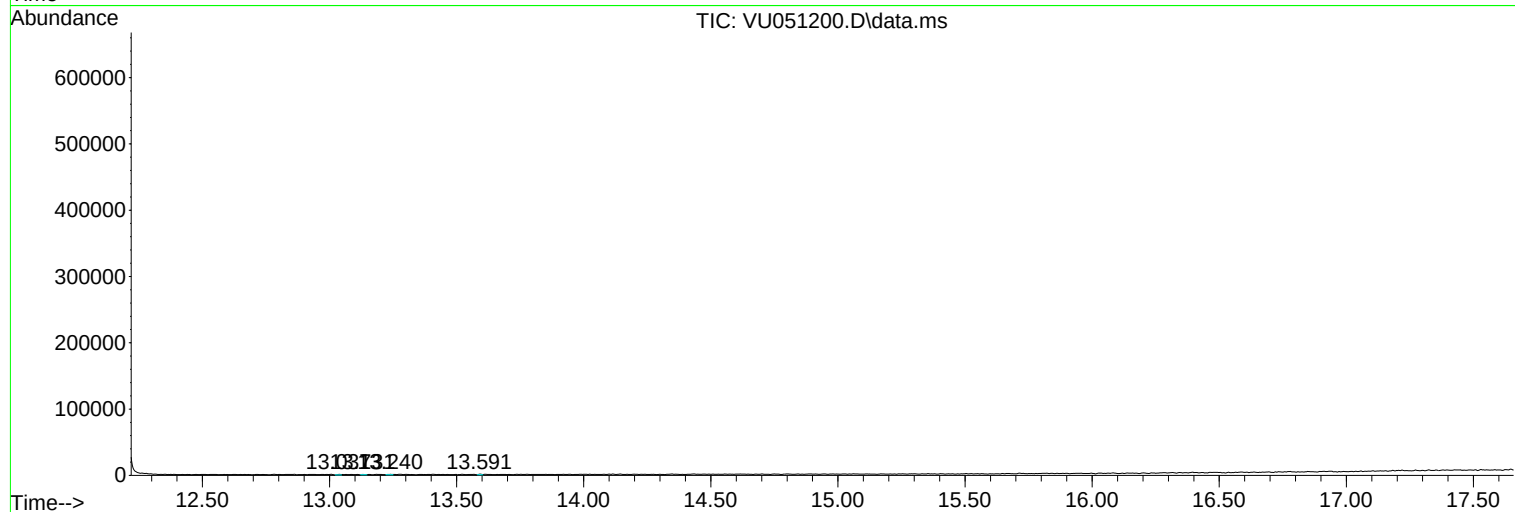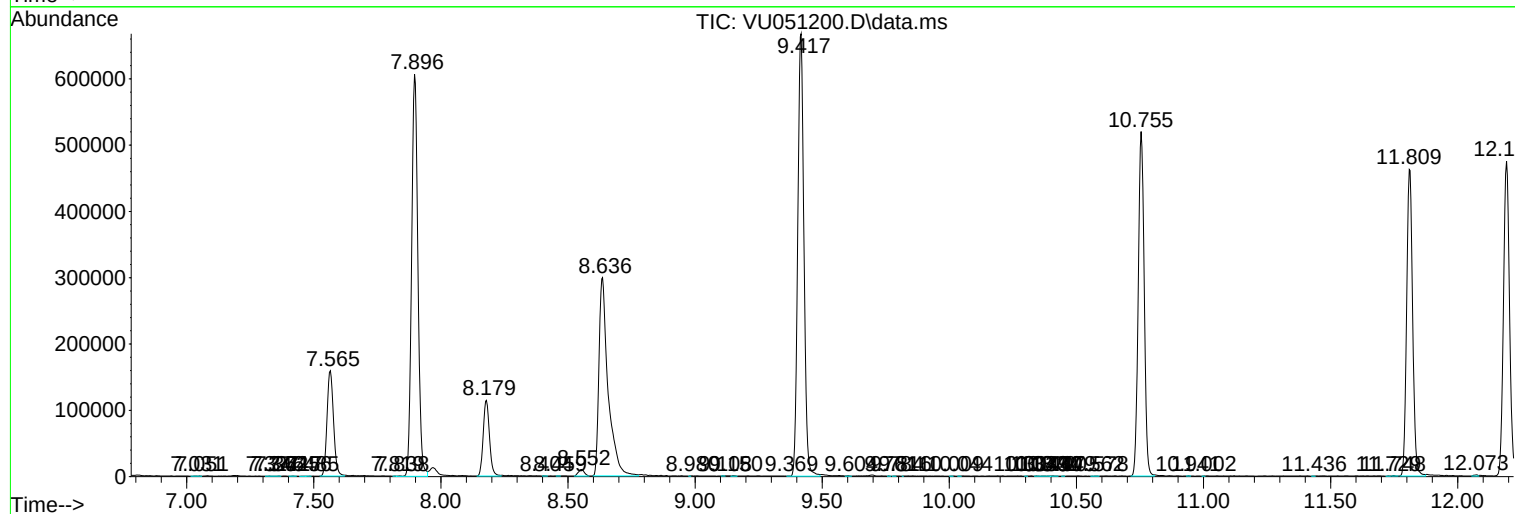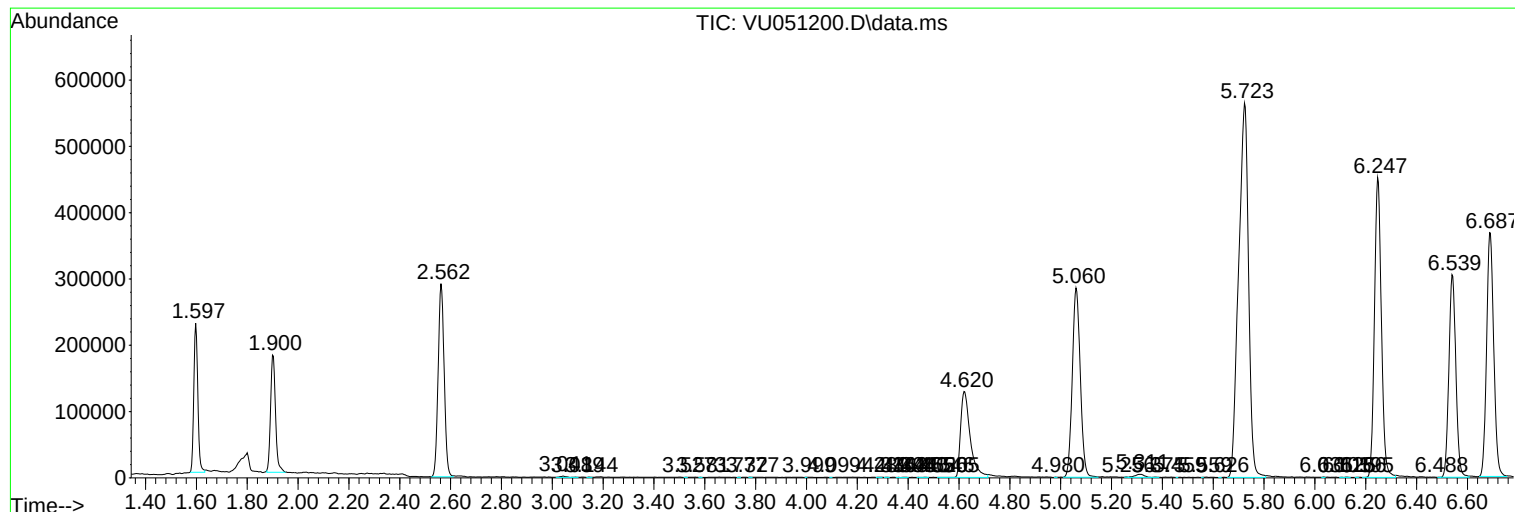

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051200.D
Acq On : 07 Oct 2022 02:49
Operator : JC/MD
Sample : N4890-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051200.D
Acq On : 07 Oct 2022 02:49
Operator : JC/MD
Sample : N4890-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------