

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051203.D
 Acq On : 07 Oct 2022 04:00
 Operator : JC/MD
 Sample : N4893-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	237060	260484	2.20%	1.146%
2	1.903	168	175	196	rVB	186533	250575	2.12%	1.102%
3	2.562	368	380	394	rBV	315723	510247	4.31%	2.244%
4	2.893	481	483	487	rBV2	391	332	0.00%	0.001%
5	3.044	524	530	534	rBV3	1087	1469	0.01%	0.006%
6	3.359	618	628	647	rVB2	9785	22351	0.19%	0.098%
7	3.523	677	679	680	rVB	243	79	0.00%	0.000%
8	3.533	680	682	684	rBV	91	39	0.00%	0.000%
9	3.591	698	700	706	rVB	252	194	0.00%	0.001%
10	3.629	710	712	715	rVB	415	207	0.00%	0.001%
11	3.661	718	722	727	rVB2	507	504	0.00%	0.002%
12	3.745	744	748	750	rVB2	287	190	0.00%	0.001%
13	3.758	750	752	755	rBV2	136	73	0.00%	0.000%
14	3.777	755	758	760	rBV	238	166	0.00%	0.001%
15	3.806	765	767	768	rBV	202	91	0.00%	0.000%
16	3.909	796	799	800	rBV	219	130	0.00%	0.001%
17	4.009	826	830	831	rBV	478	347	0.00%	0.002%
18	4.060	843	846	848	rBV2	318	188	0.00%	0.001%
19	4.140	864	871	874	rBV2	306	445	0.00%	0.002%
20	4.430	957	961	965	rBV2	234	265	0.00%	0.001%
21	4.481	976	977	979	rVB	326	78	0.00%	0.000%
22	4.517	985	988	990	rBV	228	170	0.00%	0.001%
23	4.623	1009	1021	1056	rBV	132770	376400	3.18%	1.655%
24	5.060	1140	1157	1180	rBV	287129	632861	5.35%	2.783%
25	5.202	1197	1201	1202	rBV2	629	460	0.00%	0.002%
26	5.423	1267	1270	1272	rBV	384	249	0.00%	0.001%
27	5.472	1283	1285	1287	rBV2	192	107	0.00%	0.000%
28	5.529	1298	1303	1306	rBV2	394	395	0.00%	0.002%
29	5.597	1321	1324	1328	rBV2	300	214	0.00%	0.001%
30	5.722	1342	1363	1393	rBV2	583577	1578704	13.33%	6.943%
31	5.989	1444	1446	1449	rVB2	487	245	0.00%	0.001%
32	6.005	1449	1451	1452	rBV	247	111	0.00%	0.000%
33	6.054	1465	1466	1469	rVB	588	162	0.00%	0.001%
34	6.073	1469	1472	1473	rBV	318	196	0.00%	0.001%
35	6.108	1479	1483	1485	rBV	353	295	0.00%	0.001%
36	6.156	1495	1498	1501	rBV	286	185	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051203.D
 Acq On : 07 Oct 2022 04:00
 Operator : JC/MD
 Sample : N4893-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.179	1501	1505	1509	rVB2	321	275	0.00%	0.001%
38	6.250	1510	1527	1552	rBV	490070	943361	7.97%	4.149%
39	6.455	1589	1591	1594	rVB	429	218	0.00%	0.001%
40	6.478	1594	1598	1600	rBV2	440	339	0.00%	0.001%
41	6.542	1605	1618	1640	rVB2	78905	153539	1.30%	0.675%
42	6.619	1640	1642	1646	rBV3	392	252	0.00%	0.001%
43	6.690	1649	1664	1688	rBV	378874	739355	6.24%	3.252%
44	6.886	1723	1725	1727	rBV	254	128	0.00%	0.001%
45	6.912	1731	1733	1736	rBV	197	95	0.00%	0.000%
46	6.970	1748	1751	1756	rBV2	255	264	0.00%	0.001%
47	7.034	1769	1771	1774	rVB2	374	165	0.00%	0.001%
48	7.050	1774	1776	1778	rBV	239	125	0.00%	0.001%
49	7.102	1785	1792	1794	rBV4	737	839	0.01%	0.004%
50	7.166	1807	1812	1815	rBV6	990	1111	0.01%	0.005%
51	7.230	1830	1832	1835	rBV	167	122	0.00%	0.001%
52	7.250	1835	1838	1839	rBV	184	98	0.00%	0.000%
53	7.275	1845	1846	1850	rVB	221	100	0.00%	0.000%
54	7.308	1850	1856	1861	rBV2	234	314	0.00%	0.001%
55	7.385	1877	1880	1883	rBV2	256	155	0.00%	0.001%
56	7.404	1883	1886	1887	rBV	234	137	0.00%	0.001%
57	7.423	1891	1892	1896	rBV	202	153	0.00%	0.001%
58	7.452	1899	1901	1904	rBV	205	128	0.00%	0.001%
59	7.472	1905	1907	1909	rBV	173	103	0.00%	0.000%
60	7.565	1924	1936	1955	rBV	165294	288742	2.44%	1.270%
61	7.822	2015	2016	2020	rVB	261	143	0.00%	0.001%
62	7.896	2024	2039	2056	rBV	635805	1095607	9.25%	4.818%
63	8.179	2114	2127	2150	rBV	114994	196284	1.66%	0.863%
64	8.552	2227	2243	2259	rBV	7030007	11839634	100.00%	52.070%
65	9.417	2498	2512	2533	rBV	740378	1224129	10.34%	5.384%
66	9.693	2592	2598	2606	rBV6	1816	2519	0.02%	0.011%
67	10.256	2771	2773	2774	rBV6	242	87	0.00%	0.000%
68	10.603	2878	2881	2883	rBV2	342	230	0.00%	0.001%
69	10.754	2915	2928	2947	rBV	527992	838667	7.08%	3.688%
70	10.838	2951	2954	2957	rBV3	714	594	0.01%	0.003%
71	11.121	3039	3042	3046	rBV2	394	267	0.00%	0.001%
72	11.285	3090	3093	3096	rBV2	580	429	0.00%	0.002%
73	11.407	3128	3131	3134	rBV	419	258	0.00%	0.001%
74	11.468	3141	3150	3160	rBV3	5379	7973	0.07%	0.035%
75	11.812	3244	3257	3279	rBV	521980	851373	7.19%	3.744%
76	12.063	3325	3335	3356	rBV4	18295	36910	0.31%	0.162%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051203.D
Acq On : 07 Oct 2022 04:00
Operator : JC/MD
Sample : N4893-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J21

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Title : VOC Analysis

77	12.192	3362	3375	3394	rBV	532467	872098	7.37%	3.835%
78	12.684	3523	3528	3532	rBV3	708	675	0.01%	0.003%
79	12.809	3564	3567	3569	rBV	480	361	0.00%	0.002%
80	13.076	3647	3650	3654	rBV2	553	466	0.00%	0.002%




Sum of corrected areas: 22738030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051203.D
Acq On : 07 Oct 2022 04:00
Operator : JC/MD
Sample : N4893-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

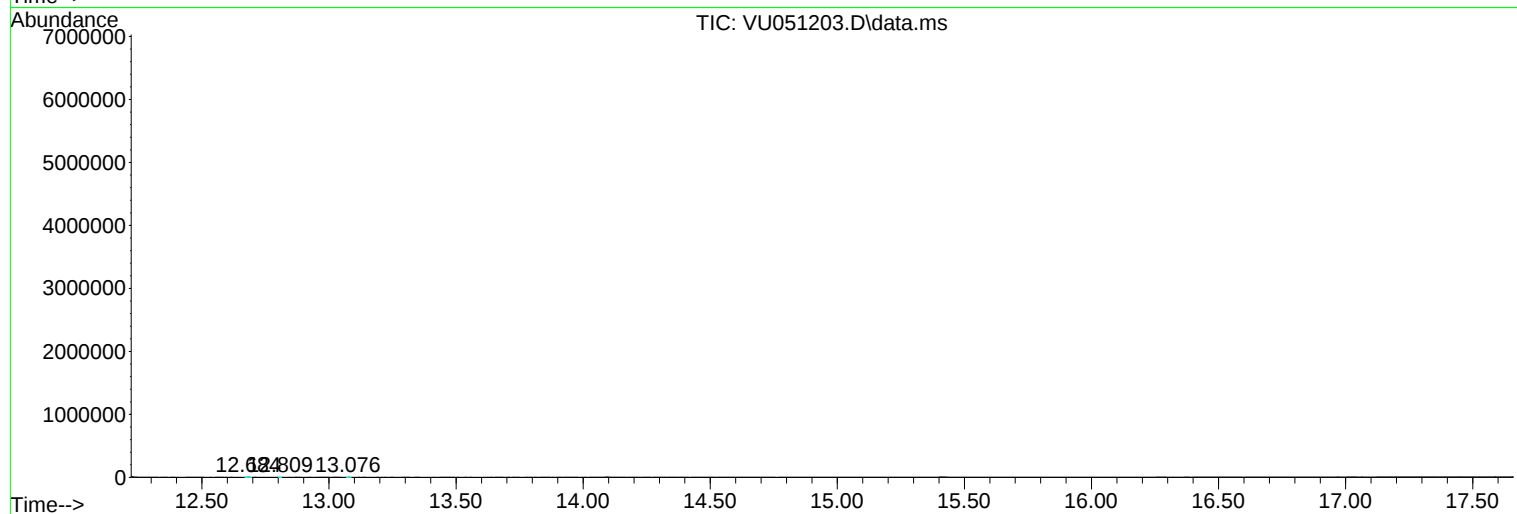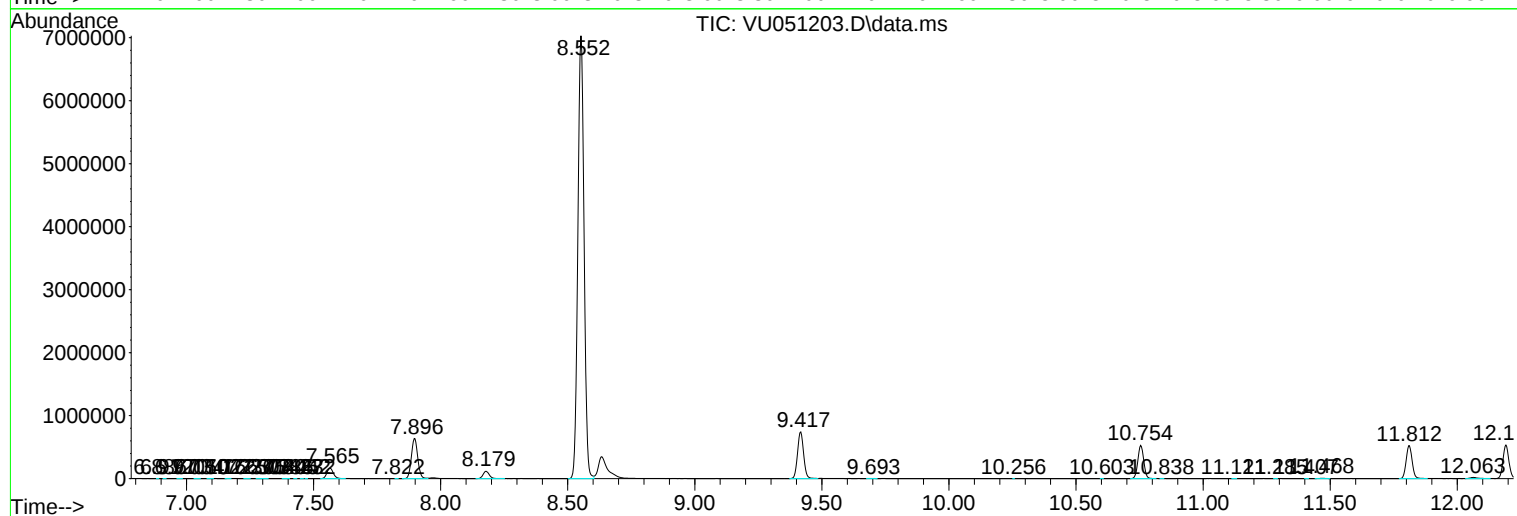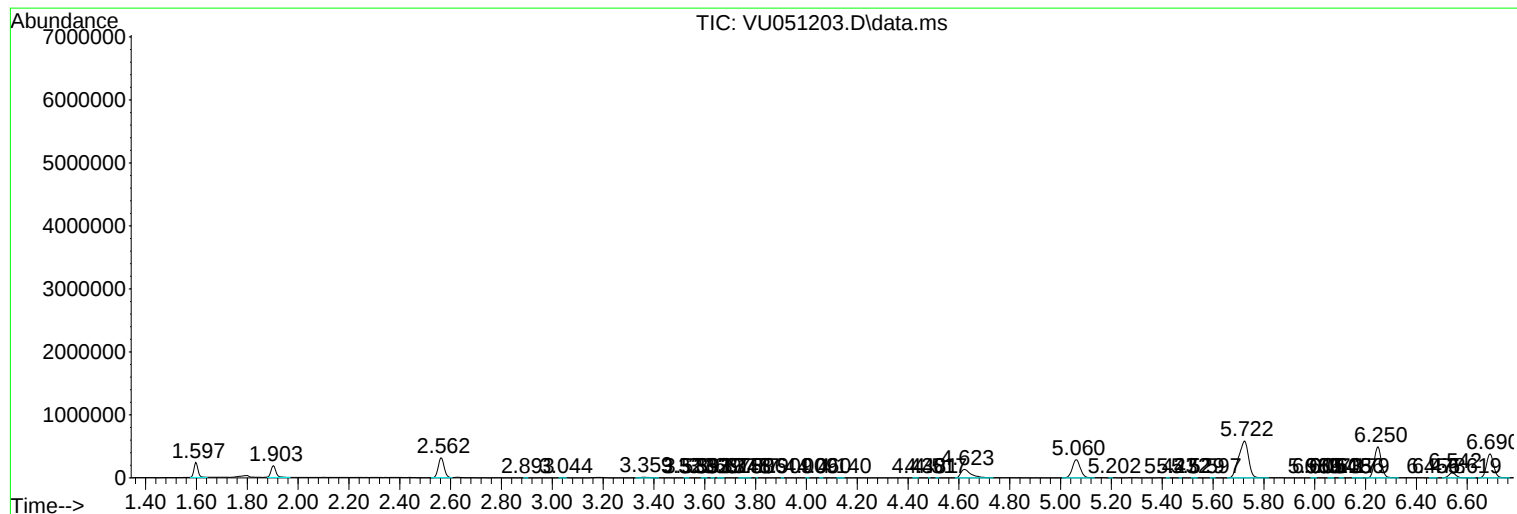

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051203.D
Acq On : 07 Oct 2022 04:00
Operator : JC/MD
Sample : N4893-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
Data File : VU051203.D
Acq On : 07 Oct 2022 04:00
Operator : JC/MD
Sample : N4893-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------