


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100622\
 Data File : VU051163.D
 Acq On : 06 Oct 2022 09:55
 Operator : JC/MD
 Sample : BFB137
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB137

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 07 02:51:40 2022

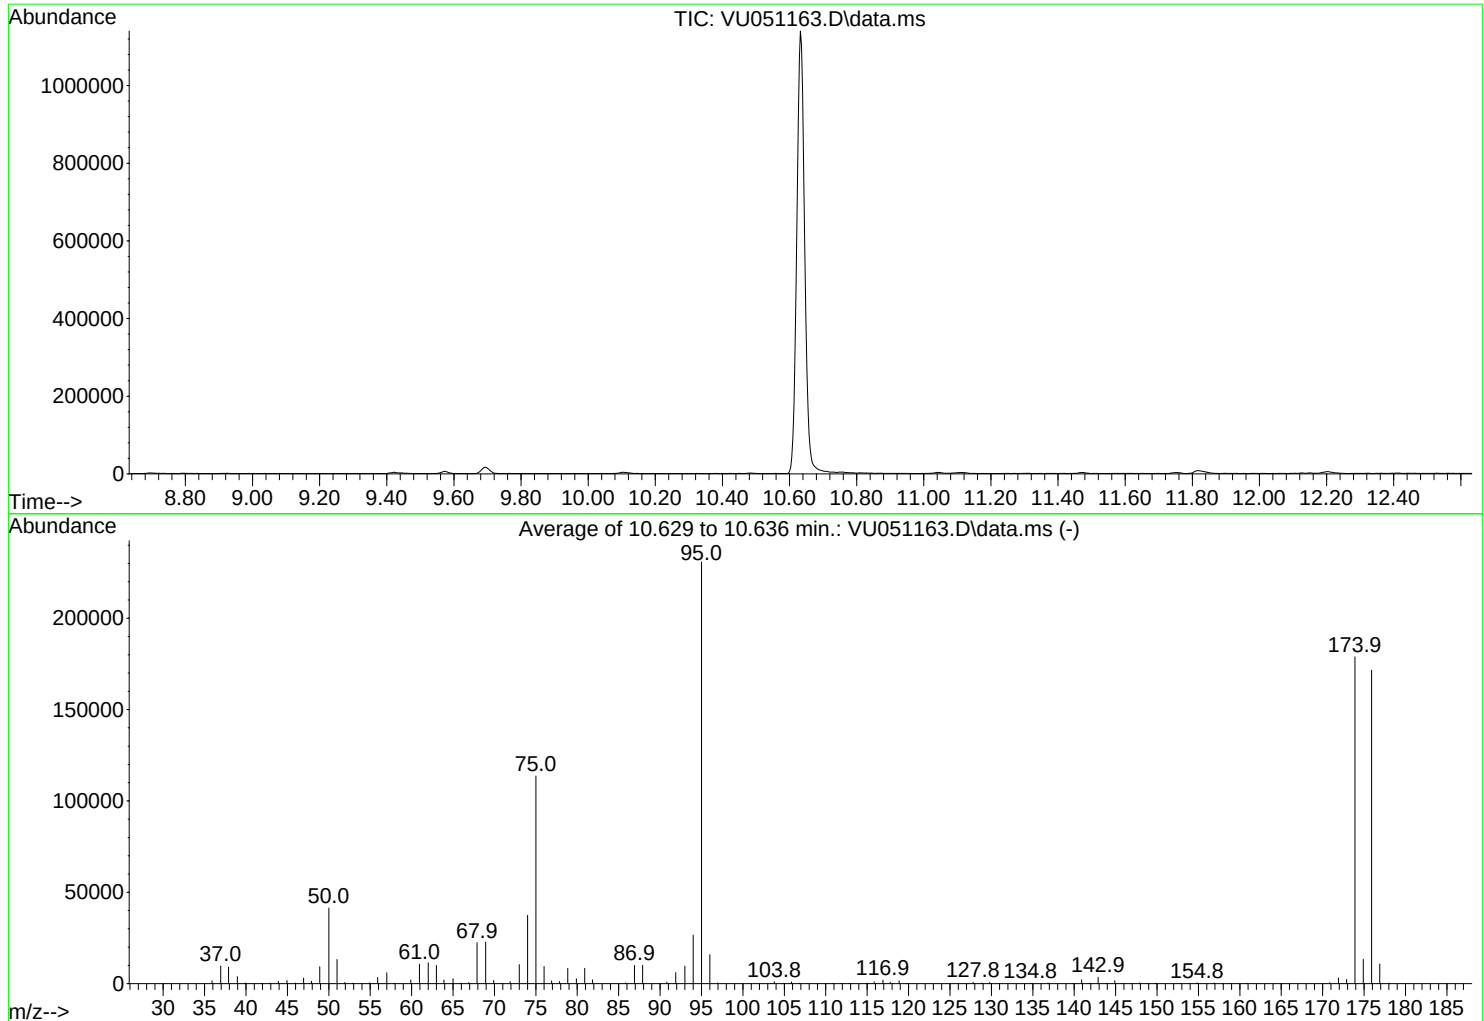

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	41448	PASS
75	95	30	80	49.3	113717	PASS
95	95	100	100	100.0	230869	PASS
96	95	5	9	6.9	15875	PASS
173	174	0.00	2	1.3	2324	PASS
174	95	50	120	77.5	178816	PASS
175	174	5	9	7.5	13330	PASS
176	174	95	101	96.0	171605	PASS
177	176	5	9	6.3	10753	PASS

Scan 2876 (10.587 min): VU051163.D\data.ms
BFB137

m/z	Abundance
39.80	274.0
43.90	661.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	1553.0
37.00	9641.0
37.90	8953.0
38.90	3808.0
39.90	572.0
40.80	164.0
41.80	143.0
42.90	323.0
43.90	1862.0
45.00	1708.0
45.90	429.0
46.90	3092.0
47.90	1337.0
48.90	9089.0
50.00	40864.0
51.00	13344.0
52.00	685.0
52.90	315.0
54.00	205.0
54.90	472.0
55.90	3397.0
57.00	5767.0
57.90	232.0
59.90	2146.0
61.00	10355.0
62.00	11186.0
63.00	9950.0
63.90	2007.0
65.00	2751.0
66.00	271.0
67.00	636.0
67.90	21584.0
68.90	22008.0
69.90	1791.0
70.90	161.0
71.90	1024.0
73.00	10248.0
74.00	36320.0
75.00	111856.0
76.00	9088.0
76.90	1465.0
77.90	1227.0
78.80	8192.0
79.90	2629.0
80.90	8395.0
81.90	2179.0
85.80	416.0
86.90	9868.0
87.90	9834.0
90.80	965.0
91.90	6025.0
93.00	9207.0
94.00	25944.0
95.00	224192.0
96.00	15804.0
97.00	437.0
103.80	1058.0
104.90	314.0
105.90	940.0
106.80	254.0
107.80	126.0
110.80	245.0
111.80	134.0
112.90	186.0
115.00	268.0
115.90	911.0
116.90	1944.0
117.80	729.0
118.80	1490.0
127.80	749.0
128.90	356.0
129.80	615.0
131.00	197.0
134.80	280.0
136.90	352.0
139.90	148.0
140.90	1990.0
141.90	229.0
142.90	3493.0
143.90	219.0
144.90	1651.0
146.00	322.0
146.90	178.0
147.90	429.0
149.80	203.0
152.80	156.0
153.90	198.0
154.90	420.0
156.90	309.0
157.90	111.0
158.70	150.0
160.80	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

170.90	544.0
171.90	3053.0
172.90	2386.0
173.90	170624.0
174.90	12962.0
175.90	163008.0
176.90	10307.0
178.00	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	1711.0
37.00	10031.0
37.90	9341.0
39.00	3928.0
40.00	647.0
40.80	120.0
41.80	146.0
42.90	269.0
44.00	1941.0
44.90	1812.0
45.90	416.0
47.00	3262.0
47.90	1326.0
48.90	9658.0
50.00	42976.0
51.00	13583.0
51.90	738.0
52.90	274.0
54.00	201.0
54.90	460.0
55.90	3367.0
57.00	6149.0
57.90	272.0
59.90	2096.0
60.90	11035.0
62.00	11890.0
63.00	10255.0
63.90	1941.0
65.00	2792.0
66.00	305.0
66.90	552.0
67.90	23160.0
68.90	23432.0
69.90	1875.0
70.90	173.0
71.90	1049.0
73.00	10759.0
74.00	38496.0
75.00	117008.0
76.00	9646.0
76.90	1518.0
77.80	1201.0
78.80	8644.0
79.90	2630.0
80.90	8600.0
81.80	2126.0
85.80	473.0
86.90	10301.0
87.90	10328.0
90.80	915.0
91.90	6173.0
93.00	9965.0
94.00	27480.0
95.00	238656.0
96.00	16552.0
96.90	416.0
103.80	1138.0
104.90	283.0
105.80	950.0
106.80	264.0
107.80	126.0
110.80	182.0
111.90	144.0
112.80	180.0
115.00	264.0
115.90	1051.0
116.90	2027.0
117.80	829.0
118.90	1626.0
127.80	841.0
128.80	369.0
129.80	669.0
131.00	207.0
134.70	313.0
136.90	331.0
139.80	142.0
140.90	2209.0
141.90	244.0
142.90	3592.0
143.90	218.0
144.90	1711.0
145.90	305.0
146.90	186.0
147.90	503.0
149.80	245.0
152.80	170.0
153.80	192.0
154.90	425.0
156.90	419.0
158.70	192.0
160.80	289.0
170.80	543.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

171.90	3183.0
172.90	2384.0
173.90	184192.0
174.90	13745.0
175.90	177216.0
176.90	10956.0
178.00	286.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	1594.0
36.90	9356.0
37.90	8842.0
39.00	3810.0
40.00	696.0
41.90	126.0
42.90	237.0
44.00	1874.0
44.90	1776.0
46.00	341.0
47.00	2911.0
47.90	1239.0
48.90	9018.0
50.00	40504.0
51.00	12766.0
51.90	682.0
52.80	289.0
53.90	179.0
54.90	484.0
55.90	3121.0
57.00	6006.0
57.90	294.0
59.90	1888.0
60.90	10657.0
62.00	11158.0
63.00	9662.0
63.90	1746.0
65.00	2617.0
65.90	332.0
66.80	557.0
67.90	22440.0
69.00	22984.0
69.90	1697.0
70.90	164.0
71.90	1010.0
73.00	10328.0
74.00	37304.0
75.00	112288.0
76.00	9441.0
76.90	1455.0
77.80	1052.0
78.90	8158.0
79.90	2538.0
80.90	8301.0
81.80	1903.0
85.90	485.0
86.90	9889.0
87.90	9889.0
90.80	803.0
91.90	5844.0
93.00	9820.0
94.00	26136.0
95.00	229760.0
96.00	15269.0
96.90	408.0
103.80	1081.0
105.00	312.0
105.80	932.0
106.80	245.0
110.80	153.0
111.80	173.0
112.80	174.0
115.00	245.0
115.80	1043.0
116.90	1805.0
117.80	872.0
118.80	1549.0
119.70	123.0
127.80	816.0
128.80	338.0
129.80	692.0
130.90	199.0
134.70	284.0
136.80	304.0
139.80	159.0
140.90	2114.0
141.80	216.0
142.90	3361.0
143.80	248.0
144.90	1612.0
145.70	327.0
146.80	170.0
147.90	518.0
148.90	142.0
149.90	263.0
152.80	159.0
153.80	189.0
154.80	433.0
156.90	499.0
158.70	206.0
160.80	284.0
170.80	510.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

171.90	3016.0
172.90	2202.0
173.90	181632.0
174.90	13282.0
175.90	174592.0
176.90	10997.0
178.00	278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137