


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100719\
Data File : VU034948.D
Acq On : 07 Oct 2019 08:59
Operator : JC/SP
Sample : BFB14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB14

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Oct 09 17:41:54 2019

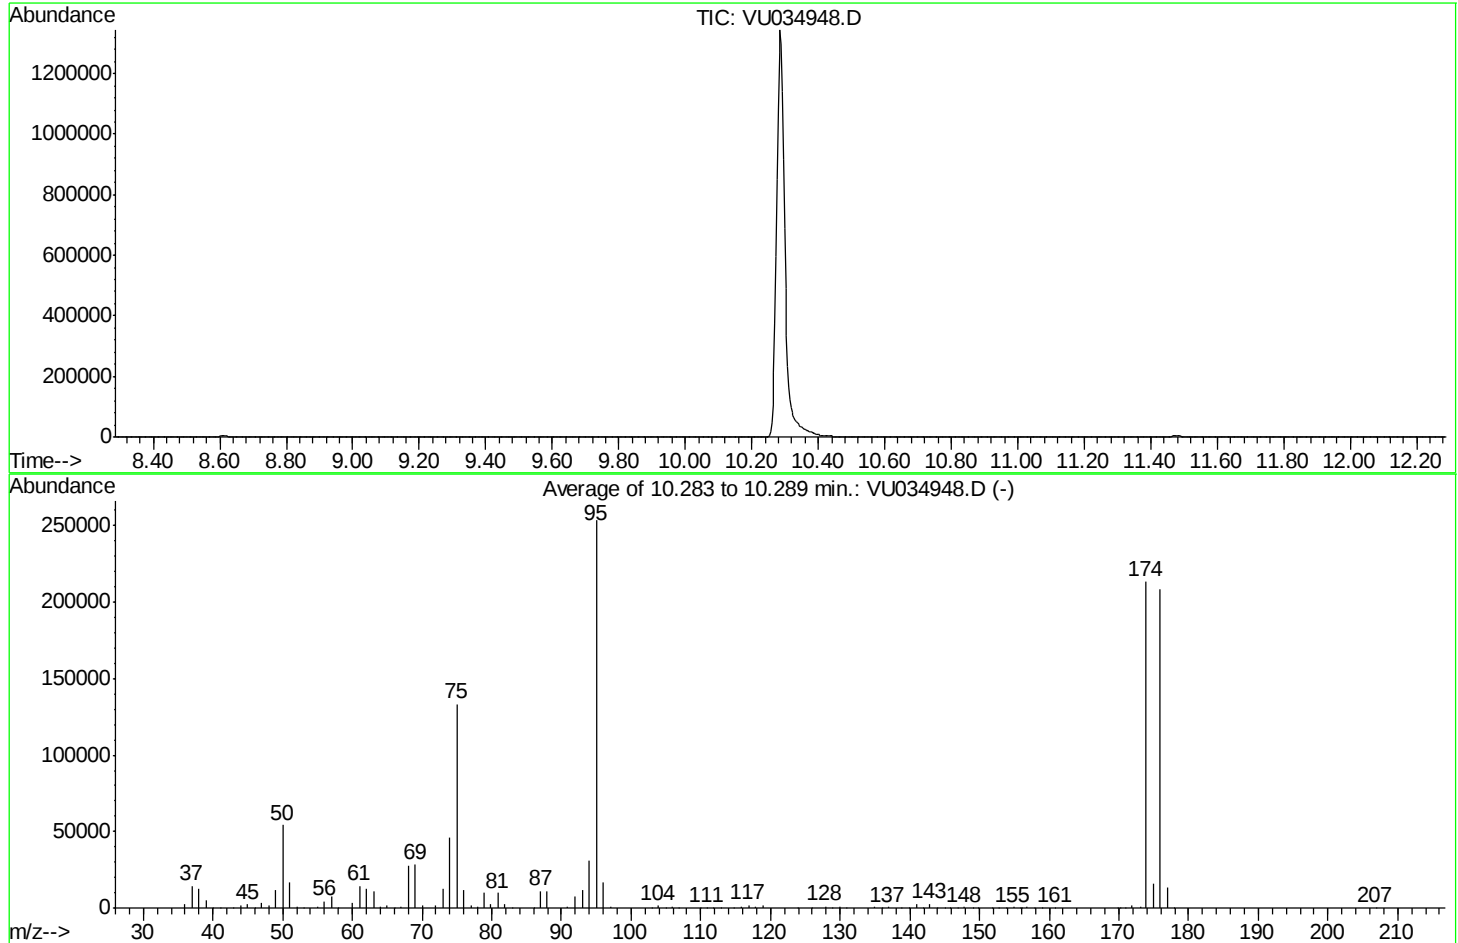

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	54274	PASS
75	95	30	80	52.6	133357	PASS
95	95	100	100	100.0	253504	PASS
96	95	5	9	6.7	16957	PASS
173	174	0.00	2	0.5	973	PASS
174	95	50	120	84.1	213290	PASS
175	174	5	9	7.6	16215	PASS
176	174	95	101	97.8	208533	PASS
177	176	5	9	6.5	13456	PASS

m/z	Abundance
36.00	2869.0
37.00	14530.0
38.00	12020.0
39.00	5185.0
40.00	455.0
41.00	111.0
43.00	244.0
44.00	2504.0
45.00	2249.0
46.10	302.0
47.00	3181.0
47.90	1480.0
49.00	11868.0
50.00	52864.0
51.00	16295.0
52.00	657.0
52.90	180.0
55.00	633.0
56.00	4581.0
57.00	7712.0
58.00	282.0
60.00	2977.0
61.00	14139.0
62.00	12801.0
63.10	10865.0
64.00	1224.0
65.00	1351.0
66.00	213.0
67.00	775.0
68.00	26888.0
69.00	27712.0
70.00	1930.0
72.00	1562.0
73.00	12099.0
74.00	45736.0
75.00	132800.0
76.00	11215.0
77.00	1319.0
77.90	1097.0
78.90	9517.0
79.90	2892.0
80.90	9799.0
81.90	2439.0
82.90	255.0
86.00	416.0
87.00	10794.0
87.90	10630.0
90.90	1078.0
92.00	7671.0
93.00	11572.0
94.00	30416.0
95.00	248768.0
96.00	16912.0
97.00	535.0
102.90	129.0
103.90	1334.0
105.00	320.0
105.90	1114.0
106.90	233.0
110.00	167.0
110.90	299.0
111.80	239.0
112.80	211.0
114.80	238.0
115.90	1096.0
116.90	1909.0
117.80	1055.0
118.90	1409.0
123.90	159.0
125.90	163.0
127.90	1051.0
128.80	432.0
129.90	901.0
130.80	262.0
134.90	534.0
136.90	637.0
139.90	155.0
141.00	2665.0
141.80	362.0
142.90	2595.0
143.80	257.0
145.00	438.0
145.80	402.0
146.80	227.0
147.80	741.0
149.00	251.0
149.90	233.0
151.80	172.0
152.80	181.0
153.80	165.0
154.90	604.0
155.80	136.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

156.80	370.0
157.90	110.0
158.90	315.0
161.00	231.0
169.80	101.0
170.90	242.0
171.90	1795.0
173.90	203648.0
175.00	15714.0
175.90	197120.0
176.90	13108.0
177.90	348.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
36.00	3045.0
37.00	14958.0
38.00	12769.0
39.00	5211.0
40.00	491.0
42.90	282.0
44.00	2485.0
45.00	2451.0
46.10	306.0
47.00	3397.0
48.00	1651.0
49.00	11931.0
50.00	56264.0
51.00	16936.0
52.00	592.0
53.00	169.0
55.00	656.0
56.00	4761.0
57.00	7869.0
57.90	325.0
60.00	3089.0
61.00	14823.0
62.00	13289.0
63.00	11348.0
64.00	1307.0
65.00	1404.0
66.00	209.0
67.00	785.0
68.00	28448.0
69.00	29304.0
70.00	2100.0
72.00	1639.0
73.00	13153.0
74.00	47608.0
75.00	137600.0
76.00	11609.0
77.00	1439.0
77.90	1128.0
78.90	9964.0
79.90	3028.0
80.90	10252.0
81.90	2504.0
82.90	229.0
86.00	455.0
87.00	11280.0
87.90	11049.0
90.90	1142.0
92.00	8146.0
93.00	12149.0
94.00	32464.0
95.00	261376.0
96.00	17496.0
97.00	568.0
102.90	121.0
103.90	1380.0
105.00	353.0
105.90	1259.0
106.90	310.0
110.00	167.0
110.90	325.0
111.80	251.0
112.80	264.0
114.80	332.0
115.90	1162.0
116.90	1978.0
117.90	1102.0
118.90	1502.0
123.90	187.0
125.90	181.0
127.90	1050.0
128.80	426.0
129.90	1009.0
130.90	312.0
134.90	561.0
135.90	100.0
136.90	580.0
138.80	105.0
139.90	142.0
140.90	2892.0
141.90	374.0
142.90	2849.0
143.90	282.0
145.00	445.0
145.80	393.0
146.80	205.0
147.80	767.0
149.00	241.0
149.80	261.0
151.90	172.0
152.80	179.0
153.80	169.0
154.90	634.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

156.00	171.0
156.80	474.0
158.00	126.0
158.90	378.0
160.90	278.0
169.90	128.0
170.90	285.0
171.90	1911.0
173.90	220288.0
175.00	16600.0
175.90	215040.0
176.90	13916.0
177.90	349.0
206.90	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

m/z	Abundance
36.00	2911.0
37.00	14178.0
38.00	12195.0
39.00	4829.0
40.00	459.0
42.90	282.0
44.00	2275.0
45.00	2415.0
46.00	263.0
47.00	3088.0
48.00	1593.0
49.00	10975.0
50.00	53696.0
51.00	16197.0
52.00	568.0
53.10	152.0
54.90	697.0
56.00	4516.0
57.00	7293.0
57.90	349.0
60.00	2846.0
61.00	14030.0
62.00	12563.0
63.00	10683.0
64.00	1263.0
65.00	1359.0
66.10	166.0
67.00	796.0
68.00	27400.0
69.00	28200.0
70.00	2004.0
72.00	1534.0
73.00	12892.0
74.00	44968.0
75.00	129672.0
76.00	11268.0
77.00	1555.0
77.90	1067.0
78.90	9750.0
79.90	2845.0
80.90	9784.0
81.90	2415.0
82.90	219.0
86.00	434.0
87.00	10771.0
88.00	10552.0
90.90	1105.0
92.00	7860.0
93.00	11672.0
94.00	31368.0
95.00	250368.0
96.00	16464.0
97.00	546.0
102.90	104.0
104.00	1308.0
104.90	344.0
105.90	1251.0
106.90	354.0
109.80	153.0
110.90	297.0
111.90	241.0
112.80	277.0
114.80	395.0
115.90	1039.0
116.90	1885.0
117.90	1084.0
118.90	1498.0
123.90	172.0
125.90	149.0
127.90	902.0
128.80	407.0
129.90	986.0
130.90	318.0
134.90	518.0
136.00	121.0
136.80	459.0
138.80	113.0
139.80	161.0
140.90	2737.0
141.90	382.0
142.90	2914.0
143.90	273.0
145.00	387.0
145.80	340.0
146.90	177.0
147.90	670.0
149.00	160.0
149.80	262.0
151.90	140.0
152.70	153.0
153.90	174.0
154.90	626.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

156.10	181.0
156.90	502.0
157.90	118.0
158.90	389.0
160.80	341.0
170.10	126.0
170.80	258.0
171.90	1843.0
173.10	2920.0
173.90	215936.0
175.00	16331.0
175.90	213440.0
176.90	13346.0
177.90	294.0
206.80	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14

Scan 2845 (10.238 min): VU034948.D
BFB14

m/z	Abundance
39.90	192.0
44.00	434.0

Instrument :
MSVOA_U
ClientSampleId :
BFB14