


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100720\
 Data File : VU040540.D
 Acq On : 07 Oct 2020 10:15
 Operator : SY/MD
 Sample : BFB33
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB203

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMUL100620WMA.M
 Title : VOC Analysis
 Last Update : Thu Oct 08 11:07:54 2020

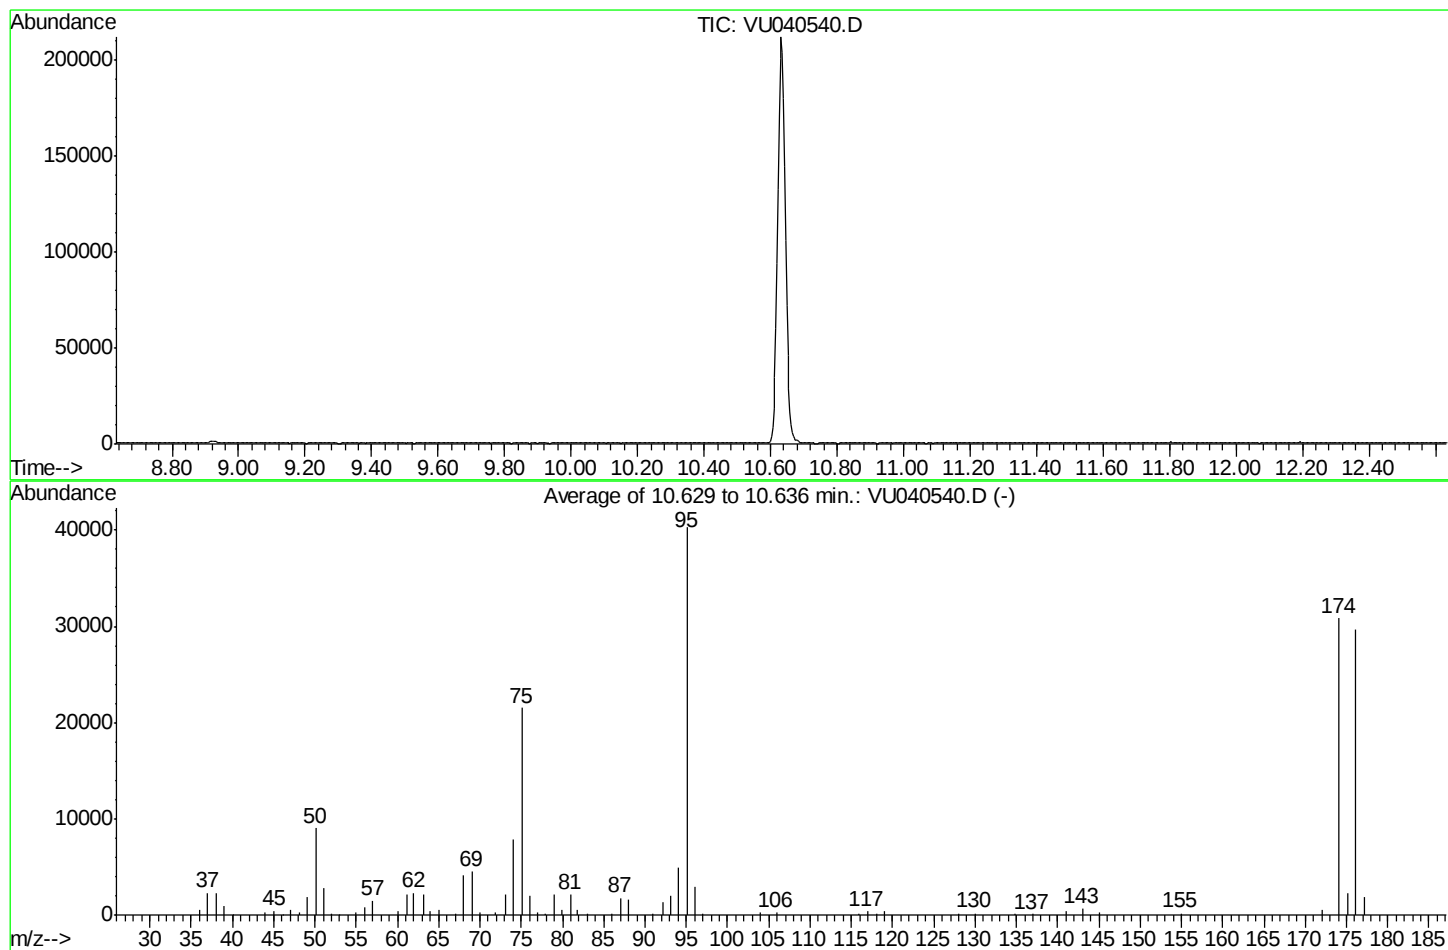

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	9024	PASS
75	95	30	80	53.3	21493	PASS
95	95	100	100	100.0	40288	PASS
96	95	5	9	7.2	2914	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.6	30848	PASS
175	174	5	9	7.4	2289	PASS
176	174	95	101	96.1	29656	PASS
177	176	5	9	6.4	1904	PASS

m/z	Abundance
35.90	497.0
37.00	2296.0
38.00	2262.0
39.10	1073.0
40.00	166.0
44.00	814.0
45.10	401.0
46.10	129.0
47.10	640.0
48.00	195.0
49.10	1937.0
50.10	8668.0
51.00	2869.0
52.00	164.0
52.90	100.0
55.00	197.0
56.00	793.0
57.00	1398.0
60.00	395.0
61.10	2048.0
62.00	2233.0
63.10	2153.0
64.00	401.0
65.10	594.0
67.10	103.0
68.10	3969.0
69.10	4488.0
70.00	250.0
71.90	319.0
73.10	2215.0
74.10	7782.0
75.10	20752.0
76.10	1989.0
77.00	210.0
77.90	147.0
79.00	1943.0
80.00	516.0
81.00	2172.0
81.80	353.0
83.00	132.0
85.90	108.0
87.00	1913.0
88.00	1558.0
91.00	238.0
92.10	1469.0
93.00	2057.0
94.10	4805.0
95.10	39640.0
96.10	2873.0
103.90	152.0
105.90	212.0
115.90	154.0
116.90	361.0
117.90	120.0
119.00	364.0
128.10	110.0
130.00	153.0
134.90	120.0
137.00	101.0
141.00	375.0
143.00	577.0
145.10	270.0
154.90	177.0
172.00	585.0
174.10	29920.0
175.10	2226.0
176.10	28208.0
177.10	1875.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203

m/z	Abundance
36.00	472.0
37.00	2372.0
38.00	2305.0
39.10	952.0
40.10	161.0
44.00	805.0
45.10	467.0
47.10	592.0
48.10	253.0
49.00	1901.0
50.10	9396.0
51.00	2948.0
52.00	158.0
52.90	101.0
55.00	252.0
56.00	857.0
57.00	1560.0
60.00	453.0
61.10	2274.0
62.00	2382.0
63.10	2251.0
64.00	400.0
65.10	564.0
67.10	123.0
68.10	4172.0
69.00	4664.0
70.00	267.0
71.90	293.0
73.10	2283.0
74.10	8061.0
75.10	22080.0
76.10	2027.0
77.00	246.0
77.90	150.0
78.90	2211.0
80.00	546.0
81.00	2208.0
81.90	494.0
83.00	105.0
85.90	115.0
87.00	1781.0
88.00	1761.0
91.00	198.0
92.10	1373.0
93.00	2124.0
94.10	5133.0
95.10	41496.0
96.10	2980.0
97.00	116.0
103.90	220.0
105.90	234.0
115.90	140.0
117.00	385.0
118.00	131.0
118.90	359.0
128.00	172.0
129.90	180.0
134.80	130.0
137.00	134.0
141.10	468.0
143.00	673.0
145.00	238.0
155.00	154.0
172.00	595.0
174.10	31888.0
175.10	2384.0
176.10	30704.0
177.10	1953.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203

m/z	Abundance
36.00	472.0
37.00	2300.0
38.00	2250.0
39.00	888.0
40.10	146.0
44.00	766.0
45.10	436.0
47.00	505.0
48.10	312.0
49.00	1842.0
50.10	9008.0
51.00	2760.0
52.00	141.0
55.00	257.0
56.00	786.0
57.00	1470.0
60.00	472.0
61.10	2258.0
62.00	2301.0
63.10	2113.0
64.00	353.0
65.00	537.0
67.10	140.0
68.00	4141.0
69.00	4406.0
70.00	242.0
71.90	248.0
73.10	2046.0
74.10	7561.0
75.10	21648.0
76.10	1944.0
77.00	243.0
78.00	172.0
78.90	2143.0
79.90	567.0
81.00	1982.0
81.90	582.0
87.00	1612.0
88.00	1656.0
90.90	121.0
92.10	1320.0
93.10	2003.0
94.10	4944.0
95.10	39728.0
96.10	2889.0
97.00	141.0
103.90	254.0
105.90	289.0
116.00	148.0
117.00	335.0
118.10	158.0
118.90	322.0
128.00	188.0
129.90	235.0
137.00	125.0
141.00	481.0
143.00	741.0
145.00	209.0
155.00	131.0
172.00	574.0
174.10	30736.0
175.10	2257.0
176.10	30056.0
177.10	1885.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203

Scan 2877 (10.591 min): VU040540.D
BFB33

m/z	Abundance
40.00	144.0
44.00	493.0

Instrument :
MSVOA_U
ClientSampleId :
BFB203