

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045199.D
 Acq On : 07 Oct 2021 10:09
 Operator : SY/MD
 Sample : VU1007MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045199.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rBV	180044	198854	14.57%	1.933%
2	1.912	171	178	197	rVB	133991	187785	13.76%	1.825%
3	2.520	365	367	369	rBV	149	82	0.01%	0.001%
4	2.568	369	382	402	rVV	282736	467436	34.26%	4.543%
5	2.797	444	453	468	rVB2	1373	2554	0.19%	0.025%
6	2.858	468	472	474	rBV	212	178	0.01%	0.002%
7	2.916	481	490	494	rBV2	239	442	0.03%	0.004%
8	2.938	494	497	499	rBV2	317	233	0.02%	0.002%
9	3.022	520	523	525	rBV	154	104	0.01%	0.001%
10	3.051	525	532	541	rBV3	1642	2472	0.18%	0.024%
11	3.192	567	576	583	rBV3	827	1592	0.12%	0.015%
12	3.295	606	608	613	rVB	131	121	0.01%	0.001%
13	3.350	620	625	627	rBV3	442	347	0.03%	0.003%
14	3.414	642	645	649	rBV	146	152	0.01%	0.001%
15	3.501	669	672	675	rVB	168	122	0.01%	0.001%
16	3.591	697	700	703	rVB2	186	137	0.01%	0.001%
17	3.610	703	706	708	rVB	189	121	0.01%	0.001%
18	3.636	711	714	718	rVB2	171	136	0.01%	0.001%
19	3.700	732	734	740	rVB2	142	129	0.01%	0.001%
20	3.780	755	759	761	rVV2	171	126	0.01%	0.001%
21	3.806	765	767	771	rVB	173	122	0.01%	0.001%
22	3.858	779	783	786	rVV2	171	134	0.01%	0.001%
23	3.874	786	788	792	rVV	176	142	0.01%	0.001%
24	3.919	800	802	805	rVV	214	113	0.01%	0.001%
25	4.009	827	830	831	rBV	186	108	0.01%	0.001%
26	4.054	841	844	847	rBV	208	164	0.01%	0.002%
27	4.099	854	858	860	rBV2	196	185	0.01%	0.002%
28	4.124	864	866	870	rVB	189	88	0.01%	0.001%
29	4.317	923	926	927	rBV	177	101	0.01%	0.001%
30	4.375	941	944	948	rBV2	142	112	0.01%	0.001%
31	4.411	950	955	956	rBV	199	163	0.01%	0.002%
32	4.456	964	969	974	rBV2	248	322	0.02%	0.003%
33	4.568	998	1004	1005	rBV2	154	146	0.01%	0.001%
34	4.626	1008	1022	1058	rBV	142108	341311	25.02%	3.317%
35	5.070	1142	1160	1182	rBV	239876	529106	38.78%	5.142%
36	5.385	1255	1258	1262	rVV3	289	215	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045199.D
 Acq On : 07 Oct 2021 10:09
 Operator : SY/MD
 Sample : VU1007MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	5.433	1270	1273	1278	rBV2	216	152	0.01%	0.001%
38	5.597	1321	1324	1326	rBV	196	120	0.01%	0.001%
39	5.732	1343	1366	1389	rBV2	505235	1364379	100.00%	13.260%
40	6.108	1481	1483	1485	rBV3	376	219	0.02%	0.002%
41	6.253	1514	1528	1550	rBV	370427	699341	51.26%	6.796%
42	6.439	1584	1586	1589	rBV	344	243	0.02%	0.002%
43	6.533	1606	1615	1626	rVB6	4954	9369	0.69%	0.091%
44	6.697	1652	1666	1683	rBV	318020	618342	45.32%	6.009%
45	6.951	1743	1745	1747	rBV2	258	157	0.01%	0.002%
46	6.986	1754	1756	1763	rVB2	209	205	0.02%	0.002%
47	7.185	1811	1818	1825	rBV4	1029	1504	0.11%	0.015%
48	7.263	1840	1842	1846	rBV	179	178	0.01%	0.002%
49	7.295	1850	1852	1854	rBV	109	80	0.01%	0.001%
50	7.362	1868	1873	1877	rBV2	176	122	0.01%	0.001%
51	7.391	1880	1882	1886	rVB	186	88	0.01%	0.001%
52	7.411	1886	1888	1890	rBV2	181	106	0.01%	0.001%
53	7.430	1891	1894	1899	rBV2	187	206	0.02%	0.002%
54	7.571	1925	1938	1967	rBV	184806	327063	23.97%	3.179%
55	7.800	2001	2009	2017	rBV3	3670	5575	0.41%	0.054%
56	7.902	2026	2041	2056	rBV	645042	1090873	79.95%	10.602%
57	8.115	2105	2107	2110	rVB	217	78	0.01%	0.001%
58	8.182	2117	2128	2144	rBV	129908	216571	15.87%	2.105%
59	8.340	2175	2177	2179	rBV	154	82	0.01%	0.001%
60	8.430	2202	2205	2208	rBV2	136	125	0.01%	0.001%
61	8.481	2217	2221	2222	rBV	262	175	0.01%	0.002%
62	8.539	2237	2239	2242	rBV2	127	94	0.01%	0.001%
63	8.636	2256	2269	2326	rVB	398912	739083	54.17%	7.183%
64	8.928	2356	2360	2364	rBV2	480	416	0.03%	0.004%
65	8.976	2371	2375	2376	rBV	154	126	0.01%	0.001%
66	9.002	2381	2383	2386	rBV2	155	107	0.01%	0.001%
67	9.176	2434	2437	2440	rBV2	184	148	0.01%	0.001%
68	9.246	2455	2459	2461	rBV	233	217	0.02%	0.002%
69	9.317	2479	2481	2484	rBV2	137	87	0.01%	0.001%
70	9.420	2500	2513	2554	rVV	518041	872142	63.92%	8.476%
71	9.697	2593	2599	2611	rVB2	2070	2859	0.21%	0.028%
72	9.864	2648	2651	2653	rBV2	189	120	0.01%	0.001%
73	10.031	2700	2703	2710	rVB2	206	213	0.02%	0.002%
74	10.060	2710	2712	2717	rBV	150	126	0.01%	0.001%
75	10.108	2717	2727	2742	rBV7	2432	4782	0.35%	0.046%
76	10.304	2785	2788	2792	rBV	192	130	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045199.D
 Acq On : 07 Oct 2021 10:09
 Operator : SY/MD
 Sample : VU1007MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	10.491	2838	2846	2854	rBV2	1873	2589	0.19%	0.025%
78	10.542	2860	2862	2864	rBV	186	90	0.01%	0.001%
79	10.648	2891	2895	2896	rBV2	280	190	0.01%	0.002%
80	10.674	2896	2903	2912	rVB2	3848	5498	0.40%	0.053%
81	10.761	2917	2930	2946	rBV	423492	681758	49.97%	6.626%
82	10.999	3001	3004	3005	rBV2	279	158	0.01%	0.002%
83	11.092	3026	3033	3038	rBV4	2184	2743	0.20%	0.027%
84	11.275	3086	3090	3092	rBV	215	155	0.01%	0.002%
85	11.301	3095	3098	3100	rBV2	279	150	0.01%	0.001%
86	11.372	3118	3120	3126	rBV2	248	266	0.02%	0.003%
87	11.468	3141	3150	3162	rVB4	4813	8319	0.61%	0.081%
88	11.700	3216	3222	3229	rVV4	1461	2101	0.15%	0.020%
89	11.748	3230	3237	3245	rVB3	3201	4667	0.34%	0.045%
90	11.815	3245	3258	3281	rBV	521412	833163	61.07%	8.097%
91	12.198	3360	3377	3399	rBV	589594	961820	70.50%	9.347%
92	12.327	3414	3417	3418	rBV	735	346	0.03%	0.003%
93	12.449	3452	3455	3459	rBV2	264	298	0.02%	0.003%
94	12.590	3497	3499	3503	rVB2	322	201	0.01%	0.002%
95	12.623	3507	3509	3511	rBV	160	96	0.01%	0.001%
96	13.002	3621	3627	3634	rVB4	1721	2468	0.18%	0.024%
97	13.227	3690	3697	3705	rVB3	4470	6314	0.46%	0.061%
98	13.848	3880	3890	3900	rVB2	9860	14735	1.08%	0.143%
99	14.092	3956	3966	3979	rBV	29814	50224	3.68%	0.488%
100	14.333	4034	4041	4053	rVB2	12963	19788	1.45%	0.192%




Sum of corrected areas: 10289795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045199.D
Acq On : 07 Oct 2021 10:09
Operator : SY/MD
Sample : VU1007MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

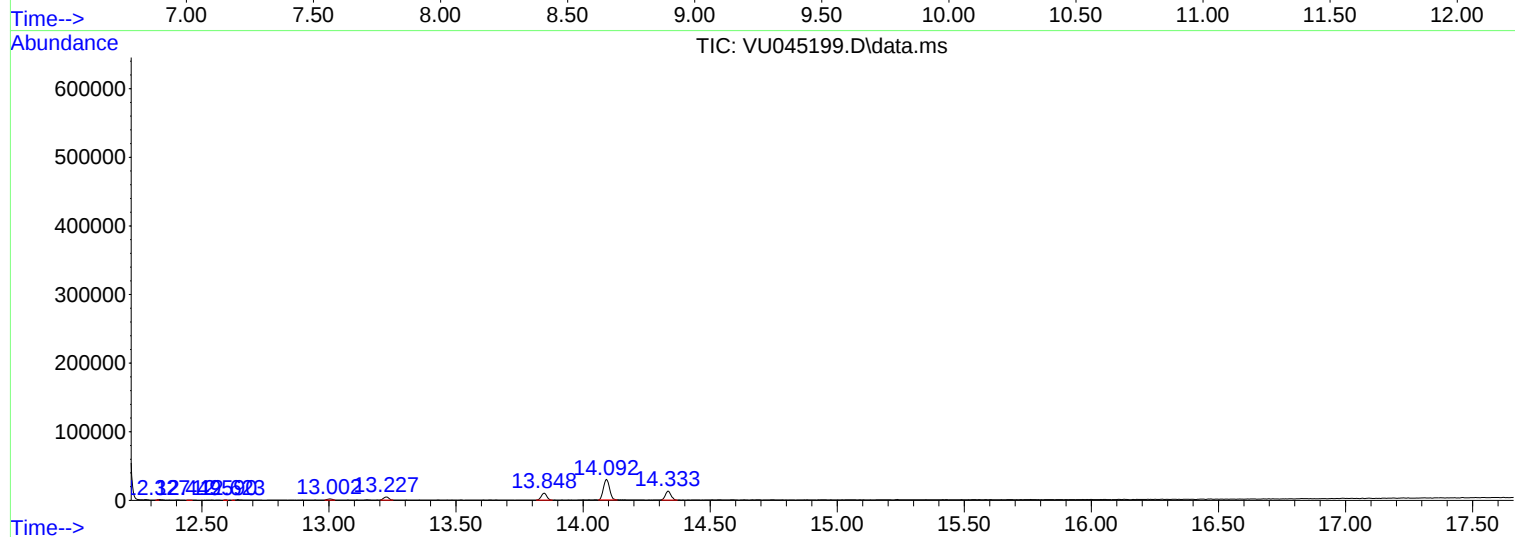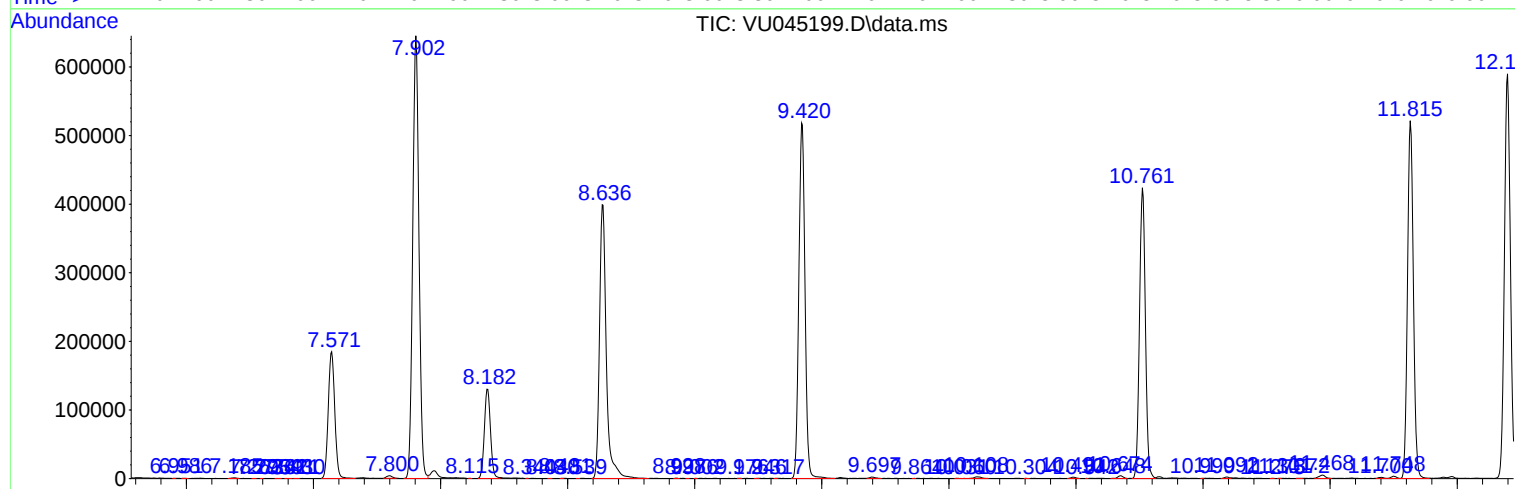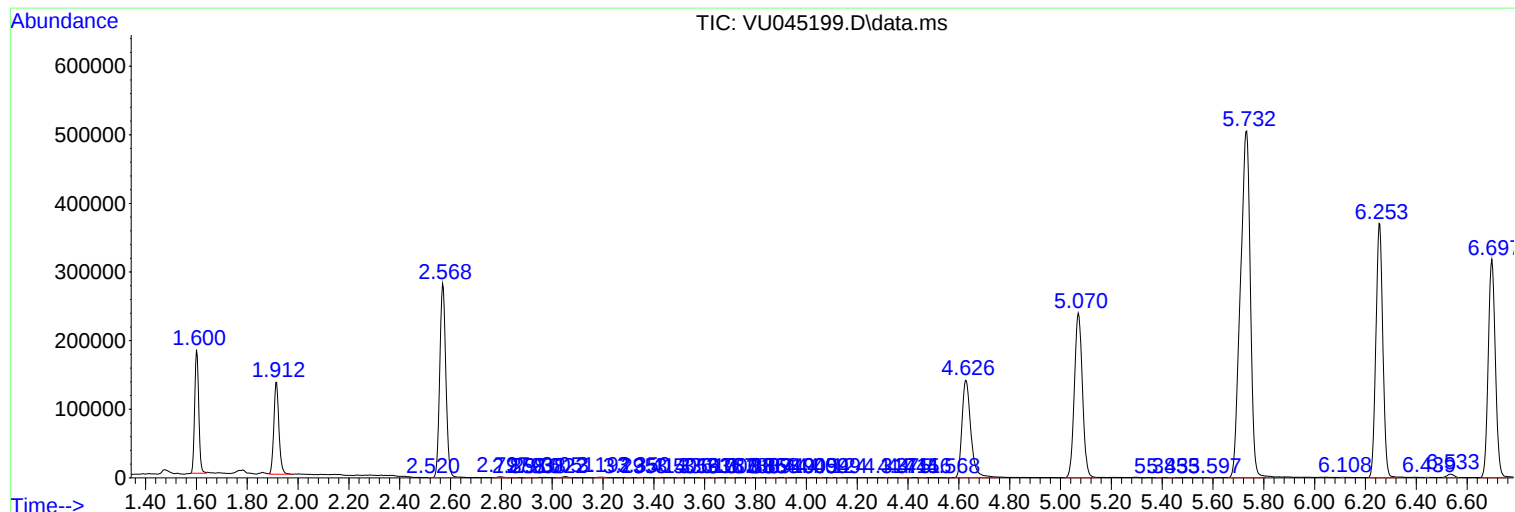

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045199.D
Acq On : 07 Oct 2021 10:09
Operator : SY/MD
Sample : VU1007MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045199.D
Acq On : 07 Oct 2021 10:09
Operator : SY/MD
Sample : VU1007MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc