

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045201.D
 Acq On : 07 Oct 2021 10:56
 Operator : SY/MD
 Sample : M4023-11 250X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	185937	202953	8.40%	1.480%
2	1.900	167	174	193	rVB	132627	183769	7.61%	1.340%
3	2.568	368	382	400	rBV3	323734	615680	25.49%	4.490%
4	2.787	441	450	451	rBV2	756	890	0.04%	0.006%
5	2.864	471	474	482	rVB	153	185	0.01%	0.001%
6	2.916	487	490	494	rBV	233	174	0.01%	0.001%
7	2.993	511	514	517	rBV	236	170	0.01%	0.001%
8	3.047	517	531	556	rBV	439595	849140	35.16%	6.192%
9	3.301	608	610	612	rBV2	153	103	0.00%	0.001%
10	3.353	620	626	627	rBV2	818	726	0.03%	0.005%
11	3.501	668	672	674	rBV	200	150	0.01%	0.001%
12	3.517	674	677	681	rBV2	208	179	0.01%	0.001%
13	3.607	702	705	708	rBV2	135	132	0.01%	0.001%
14	3.684	725	729	733	rVV2	217	202	0.01%	0.001%
15	3.742	745	747	749	rBV	150	105	0.00%	0.001%
16	3.774	754	757	760	rBV	159	129	0.01%	0.001%
17	3.874	773	788	808	rVB2	19018	42525	1.76%	0.310%
18	3.948	808	811	814	rVB2	198	114	0.00%	0.001%
19	3.993	820	825	828	rBV2	173	145	0.01%	0.001%
20	4.028	834	836	839	rBV2	192	113	0.00%	0.001%
21	4.067	844	848	850	rBV2	181	182	0.01%	0.001%
22	4.163	874	878	883	rBV2	178	257	0.01%	0.002%
23	4.227	895	898	900	rBV	189	126	0.01%	0.001%
24	4.276	911	913	916	rVB2	168	95	0.00%	0.001%
25	4.321	921	927	930	rBV2	186	268	0.01%	0.002%
26	4.359	936	939	944	rBV2	249	194	0.01%	0.001%
27	4.385	944	947	950	rBV	231	188	0.01%	0.001%
28	4.501	979	983	984	rBV	140	113	0.00%	0.001%
29	4.629	1008	1023	1026	rBV	147745	262189	10.86%	1.912%
30	4.951	1120	1123	1126	rVB2	175	96	0.00%	0.001%
31	5.070	1140	1160	1180	rBV	223298	493317	20.43%	3.598%
32	5.215	1200	1205	1210	rVB3	500	603	0.02%	0.004%
33	5.321	1220	1238	1261	rBV	268155	603212	24.98%	4.399%
34	5.440	1272	1275	1277	rBV	150	116	0.00%	0.001%
35	5.649	1338	1340	1343	rBV	208	157	0.01%	0.001%
36	5.729	1343	1365	1384	rBV2	477227	1277939	52.92%	9.319%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045201.D
 Acq On : 07 Oct 2021 10:56
 Operator : SY/MD
 Sample : M4023-11 250X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.169	1499	1502	1508	rVB3	304	352	0.01%	0.003%
38	6.253	1508	1528	1548	rBV	374339	703181	29.12%	5.128%
39	6.436	1582	1585	1590	rBV2	249	231	0.01%	0.002%
40	6.462	1590	1593	1595	rBV2	278	191	0.01%	0.001%
41	6.546	1603	1619	1651	rBV	1302973	2414912	100.00%	17.611%
42	6.694	1653	1665	1689	rVB	297226	582384	24.12%	4.247%
43	7.108	1788	1794	1798	rBV2	195	291	0.01%	0.002%
44	7.179	1807	1816	1827	rBV4	1191	1904	0.08%	0.014%
45	7.337	1862	1865	1868	rBV2	209	193	0.01%	0.001%
46	7.568	1924	1937	1953	rBV	163389	280885	11.63%	2.048%
47	7.694	1969	1976	1982	rVB4	677	1051	0.04%	0.008%
48	7.800	2000	2009	2015	rBV3	989	1603	0.07%	0.012%
49	7.903	2026	2041	2055	rBV	586864	1000434	41.43%	7.296%
50	8.182	2116	2128	2144	rBV	115939	189045	7.83%	1.379%
51	8.356	2179	2182	2186	rBV2	185	138	0.01%	0.001%
52	8.404	2189	2197	2205	rVV3	5290	8254	0.34%	0.060%
53	8.472	2215	2218	2221	rBV2	234	150	0.01%	0.001%
54	8.488	2221	2223	2225	rBV3	214	110	0.00%	0.001%
55	8.530	2233	2236	2238	rBV2	180	131	0.01%	0.001%
56	8.636	2256	2269	2306	rBV	433024	742305	30.74%	5.413%
57	8.886	2345	2347	2351	rBV	133	105	0.00%	0.001%
58	8.960	2366	2370	2374	rVB2	183	185	0.01%	0.001%
59	9.044	2391	2396	2401	rVB	194	234	0.01%	0.002%
60	9.070	2401	2404	2407	rBV	178	136	0.01%	0.001%
61	9.108	2412	2416	2418	rBV	190	98	0.00%	0.001%
62	9.124	2418	2421	2426	rBV	182	197	0.01%	0.001%
63	9.214	2446	2449	2451	rBV2	173	114	0.00%	0.001%
64	9.279	2466	2469	2471	rBV2	173	134	0.01%	0.001%
65	9.327	2479	2484	2486	rBV2	266	274	0.01%	0.002%
66	9.420	2500	2513	2531	rBV	533527	865032	35.82%	6.308%
67	9.575	2556	2561	2570	rVB3	3541	4567	0.19%	0.033%
68	9.616	2570	2574	2578	rVB2	230	179	0.01%	0.001%
69	9.639	2578	2581	2583	rBV2	183	118	0.00%	0.001%
70	9.693	2589	2598	2609	rBV2	13592	21227	0.88%	0.155%
71	9.803	2629	2632	2637	rBV2	215	173	0.01%	0.001%
72	9.864	2648	2651	2652	rBV	156	94	0.00%	0.001%
73	9.906	2662	2664	2669	rVB2	163	157	0.01%	0.001%
74	10.002	2691	2694	2701	rVB2	185	146	0.01%	0.001%
75	10.038	2701	2705	2709	rBV	171	203	0.01%	0.001%
76	10.105	2716	2726	2736	rVB	6491	9663	0.40%	0.070%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045201.D
 Acq On : 07 Oct 2021 10:56
 Operator : SY/MD
 Sample : M4023-11 250X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.173	2745	2747	2749	rBV	161	96	0.00%	0.001%
78	10.388	2810	2814	2817	rBV	152	145	0.01%	0.001%
79	10.623	2884	2887	2889	rBV	178	116	0.00%	0.001%
80	10.655	2894	2897	2898	rBV	448	267	0.01%	0.002%
81	10.674	2898	2903	2910	rVB3	1915	2516	0.10%	0.018%
82	10.761	2917	2930	2952	rVB	422238	677906	28.07%	4.944%
83	10.870	2960	2964	2968	rVB2	348	241	0.01%	0.002%
84	10.928	2979	2982	2986	rVB2	278	192	0.01%	0.001%
85	11.079	3025	3029	3031	rBV	212	212	0.01%	0.002%
86	11.124	3039	3043	3047	rBV2	541	479	0.02%	0.003%
87	11.250	3079	3082	3086	rVV	237	180	0.01%	0.001%
88	11.279	3088	3091	3096	rVB2	207	175	0.01%	0.001%
89	11.465	3139	3149	3158	rBV4	1923	3478	0.14%	0.025%
90	11.700	3216	3222	3226	rVB3	1013	1192	0.05%	0.009%
91	11.735	3231	3233	3235	rBV2	193	106	0.00%	0.001%
92	11.816	3245	3258	3274	rBV	504716	786840	32.58%	5.738%
93	12.031	3322	3325	3327	rBV	244	174	0.01%	0.001%
94	12.195	3364	3376	3397	rVB	542045	863479	35.76%	6.297%
95	12.346	3421	3423	3428	rVB	281	123	0.01%	0.001%
96	12.574	3490	3494	3499	rVB2	281	269	0.01%	0.002%
97	13.224	3692	3696	3700	rBV2	500	548	0.02%	0.004%
98	13.844	3885	3889	3896	rVB3	1236	1325	0.05%	0.010%
99	14.092	3962	3966	3973	rVB3	2611	3287	0.14%	0.024%
100	14.333	4036	4041	4049	rBV4	1260	1822	0.08%	0.013%




Sum of corrected areas: 13712585

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045201.D
Acq On : 07 Oct 2021 10:56
Operator : SY/MD
Sample : M4023-11 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

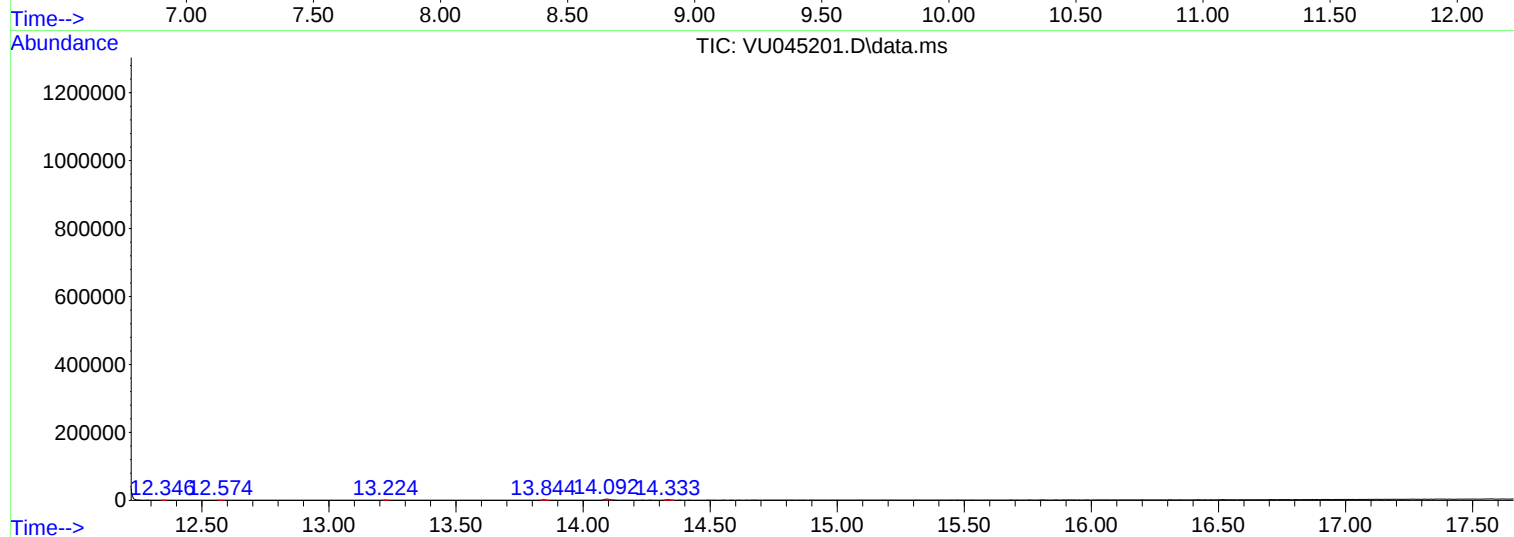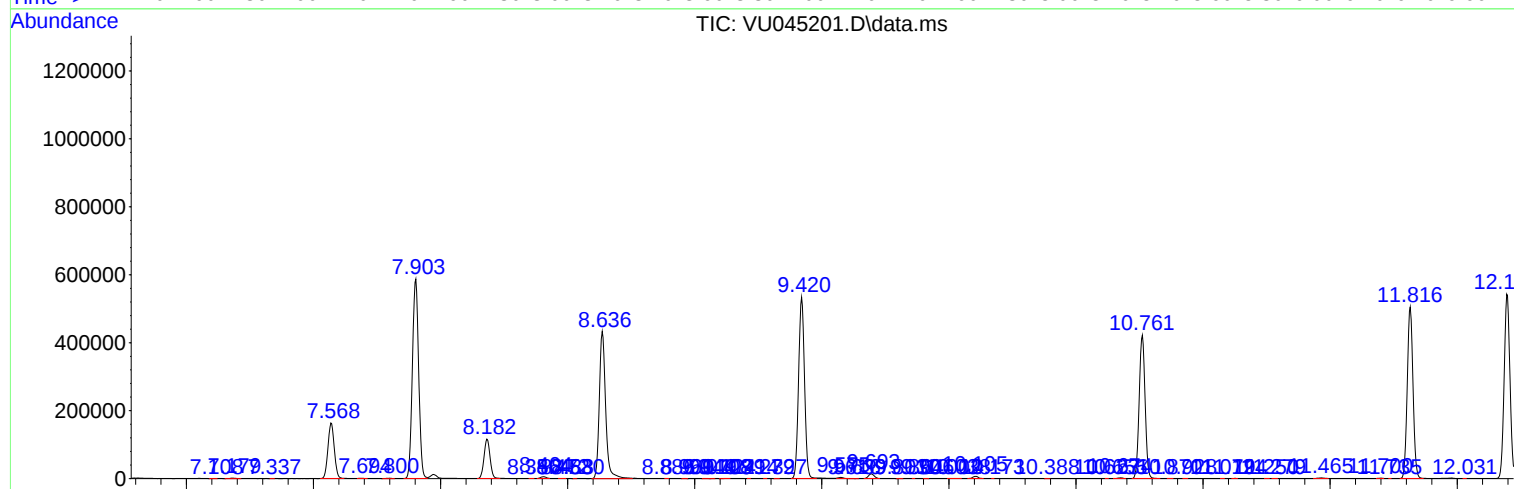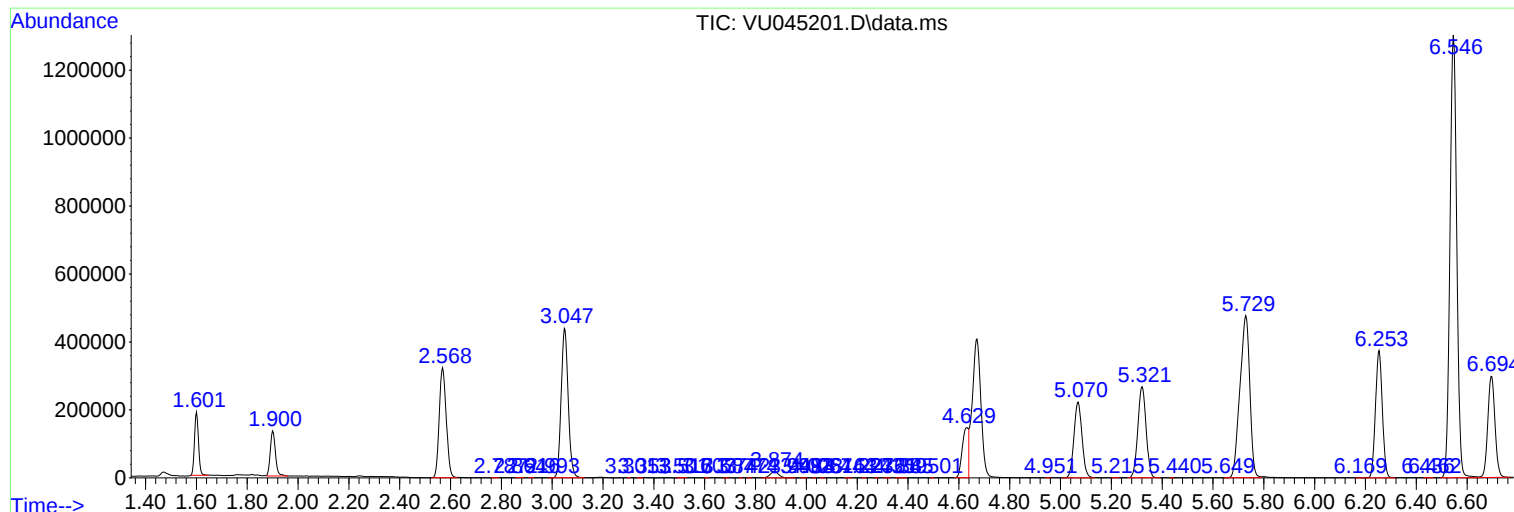

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045201.D
Acq On : 07 Oct 2021 10:56
Operator : SY/MD
Sample : M4023-11 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045201.D
Acq On : 07 Oct 2021 10:56
Operator : SY/MD
Sample : M4023-11 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
