

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045203.D
 Acq On : 07 Oct 2021 11:43
 Operator : SY/MD
 Sample : M4023-13 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	62	rVB	13104	27639	2.09%	0.239%
2	1.601	73	81	94	rBV	193368	207664	15.73%	1.792%
3	1.897	164	173	186	rVB	136016	183590	13.91%	1.584%
4	2.565	368	381	400	rBV2	290345	516188	39.11%	4.455%
5	2.729	426	432	435	rBV2	310	322	0.02%	0.003%
6	2.784	440	449	458	rVB3	771	1585	0.12%	0.014%
7	2.823	458	461	464	rBV2	235	219	0.02%	0.002%
8	2.893	477	483	488	rBV	205	285	0.02%	0.002%
9	2.954	494	502	506	rBV3	517	667	0.05%	0.006%
10	3.048	518	531	548	rVV2	24393	45592	3.45%	0.393%
11	3.196	562	577	587	rBV3	1739	4155	0.31%	0.036%
12	3.353	614	626	640	rVB2	25360	49218	3.73%	0.425%
13	3.472	661	663	669	rVB	147	167	0.01%	0.001%
14	3.591	697	700	705	rBV	213	232	0.02%	0.002%
15	3.874	774	788	805	rBV3	9189	21317	1.61%	0.184%
16	3.993	820	825	831	rBV2	233	347	0.03%	0.003%
17	4.077	848	851	856	rVB	194	169	0.01%	0.001%
18	4.263	905	909	914	rBV2	180	237	0.02%	0.002%
19	4.633	1006	1024	1025	rBV	152135	239244	18.12%	2.065%
20	4.874	1095	1099	1103	rVB4	366	274	0.02%	0.002%
21	4.961	1122	1126	1130	rVB2	254	198	0.02%	0.002%
22	5.067	1142	1159	1183	rBV	233328	510185	38.65%	4.403%
23	5.321	1221	1238	1260	rVV	131759	299788	22.71%	2.587%
24	5.456	1277	1280	1286	rVB2	220	257	0.02%	0.002%
25	5.494	1286	1292	1295	rBV2	224	263	0.02%	0.002%
26	5.575	1314	1317	1320	rBV2	176	184	0.01%	0.002%
27	5.617	1327	1330	1333	rVB2	204	160	0.01%	0.001%
28	5.639	1333	1337	1341	rBV	210	155	0.01%	0.001%
29	5.729	1342	1365	1385	rBV2	495817	1319980	100.00%	11.392%
30	5.945	1429	1432	1439	rBV2	186	214	0.02%	0.002%
31	6.035	1458	1460	1463	rBV2	228	163	0.01%	0.001%
32	6.109	1478	1483	1485	rBV2	319	321	0.02%	0.003%
33	6.144	1491	1494	1496	rBV2	264	236	0.02%	0.002%
34	6.173	1501	1503	1508	rVB2	311	186	0.01%	0.002%
35	6.253	1511	1528	1546	rBV	390321	726610	55.05%	6.271%
36	6.546	1604	1619	1651	rBV	628991	1167249	88.43%	10.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045203.D
 Acq On : 07 Oct 2021 11:43
 Operator : SY/MD
 Sample : M4023-13 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.694	1651	1665	1695	rVB	308186	603960	45.76%	5.212%
38	6.803	1695	1699	1701	rBV3	708	595	0.05%	0.005%
39	6.883	1721	1724	1730	rVB2	322	231	0.02%	0.002%
40	7.051	1764	1776	1782	rBV3	655	1199	0.09%	0.010%
41	7.186	1807	1818	1826	rVV5	1283	2186	0.17%	0.019%
42	7.266	1838	1843	1847	rVV	159	212	0.02%	0.002%
43	7.498	1907	1915	1919	rVB2	241	334	0.03%	0.003%
44	7.568	1919	1937	1955	rBV	166901	286297	21.69%	2.471%
45	7.691	1967	1975	1984	rVB4	916	1436	0.11%	0.012%
46	7.903	2025	2041	2055	rBV	614519	1046680	79.30%	9.033%
47	7.973	2056	2063	2079	rVB	9208	15835	1.20%	0.137%
48	8.125	2106	2110	2115	rBV2	259	274	0.02%	0.002%
49	8.182	2115	2128	2143	rBV	117159	191227	14.49%	1.650%
50	8.298	2161	2164	2171	rVB2	335	398	0.03%	0.003%
51	8.340	2171	2177	2180	rBV2	234	197	0.01%	0.002%
52	8.404	2190	2197	2209	rVB3	2562	4190	0.32%	0.036%
53	8.543	2233	2240	2244	rBV	248	195	0.01%	0.002%
54	8.575	2245	2250	2253	rBV2	179	179	0.01%	0.002%
55	8.636	2257	2269	2304	rBV	433082	756331	57.30%	6.527%
56	8.861	2337	2339	2343	rVB2	273	152	0.01%	0.001%
57	8.935	2357	2362	2365	rBV2	177	214	0.02%	0.002%
58	9.092	2405	2411	2415	rBV2	170	191	0.01%	0.002%
59	9.266	2461	2465	2469	rBV2	191	212	0.02%	0.002%
60	9.292	2469	2473	2476	rVB3	333	259	0.02%	0.002%
61	9.420	2499	2513	2548	rBV	550477	907809	68.77%	7.834%
62	9.578	2554	2562	2568	rVB3	582	1017	0.08%	0.009%
63	9.616	2569	2574	2577	rBV	251	252	0.02%	0.002%
64	9.655	2582	2586	2592	rBV2	170	227	0.02%	0.002%
65	9.697	2592	2599	2608	rVB3	1454	2218	0.17%	0.019%
66	9.842	2642	2644	2647	rBV	245	187	0.01%	0.002%
67	9.870	2649	2653	2658	rVV2	178	189	0.01%	0.002%
68	9.967	2679	2683	2685	rBV	175	159	0.01%	0.001%
69	10.018	2696	2699	2705	rVB2	181	239	0.02%	0.002%
70	10.063	2710	2713	2718	rVV2	184	178	0.01%	0.002%
71	10.105	2718	2726	2733	rVV2	1241	1697	0.13%	0.015%
72	10.243	2765	2769	2775	rBV2	388	590	0.04%	0.005%
73	10.600	2877	2880	2886	rBV2	213	196	0.01%	0.002%
74	10.636	2888	2891	2896	rVB2	243	241	0.02%	0.002%
75	10.671	2896	2902	2910	rBV4	2033	2881	0.22%	0.025%
76	10.713	2910	2915	2917	rBV2	176	163	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045203.D
 Acq On : 07 Oct 2021 11:43
 Operator : SY/MD
 Sample : M4023-13 40X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	10.761	2917	2930	2951	rVV	441804	702684	53.23%	6.064%
78	10.989	2998	3001	3003	rBV	241	187	0.01%	0.002%
79	11.006	3003	3006	3011	rVB2	281	267	0.02%	0.002%
80	11.092	3029	3033	3036	rVB	216	176	0.01%	0.002%
81	11.115	3037	3040	3044	rBV2	216	190	0.01%	0.002%
82	11.465	3143	3149	3158	rVB4	1444	2539	0.19%	0.022%
83	11.546	3171	3174	3178	rVV2	166	175	0.01%	0.002%
84	11.575	3180	3183	3186	rVV2	246	172	0.01%	0.001%
85	11.700	3218	3222	3227	rVB3	695	696	0.05%	0.006%
86	11.816	3245	3258	3275	rBV	519498	821539	62.24%	7.090%
87	11.941	3290	3297	3300	rBV4	588	569	0.04%	0.005%
88	11.977	3301	3308	3320	rVB4	1208	1848	0.14%	0.016%
89	12.041	3325	3328	3331	rBV	185	169	0.01%	0.001%
90	12.195	3363	3376	3397	rVV	554383	897318	67.98%	7.744%
91	12.861	3579	3583	3586	rBV2	416	327	0.02%	0.003%
92	13.002	3623	3627	3631	rBV2	200	224	0.02%	0.002%
93	13.121	3660	3664	3666	rBV	236	190	0.01%	0.002%
94	13.349	3730	3735	3737	rBV	165	170	0.01%	0.001%
95	13.822	3879	3882	3884	rBV	210	170	0.01%	0.001%
96	14.092	3963	3966	3968	rBV	572	433	0.03%	0.004%
97	14.398	4058	4061	4063	rBV	251	154	0.01%	0.001%
98	14.632	4131	4134	4135	rBV2	379	211	0.02%	0.002%
99	14.787	4180	4182	4184	rBV2	303	210	0.02%	0.002%
100	14.986	4242	4244	4248	rBV2	276	246	0.02%	0.002%




Sum of corrected areas: 11587351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045203.D
Acq On : 07 Oct 2021 11:43
Operator : SY/MD
Sample : M4023-13 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

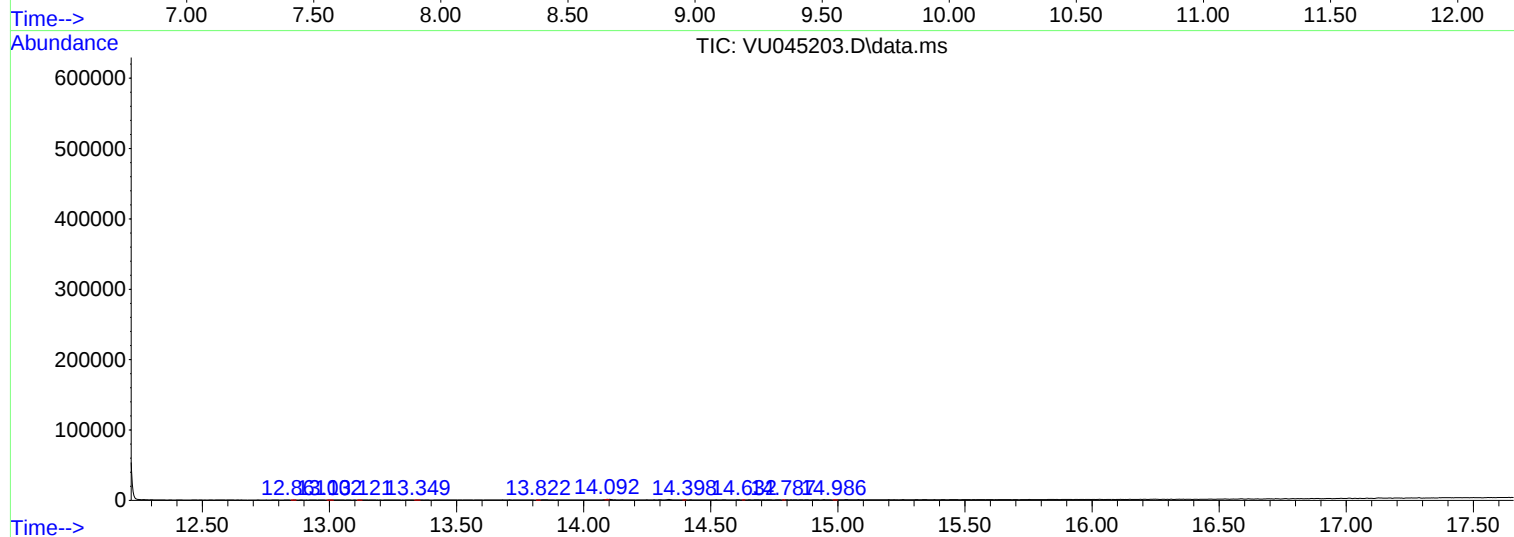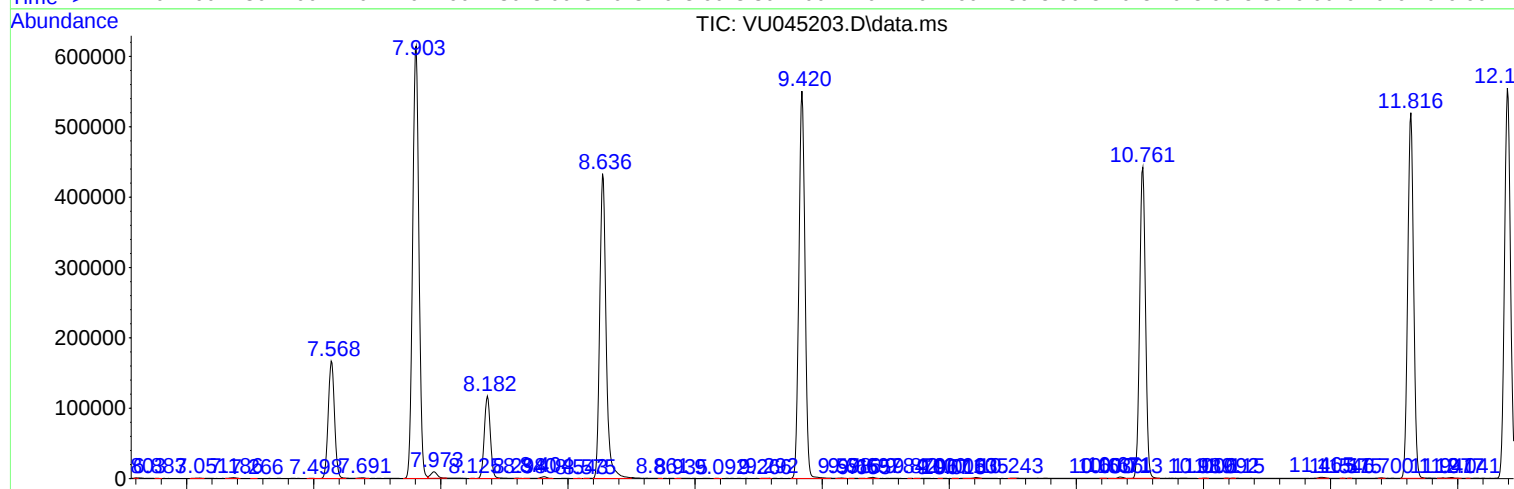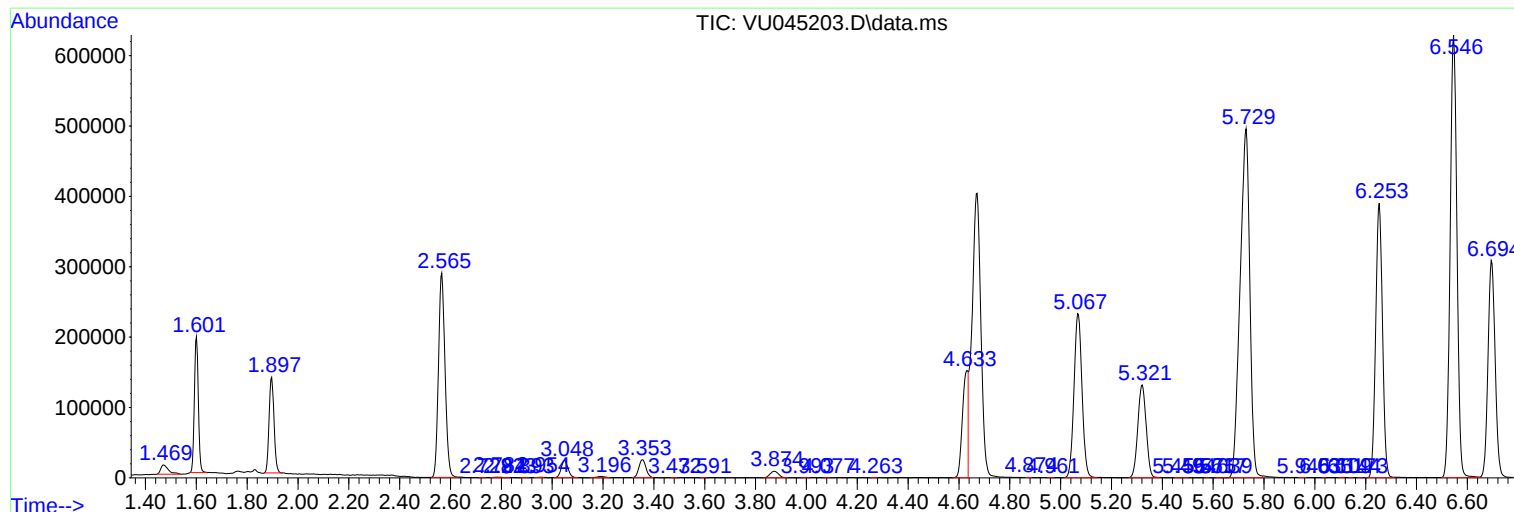

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045203.D
Acq On : 07 Oct 2021 11:43
Operator : SY/MD
Sample : M4023-13 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045203.D
Acq On : 07 Oct 2021 11:43
Operator : SY/MD
Sample : M4023-13 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
