

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045204.D
 Acq On : 07 Oct 2021 12:07
 Operator : SY/MD
 Sample : M4025-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045204.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	52	rBV	12995	22586	1.11%	0.187%
2	1.600	74	81	96	rVB	190278	207605	10.16%	1.716%
3	1.896	164	173	195	rVB	132692	183733	8.99%	1.518%
4	2.565	368	381	399	rBV3	313035	590983	28.92%	4.884%
5	2.774	437	446	458	rVV3	2094	4313	0.21%	0.036%
6	2.845	464	468	471	rBV2	178	195	0.01%	0.002%
7	2.877	475	478	480	rBV	208	133	0.01%	0.001%
8	2.954	497	502	503	rBV	409	339	0.02%	0.003%
9	3.047	522	531	540	rBV3	895	1490	0.07%	0.012%
10	3.189	563	575	590	rVV	4133	9045	0.44%	0.075%
11	3.292	602	607	608	rBV2	156	138	0.01%	0.001%
12	3.356	618	627	634	rBV4	1303	2100	0.10%	0.017%
13	3.723	737	741	744	rBV	229	169	0.01%	0.001%
14	3.874	774	788	805	rVB3	6805	15435	0.76%	0.128%
15	4.089	849	855	859	rBV2	198	255	0.01%	0.002%
16	4.176	875	882	884	rBV	170	181	0.01%	0.001%
17	4.311	921	924	927	rBV2	159	141	0.01%	0.001%
18	4.359	936	939	943	rBV2	169	146	0.01%	0.001%
19	4.385	943	947	951	rBV2	190	221	0.01%	0.002%
20	4.420	955	958	964	rVB2	197	250	0.01%	0.002%
21	4.481	972	977	980	rBV2	175	173	0.01%	0.001%
22	4.552	995	999	1002	rBV	139	142	0.01%	0.001%
23	4.629	1008	1023	1027	rBV	139145	269859	13.21%	2.230%
24	4.800	1071	1076	1079	rBV3	216	233	0.01%	0.002%
25	4.928	1111	1116	1119	rBV2	249	174	0.01%	0.001%
26	4.964	1125	1127	1130	rVB2	319	180	0.01%	0.001%
27	5.067	1143	1159	1182	rBV	225012	493784	24.17%	4.080%
28	5.208	1197	1203	1205	rBV2	380	425	0.02%	0.004%
29	5.317	1222	1237	1256	rBV2	29989	66417	3.25%	0.549%
30	5.504	1291	1295	1299	rVB2	192	154	0.01%	0.001%
31	5.604	1323	1326	1330	rVB2	212	169	0.01%	0.001%
32	5.729	1343	1365	1392	rBV2	479924	1292651	63.26%	10.682%
33	5.957	1433	1436	1438	rBV	236	167	0.01%	0.001%
34	5.999	1448	1449	1452	rBV2	232	135	0.01%	0.001%
35	6.038	1458	1461	1464	rVV2	155	157	0.01%	0.001%
36	6.108	1479	1483	1486	rVB3	286	254	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045204.D
 Acq On : 07 Oct 2021 12:07
 Operator : SY/MD
 Sample : M4025-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.128	1486	1489	1492	rBV2	282	243	0.01%	0.002%
38	6.144	1492	1494	1498	rVB2	246	156	0.01%	0.001%
39	6.173	1498	1503	1505	rBV2	346	362	0.02%	0.003%
40	6.253	1512	1528	1544	rBV	389203	732310	35.84%	6.052%
41	6.385	1567	1569	1573	rVB3	346	186	0.01%	0.002%
42	6.427	1580	1582	1585	rBV2	203	139	0.01%	0.001%
43	6.546	1603	1619	1649	rBV	1096130	2043285	100.00%	16.885%
44	6.697	1651	1666	1688	rVB	301018	587464	28.75%	4.855%
45	6.800	1694	1698	1699	rBV2	471	314	0.02%	0.003%
46	6.870	1716	1720	1724	rBV2	261	281	0.01%	0.002%
47	7.054	1769	1777	1783	rVB	463	679	0.03%	0.006%
48	7.150	1803	1807	1809	rBV2	199	154	0.01%	0.001%
49	7.163	1809	1811	1812	rBV	337	155	0.01%	0.001%
50	7.179	1812	1816	1823	rVB4	878	1131	0.06%	0.009%
51	7.247	1833	1837	1843	rVV2	401	526	0.03%	0.004%
52	7.568	1924	1937	1954	rBV	168660	288581	14.12%	2.385%
53	7.684	1966	1973	1975	rBV3	775	776	0.04%	0.006%
54	7.828	2014	2018	2019	rBV	211	170	0.01%	0.001%
55	7.902	2025	2041	2056	rBV	604909	1026435	50.23%	8.482%
56	7.973	2056	2063	2073	rVB	8751	14081	0.69%	0.116%
57	8.073	2092	2094	2096	rBV	220	144	0.01%	0.001%
58	8.182	2115	2128	2146	rBV	118134	192240	9.41%	1.589%
59	8.401	2190	2196	2204	rBV2	1794	2684	0.13%	0.022%
60	8.504	2224	2228	2237	rBV2	193	361	0.02%	0.003%
61	8.636	2256	2269	2313	rBV	414254	725724	35.52%	5.997%
62	9.054	2397	2399	2404	rBV2	143	159	0.01%	0.001%
63	9.137	2422	2425	2428	rBV2	174	159	0.01%	0.001%
64	9.420	2500	2513	2546	rBV	561141	916234	44.84%	7.571%
65	9.571	2554	2560	2562	rBV3	352	355	0.02%	0.003%
66	9.697	2592	2599	2607	rBV5	1269	1900	0.09%	0.016%
67	9.938	2671	2674	2677	rBV2	169	134	0.01%	0.001%
68	10.028	2697	2702	2705	rBV2	254	275	0.01%	0.002%
69	10.105	2723	2726	2731	rVB3	337	325	0.02%	0.003%
70	10.205	2754	2757	2759	rBV2	241	175	0.01%	0.001%
71	10.330	2792	2796	2798	rBV2	183	176	0.01%	0.001%
72	10.516	2850	2854	2856	rBV2	274	246	0.01%	0.002%
73	10.558	2862	2867	2868	rBV	217	200	0.01%	0.002%
74	10.590	2873	2877	2880	rBV2	201	151	0.01%	0.001%
75	10.674	2894	2903	2910	rVB2	2368	3031	0.15%	0.025%
76	10.761	2917	2930	2953	rVB	431119	687338	33.64%	5.680%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045204.D
 Acq On : 07 Oct 2021 12:07
 Operator : SY/MD
 Sample : M4025-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.092	3028	3033	3034	rBV	217	149	0.01%	0.001%
78	11.121	3038	3042	3047	rVV3	372	324	0.02%	0.003%
79	11.205	3064	3068	3070	rBV2	214	172	0.01%	0.001%
80	11.369	3116	3119	3124	rBV	297	362	0.02%	0.003%
81	11.462	3141	3148	3157	rVB6	1781	3045	0.15%	0.025%
82	11.504	3157	3161	3163	rBV	174	154	0.01%	0.001%
83	11.623	3195	3198	3199	rBV2	248	139	0.01%	0.001%
84	11.639	3199	3203	3209	rVB3	1022	1085	0.05%	0.009%
85	11.697	3216	3221	3229	rVB5	870	1302	0.06%	0.011%
86	11.738	3230	3234	3237	rBV2	172	187	0.01%	0.002%
87	11.815	3245	3258	3283	rBV	520455	819297	40.10%	6.770%
88	11.941	3293	3297	3303	rBV4	513	711	0.03%	0.006%
89	11.976	3303	3308	3316	rVB4	1525	1838	0.09%	0.015%
90	12.047	3327	3330	3333	rBV2	218	198	0.01%	0.002%
91	12.076	3336	3339	3343	rVB3	179	165	0.01%	0.001%
92	12.114	3348	3351	3353	rBV	249	197	0.01%	0.002%
93	12.195	3362	3376	3400	rBV	545364	876007	42.87%	7.239%
94	12.333	3416	3419	3421	rBV2	371	239	0.01%	0.002%
95	12.523	3472	3478	3479	rBV	208	230	0.01%	0.002%
96	12.635	3509	3513	3514	rBV	265	187	0.01%	0.002%
97	13.777	3864	3868	3872	rVB	276	252	0.01%	0.002%
98	13.799	3872	3875	3877	rBV	176	145	0.01%	0.001%
99	13.954	3919	3923	3931	rBV2	420	672	0.03%	0.006%
100	14.249	4013	4015	4019	rBV2	232	170	0.01%	0.001%




Sum of corrected areas: 12101198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045204.D
Acq On : 07 Oct 2021 12:07
Operator : SY/MD
Sample : M4025-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

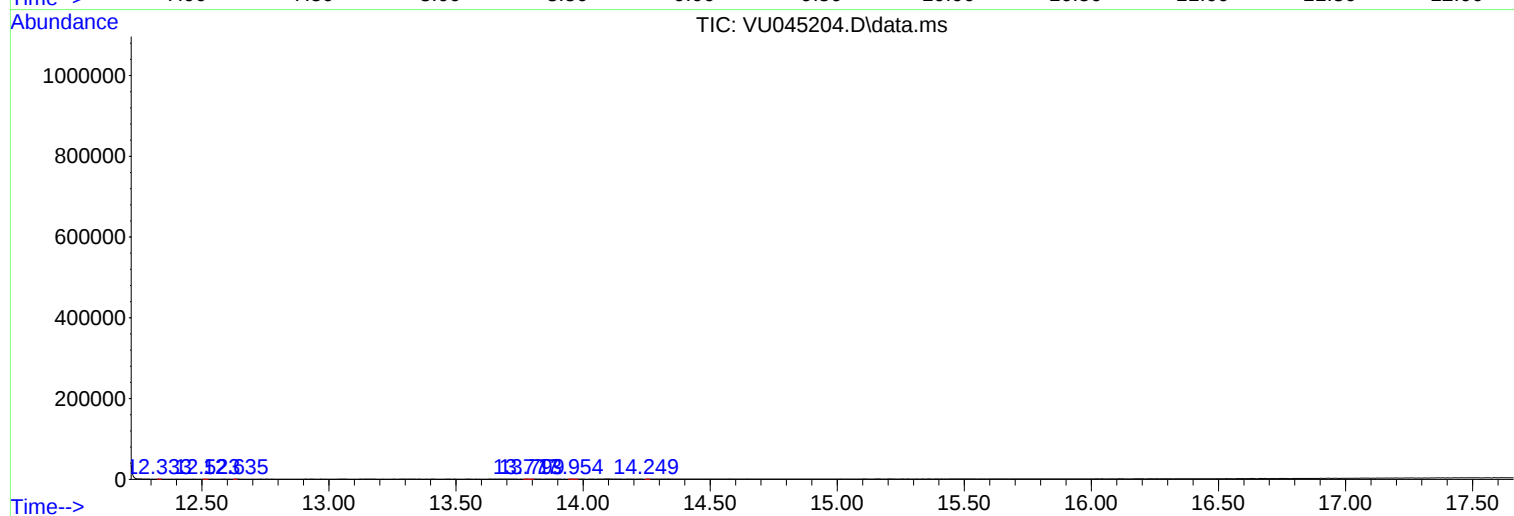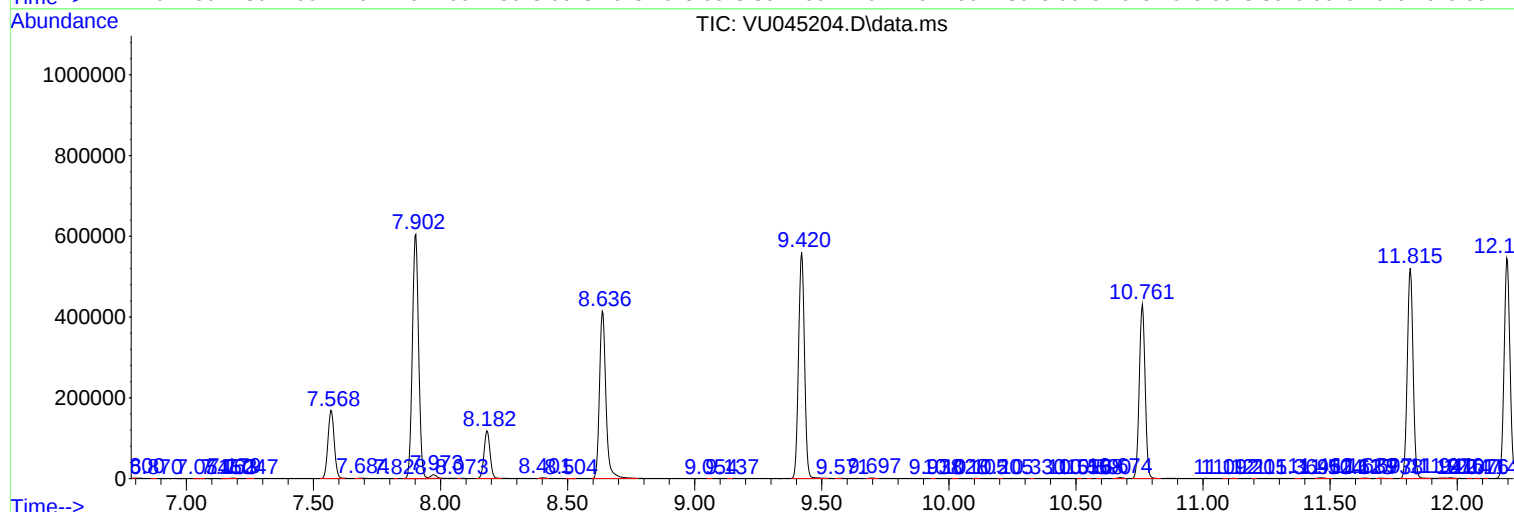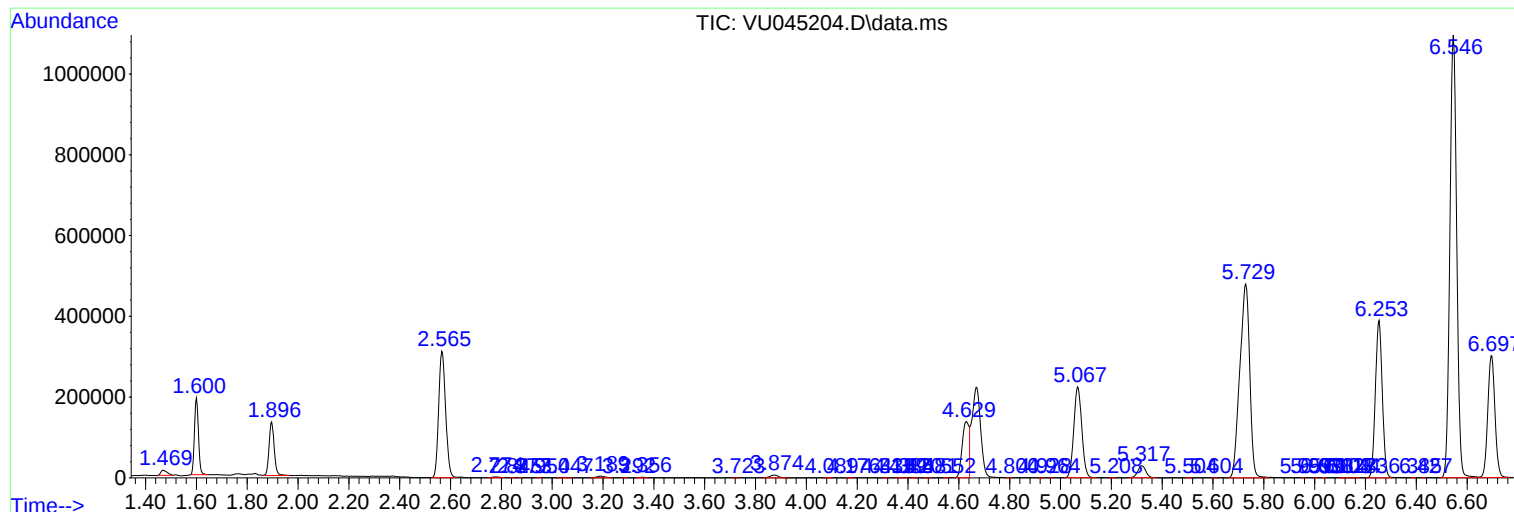

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045204.D
Acq On : 07 Oct 2021 12:07
Operator : SY/MD
Sample : M4025-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045204.D
Acq On : 07 Oct 2021 12:07
Operator : SY/MD
Sample : M4025-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
