

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045206.D
 Acq On : 07 Oct 2021 12:55
 Operator : SY/MD
 Sample : M4025-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045206.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	54	rBV	15039	28659	2.23%	0.294%
2	1.600	74	81	91	rVB	178545	191599	14.93%	1.966%
3	1.899	166	174	194	rVB	132536	182424	14.21%	1.872%
4	2.497	356	360	362	rBV	326	239	0.02%	0.002%
5	2.565	368	381	398	rBV	260684	437180	34.07%	4.486%
6	2.774	435	446	466	rBV	3804	7767	0.61%	0.080%
7	2.954	498	502	506	rBV	305	354	0.03%	0.004%
8	3.041	525	529	531	rBV3	483	371	0.03%	0.004%
9	3.115	548	552	554	rBV	197	185	0.01%	0.002%
10	3.144	558	561	564	rVV2	207	198	0.02%	0.002%
11	3.192	564	576	590	rVB3	7081	15683	1.22%	0.161%
12	3.349	620	625	629	rBV2	209	200	0.02%	0.002%
13	3.562	689	691	695	rBV	195	167	0.01%	0.002%
14	3.636	712	714	720	rVB	221	216	0.02%	0.002%
15	3.800	761	765	768	rBV	198	222	0.02%	0.002%
16	4.192	885	887	892	rBV2	184	175	0.01%	0.002%
17	4.430	957	961	965	rVB2	270	247	0.02%	0.003%
18	4.456	965	969	972	rBV	246	265	0.02%	0.003%
19	4.552	994	999	1002	rBV2	171	180	0.01%	0.002%
20	4.629	1007	1023	1051	rBV	140515	330698	25.77%	3.394%
21	4.947	1120	1122	1125	rVB	284	162	0.01%	0.002%
22	4.967	1126	1128	1132	rBV2	247	172	0.01%	0.002%
23	5.066	1140	1159	1184	rBV	228436	496684	38.70%	5.097%
24	5.218	1204	1206	1211	rVB3	363	190	0.01%	0.002%
25	5.285	1222	1227	1228	rBV	390	281	0.02%	0.003%
26	5.375	1252	1255	1259	rVB2	270	240	0.02%	0.002%
27	5.439	1269	1275	1279	rBV	154	156	0.01%	0.002%
28	5.597	1319	1324	1327	rBV2	233	264	0.02%	0.003%
29	5.729	1342	1365	1385	rBV2	478271	1283343	100.00%	13.169%
30	6.253	1511	1528	1560	rBV	375213	706181	55.03%	7.247%
31	6.369	1560	1564	1567	rVV2	158	159	0.01%	0.002%
32	6.536	1606	1616	1627	rVB8	5039	9058	0.71%	0.093%
33	6.607	1635	1638	1642	rBV	208	188	0.01%	0.002%
34	6.697	1650	1666	1690	rBV	304355	588719	45.87%	6.041%
35	6.796	1695	1697	1698	rBV	431	210	0.02%	0.002%
36	7.047	1773	1775	1779	rVB2	306	214	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045206.D
 Acq On : 07 Oct 2021 12:55
 Operator : SY/MD
 Sample : M4025-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.131	1796	1801	1803	rBV	168	173	0.01%	0.002%
38	7.182	1811	1817	1818	rBV2	790	699	0.05%	0.007%
39	7.285	1844	1849	1851	rBV	212	181	0.01%	0.002%
40	7.407	1884	1887	1888	rBV2	411	226	0.02%	0.002%
41	7.484	1908	1911	1915	rBV	156	164	0.01%	0.002%
42	7.568	1924	1937	1959	rVV	164271	282638	22.02%	2.900%
43	7.674	1965	1970	1971	rBV2	337	231	0.02%	0.002%
44	7.687	1971	1974	1981	rVB4	683	877	0.07%	0.009%
45	7.841	2018	2022	2026	rBV2	199	246	0.02%	0.003%
46	7.902	2026	2041	2056	rBV	592725	1015311	79.11%	10.419%
47	7.973	2057	2063	2073	rVB	8550	13326	1.04%	0.137%
48	8.182	2116	2128	2149	rBV	115250	191354	14.91%	1.964%
49	8.295	2160	2163	2166	rBV2	435	286	0.02%	0.003%
50	8.404	2193	2197	2201	rVB	182	179	0.01%	0.002%
51	8.471	2213	2218	2230	rVB2	537	1076	0.08%	0.011%
52	8.536	2234	2238	2240	rBV	220	160	0.01%	0.002%
53	8.635	2257	2269	2302	rBV	413935	728920	56.80%	7.480%
54	8.896	2342	2350	2353	rBV2	179	290	0.02%	0.003%
55	9.021	2383	2389	2392	rBV	226	265	0.02%	0.003%
56	9.134	2417	2424	2432	rBV2	190	392	0.03%	0.004%
57	9.420	2500	2513	2552	rVB	536704	877614	68.38%	9.006%
58	9.574	2558	2561	2565	rVB2	321	255	0.02%	0.003%
59	9.693	2593	2598	2609	rBV2	1215	1697	0.13%	0.017%
60	9.754	2614	2617	2620	rBV2	217	156	0.01%	0.002%
61	9.777	2621	2624	2628	rBV	162	169	0.01%	0.002%
62	9.867	2647	2652	2656	rBV2	251	347	0.03%	0.004%
63	9.912	2661	2666	2671	rVV2	223	275	0.02%	0.003%
64	10.037	2702	2705	2709	rVB2	201	158	0.01%	0.002%
65	10.076	2713	2717	2720	rVB2	209	202	0.02%	0.002%
66	10.102	2720	2725	2729	rBV3	494	555	0.04%	0.006%
67	10.288	2780	2783	2787	rBV2	196	170	0.01%	0.002%
68	10.394	2811	2816	2819	rBV	245	299	0.02%	0.003%
69	10.565	2866	2869	2873	rVB	254	202	0.02%	0.002%
70	10.674	2896	2903	2911	rVB2	2079	2833	0.22%	0.029%
71	10.761	2916	2930	2952	rVB	423328	675628	52.65%	6.933%
72	10.870	2955	2964	2968	rBV3	441	679	0.05%	0.007%
73	10.896	2968	2972	2976	rVB2	483	478	0.04%	0.005%
74	10.954	2987	2990	2996	rBV2	163	179	0.01%	0.002%
75	10.999	3001	3004	3010	rVB3	294	353	0.03%	0.004%
76	11.034	3010	3015	3022	rBV2	192	318	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045206.D
 Acq On : 07 Oct 2021 12:55
 Operator : SY/MD
 Sample : M4025-20
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.124	3039	3043	3046	rVB3	315	251	0.02%	0.003%
78	11.275	3087	3090	3093	rBV	275	215	0.02%	0.002%
79	11.362	3113	3117	3124	rBV2	249	277	0.02%	0.003%
80	11.458	3140	3147	3148	rBV3	1066	983	0.08%	0.010%
81	11.635	3196	3202	3210	rBV2	673	982	0.08%	0.010%
82	11.700	3218	3222	3227	rVB2	822	730	0.06%	0.007%
83	11.719	3227	3228	3234	rVB2	254	196	0.02%	0.002%
84	11.748	3234	3237	3241	rBV2	163	159	0.01%	0.002%
85	11.815	3245	3258	3276	rBV	496994	787909	61.40%	8.085%
86	11.976	3303	3308	3314	rVB4	1239	1618	0.13%	0.017%
87	12.005	3314	3317	3322	rBV2	155	170	0.01%	0.002%
88	12.073	3334	3338	3342	rVB3	392	278	0.02%	0.003%
89	12.195	3361	3376	3396	rBV	533418	865479	67.44%	8.881%
90	12.655	3516	3519	3522	rBV2	289	172	0.01%	0.002%
91	12.741	3542	3546	3549	rBV2	222	233	0.02%	0.002%
92	12.915	3594	3600	3602	rBV2	150	168	0.01%	0.002%
93	12.963	3612	3615	3618	rBV	235	175	0.01%	0.002%
94	13.272	3704	3711	3715	rBV2	272	421	0.03%	0.004%
95	13.426	3756	3759	3762	rBV2	236	228	0.02%	0.002%
96	13.973	3925	3929	3931	rBV2	287	246	0.02%	0.003%
97	14.314	4031	4035	4036	rBV2	328	246	0.02%	0.003%
98	14.359	4046	4049	4050	rBV2	283	171	0.01%	0.002%
99	14.709	4152	4158	4161	rBV3	444	627	0.05%	0.006%
100	14.799	4183	4186	4189	rBV	297	227	0.02%	0.002%


Sum of corrected areas: 9744972

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045206.D
Acq On : 07 Oct 2021 12:55
Operator : SY/MD
Sample : M4025-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

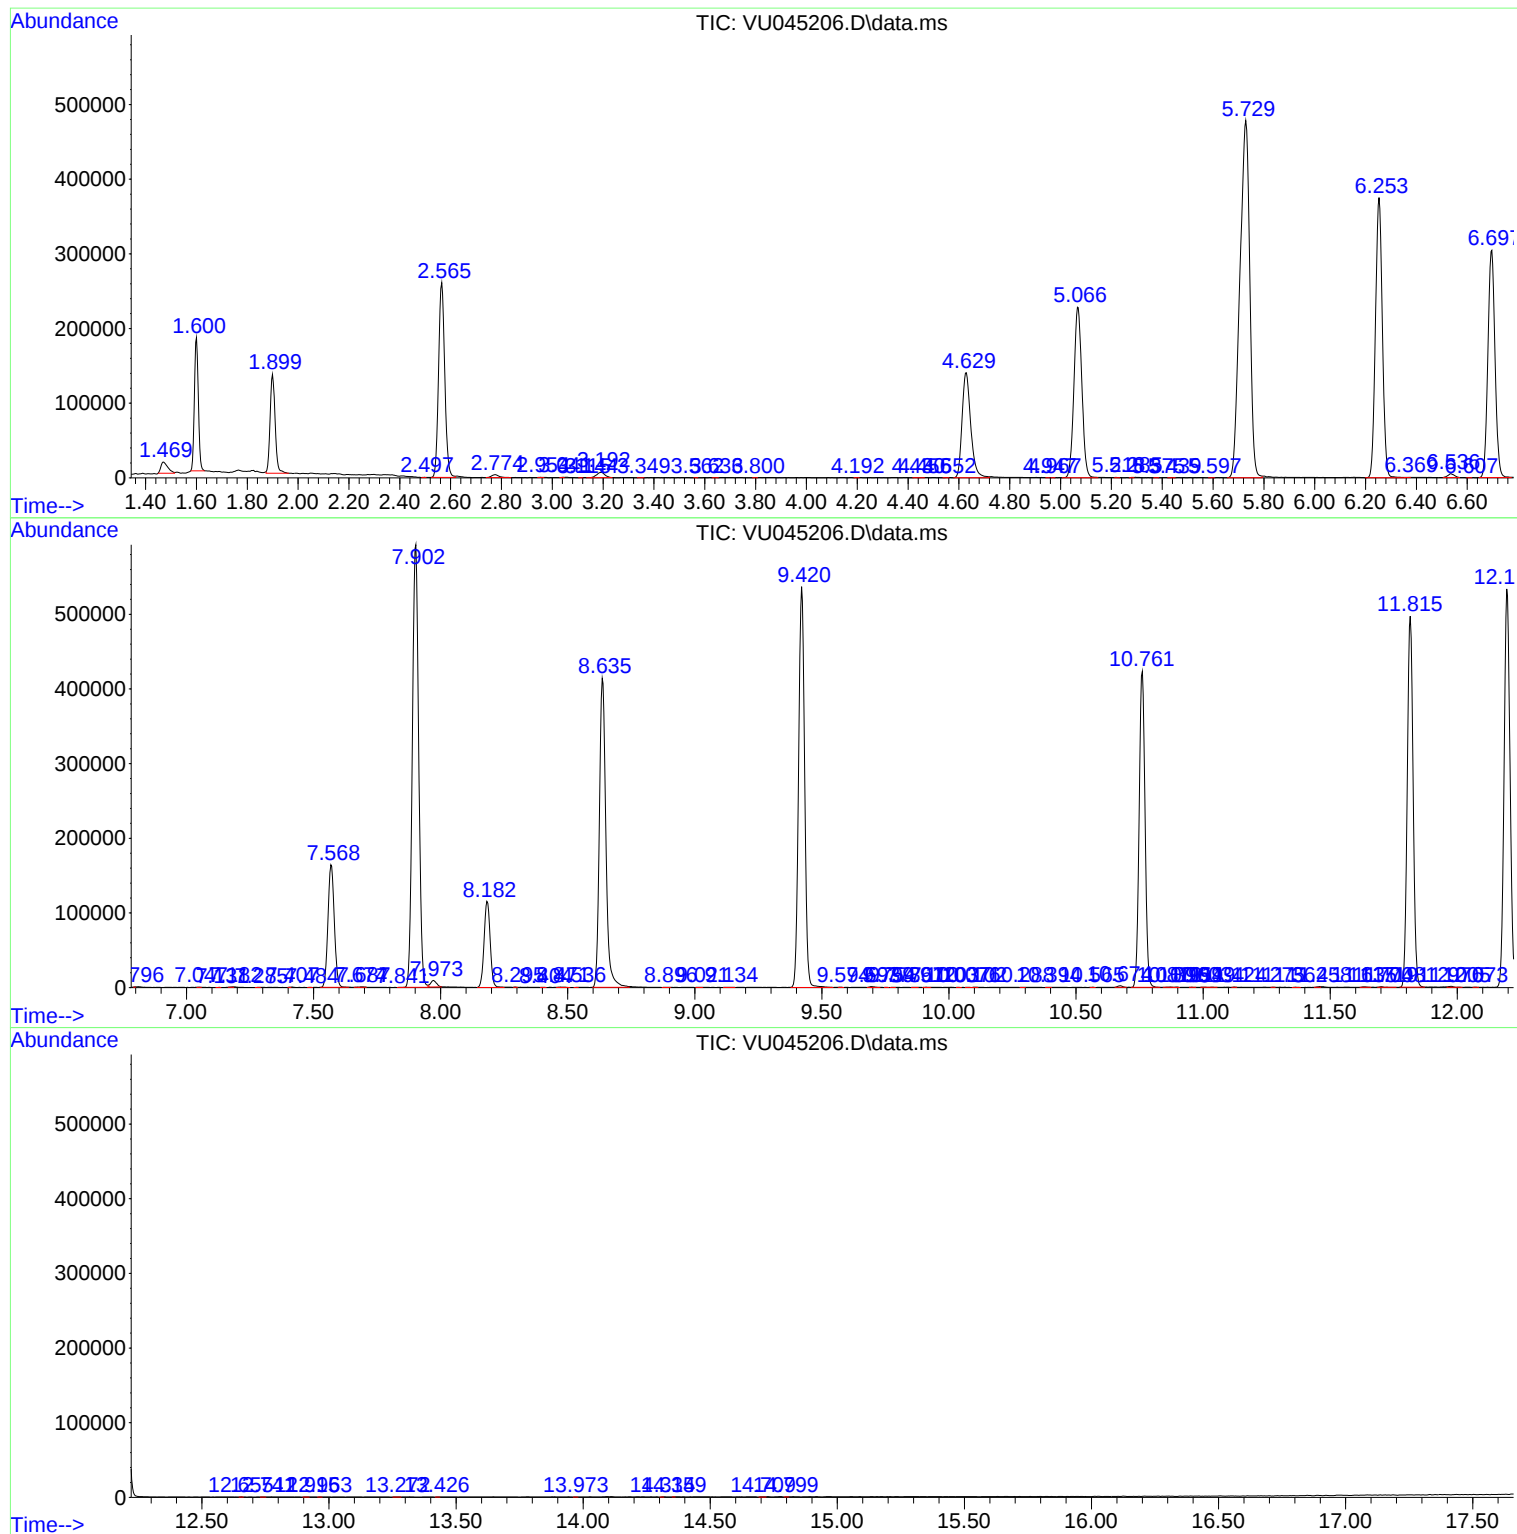

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045206.D
Acq On : 07 Oct 2021 12:55
Operator : SY/MD
Sample : M4025-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045206.D
Acq On : 07 Oct 2021 12:55
Operator : SY/MD
Sample : M4025-20
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------