

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045213.D
 Acq On : 07 Oct 2021 15:41
 Operator : SY/MD
 Sample : M4025-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

Signal : TIC: VU045213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	33	40	62	rBV	24047	48448	1.10%	0.306%
2	1.600	74	81	95	rVB	185038	195572	4.44%	1.235%
3	1.890	163	171	187	rVB	132453	179373	4.07%	1.133%
4	2.475	351	353	358	rVB2	451	348	0.01%	0.002%
5	2.565	367	381	402	rBV2	332816	650385	14.75%	4.108%
6	2.703	421	424	428	rBV	181	223	0.01%	0.001%
7	2.758	437	441	443	rBV3	239	190	0.00%	0.001%
8	2.780	445	448	452	rVV2	311	282	0.01%	0.002%
9	3.005	515	518	523	rVB2	195	186	0.00%	0.001%
10	3.147	557	562	565	rVB2	186	160	0.00%	0.001%
11	3.192	565	576	592	rVB2	2299	5157	0.12%	0.033%
12	3.353	615	626	638	rVV2	11832	21816	0.49%	0.138%
13	3.465	658	661	664	rBV2	207	191	0.00%	0.001%
14	3.546	684	686	691	rVB2	201	164	0.00%	0.001%
15	3.620	705	709	714	rBV	210	248	0.01%	0.002%
16	3.649	715	718	725	rVV2	249	297	0.01%	0.002%
17	3.713	735	738	740	rBV	194	153	0.00%	0.001%
18	3.774	753	757	759	rBV2	181	164	0.00%	0.001%
19	3.870	773	787	804	rVB2	7292	16307	0.37%	0.103%
20	4.015	830	832	838	rBV2	147	150	0.00%	0.001%
21	4.047	838	842	848	rBV	200	270	0.01%	0.002%
22	4.131	864	868	871	rBV2	184	161	0.00%	0.001%
23	4.668	1007	1035	1063	rVV2	498341	1407058	31.92%	8.886%
24	4.883	1098	1102	1106	rVB2	309	262	0.01%	0.002%
25	4.941	1117	1120	1123	rVB3	359	177	0.00%	0.001%
26	5.066	1142	1159	1181	rBV	219182	482995	10.96%	3.050%
27	5.195	1196	1199	1202	rBV2	180	141	0.00%	0.001%
28	5.221	1202	1207	1212	rVV3	221	262	0.01%	0.002%
29	5.320	1219	1238	1261	rBV	230084	516683	11.72%	3.263%
30	5.616	1324	1330	1333	rBV2	160	205	0.00%	0.001%
31	5.729	1342	1365	1386	rBV2	469502	1251390	28.39%	7.903%
32	6.041	1458	1462	1466	rVB2	263	283	0.01%	0.002%
33	6.111	1481	1484	1488	rBV2	311	281	0.01%	0.002%
34	6.253	1512	1528	1549	rBV	383683	715539	16.23%	4.519%
35	6.439	1581	1586	1591	rBV2	131	177	0.00%	0.001%
36	6.481	1594	1599	1601	rBV3	283	286	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045213.D
 Acq On : 07 Oct 2021 15:41
 Operator : SY/MD
 Sample : M4025-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.546	1602	1619	1651	rBV	2364082	4407985	100.00%	27.839%
38	6.697	1653	1666	1686	rVB	293878	575166	13.05%	3.633%
39	6.973	1749	1752	1756	rBV2	240	233	0.01%	0.001%
40	7.044	1768	1774	1781	rBV	495	601	0.01%	0.004%
41	7.099	1786	1791	1795	rVB2	266	263	0.01%	0.002%
42	7.182	1811	1817	1826	rVB4	1122	1334	0.03%	0.008%
43	7.346	1860	1868	1874	rBV2	267	542	0.01%	0.003%
44	7.510	1915	1919	1923	rBV2	162	198	0.00%	0.001%
45	7.568	1923	1937	1956	rBV	149031	259975	5.90%	1.642%
46	7.690	1968	1975	1983	rBV4	793	1316	0.03%	0.008%
47	7.902	2026	2041	2056	rBV	567625	977253	22.17%	6.172%
48	7.973	2056	2063	2074	rVB	8060	12919	0.29%	0.082%
49	8.041	2082	2084	2087	rBV2	213	148	0.00%	0.001%
50	8.182	2116	2128	2141	rBV	103748	173694	3.94%	1.097%
51	8.256	2149	2151	2154	rVB3	510	274	0.01%	0.002%
52	8.291	2160	2162	2166	rVV2	220	179	0.00%	0.001%
53	8.327	2166	2173	2177	rVB2	286	425	0.01%	0.003%
54	8.407	2188	2198	2207	rVB4	3999	6170	0.14%	0.039%
55	8.475	2210	2219	2228	rVB2	800	1361	0.03%	0.009%
56	8.510	2228	2230	2235	rVB2	259	221	0.01%	0.001%
57	8.635	2255	2269	2302	rBV	402870	711876	16.15%	4.496%
58	8.809	2321	2323	2329	rVB3	313	292	0.01%	0.002%
59	8.861	2336	2339	2343	rVB2	191	173	0.00%	0.001%
60	8.941	2361	2364	2367	rVB2	223	177	0.00%	0.001%
61	8.989	2376	2379	2385	rVB2	218	253	0.01%	0.002%
62	9.024	2385	2390	2393	rBV2	152	170	0.00%	0.001%
63	9.089	2405	2410	2414	rVV2	177	203	0.00%	0.001%
64	9.124	2418	2421	2424	rBV	218	193	0.00%	0.001%
65	9.179	2434	2438	2444	rVB2	230	260	0.01%	0.002%
66	9.211	2444	2448	2454	rBV2	247	345	0.01%	0.002%
67	9.256	2454	2462	2468	rBV2	528	904	0.02%	0.006%
68	9.288	2468	2472	2476	rVV2	363	395	0.01%	0.002%
69	9.420	2499	2513	2534	rBV	543799	893004	20.26%	5.640%
70	9.536	2547	2549	2555	rVB3	1291	1171	0.03%	0.007%
71	9.571	2557	2560	2566	rVV3	209	220	0.00%	0.001%
72	9.700	2592	2600	2608	rBV4	588	1070	0.02%	0.007%
73	9.947	2671	2677	2680	rBV2	222	297	0.01%	0.002%
74	10.526	2854	2857	2861	rBV	221	246	0.01%	0.002%
75	10.568	2867	2870	2874	rBV	292	246	0.01%	0.002%
76	10.613	2876	2884	2887	rBV2	302	350	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045213.D
 Acq On : 07 Oct 2021 15:41
 Operator : SY/MD
 Sample : M4025-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.674	2895	2903	2908	rBV2	1325	1770	0.04%	0.011%
78	10.761	2916	2930	2950	rVB	421419	666506	15.12%	4.209%
79	10.832	2950	2952	2955	rVB2	256	164	0.00%	0.001%
80	10.867	2959	2963	2967	rBV3	523	466	0.01%	0.003%
81	11.008	3004	3007	3010	rBV	224	143	0.00%	0.001%
82	11.098	3028	3035	3039	rBV2	296	395	0.01%	0.002%
83	11.121	3039	3042	3044	rBV2	248	198	0.00%	0.001%
84	11.169	3055	3057	3061	rBV2	150	143	0.00%	0.001%
85	11.465	3142	3149	3150	rBV2	768	835	0.02%	0.005%
86	11.532	3166	3170	3174	rVB3	370	269	0.01%	0.002%
87	11.693	3214	3220	3221	rBV	398	356	0.01%	0.002%
88	11.735	3229	3233	3235	rBV	238	196	0.00%	0.001%
89	11.815	3245	3258	3277	rBV	509237	795646	18.05%	5.025%
90	11.976	3303	3308	3312	rBV3	626	660	0.01%	0.004%
91	12.195	3363	3376	3396	rBV	525373	835681	18.96%	5.278%
92	12.410	3440	3443	3445	rBV	194	145	0.00%	0.001%
93	12.645	3513	3516	3520	rBV	375	289	0.01%	0.002%
94	12.957	3606	3613	3616	rBV2	325	312	0.01%	0.002%
95	12.986	3617	3622	3625	rBV	248	310	0.01%	0.002%
96	13.237	3696	3700	3703	rBV	230	250	0.01%	0.002%
97	14.384	4053	4057	4060	rBV3	258	242	0.01%	0.002%
98	14.799	4183	4186	4188	rBV3	251	159	0.00%	0.001%
99	14.912	4218	4221	4224	rBV	560	454	0.01%	0.003%
100	16.117	4594	4596	4597	rBV	416	187	0.00%	0.001%




Sum of corrected areas: 15833862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045213.D
Acq On : 07 Oct 2021 15:41
Operator : SY/MD
Sample : M4025-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

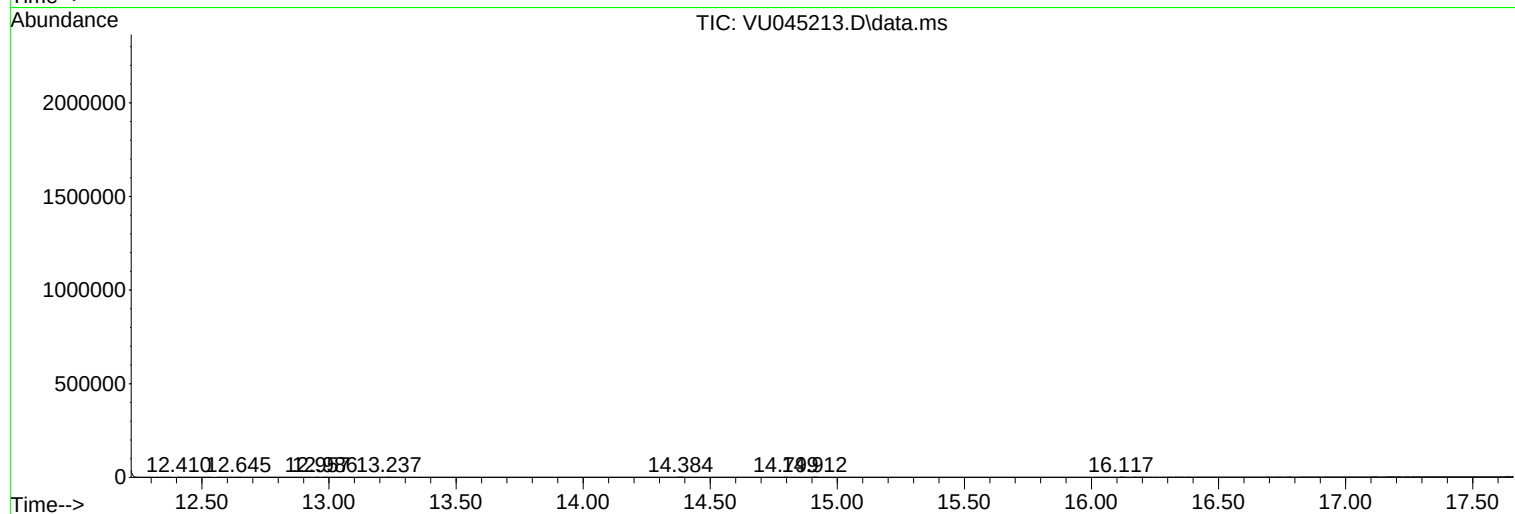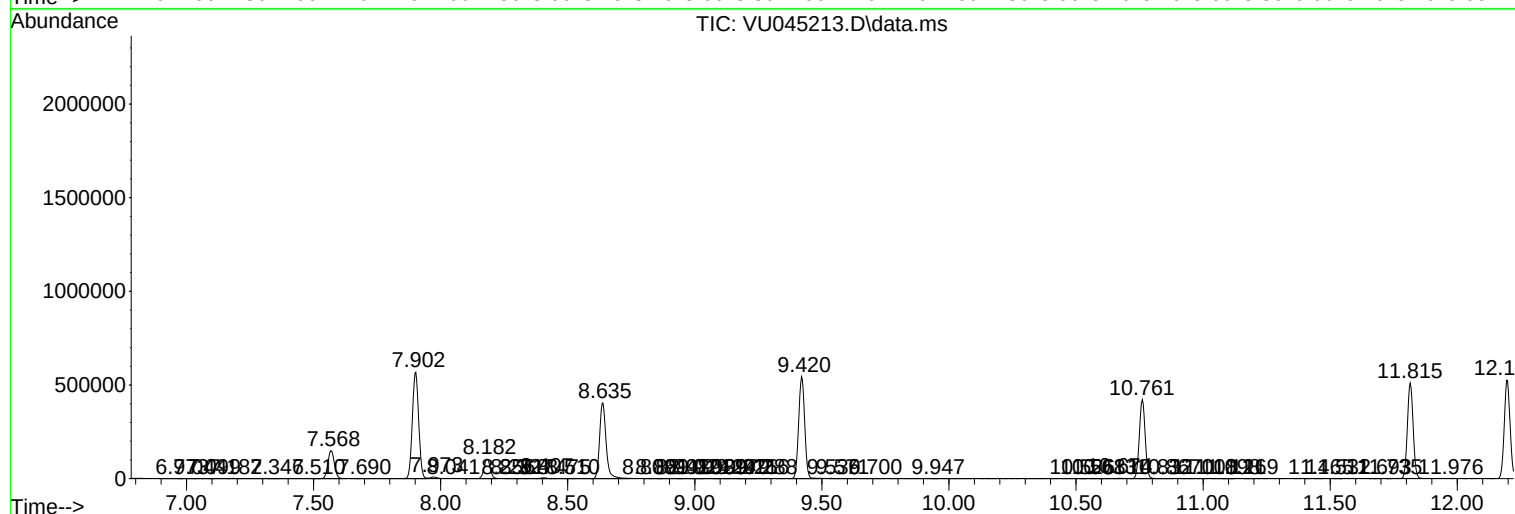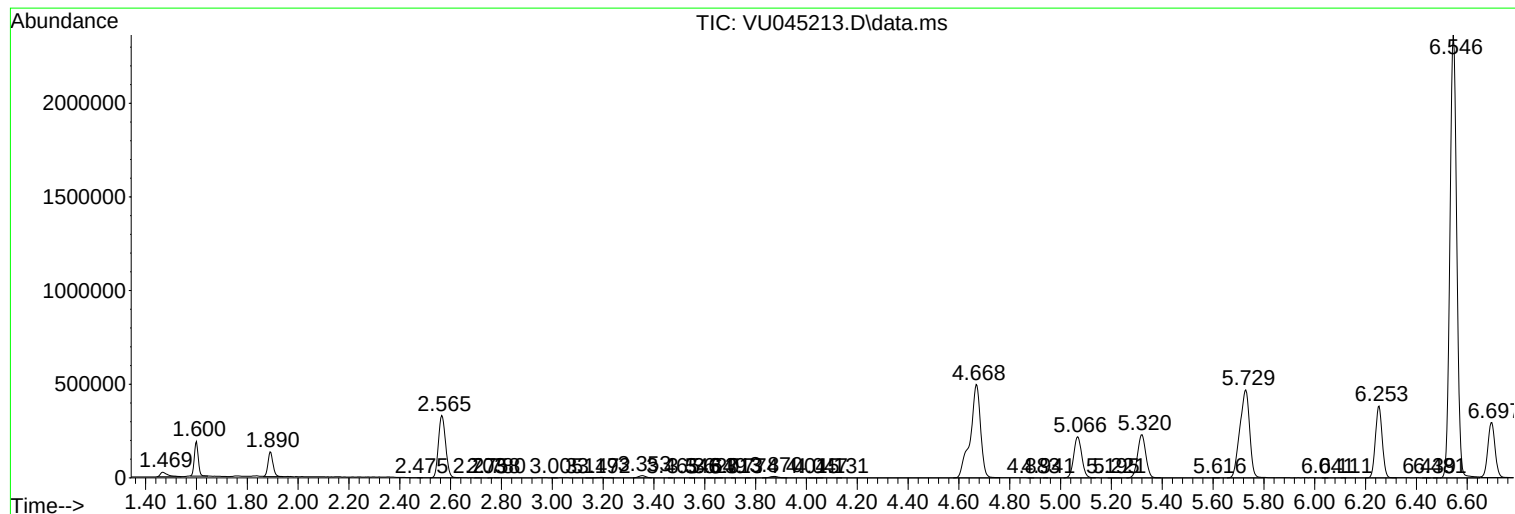

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045213.D
Acq On : 07 Oct 2021 15:41
Operator : SY/MD
Sample : M4025-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045213.D
Acq On : 07 Oct 2021 15:41
Operator : SY/MD
Sample : M4025-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------