

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045217.D
 Acq On : 07 Oct 2021 18:24
 Operator : SY/MD
 Sample : VU1007WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	53	rBV	12073	20408	1.50%	0.196%
2	1.600	73	81	97	rVB	217542	229225	16.84%	2.197%
3	1.896	164	173	192	rVB	145915	202486	14.88%	1.940%
4	2.562	368	380	407	rBV	292219	492391	36.18%	4.718%
5	2.678	413	416	419	rBV	255	189	0.01%	0.002%
6	2.790	444	451	459	rBV4	1033	1767	0.13%	0.017%
7	2.961	499	504	507	rVV2	308	326	0.02%	0.003%
8	3.051	522	532	540	rVB4	2158	4071	0.30%	0.039%
9	3.192	566	576	588	rVV3	1350	3002	0.22%	0.029%
10	3.292	603	607	614	rVB2	266	314	0.02%	0.003%
11	3.350	622	625	626	rBV	302	208	0.02%	0.002%
12	3.694	729	732	736	rBV	225	168	0.01%	0.002%
13	3.967	814	817	822	rVB2	296	237	0.02%	0.002%
14	3.999	822	827	831	rVB2	211	212	0.02%	0.002%
15	4.054	837	844	846	rBV2	275	258	0.02%	0.002%
16	4.182	881	884	887	rBV2	166	159	0.01%	0.002%
17	4.276	909	913	917	rVV2	146	179	0.01%	0.002%
18	4.314	919	925	928	rBV	175	232	0.02%	0.002%
19	4.427	957	960	965	rVB2	224	240	0.02%	0.002%
20	4.459	965	970	977	rVB2	258	351	0.03%	0.003%
21	4.494	977	981	984	rBV2	223	214	0.02%	0.002%
22	4.549	994	998	1001	rBV	151	179	0.01%	0.002%
23	4.629	1007	1023	1048	rBV	140893	330015	24.25%	3.162%
24	4.948	1118	1122	1125	rBV2	294	264	0.02%	0.003%
25	5.067	1142	1159	1182	rBV	237656	519635	38.18%	4.979%
26	5.295	1224	1230	1237	rBV2	556	860	0.06%	0.008%
27	5.388	1257	1259	1264	rVB	222	167	0.01%	0.002%
28	5.542	1300	1307	1311	rBV2	224	321	0.02%	0.003%
29	5.604	1322	1326	1330	rBV2	221	227	0.02%	0.002%
30	5.626	1330	1333	1337	rBV2	205	217	0.02%	0.002%
31	5.729	1342	1365	1397	rBV2	515522	1360899	100.00%	13.041%
32	5.931	1425	1428	1430	rBV2	265	178	0.01%	0.002%
33	6.112	1481	1484	1486	rBV3	319	190	0.01%	0.002%
34	6.253	1513	1528	1550	rBV	400089	744428	54.70%	7.133%
35	6.533	1606	1615	1626	rVB8	4892	9334	0.69%	0.089%
36	6.697	1648	1666	1685	rBV	320509	619819	45.54%	5.939%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045217.D
 Acq On : 07 Oct 2021 18:24
 Operator : SY/MD
 Sample : VU1007WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.806	1696	1700	1701	rBV	519	385	0.03%	0.004%
38	6.841	1708	1711	1713	rVB2	316	191	0.01%	0.002%
39	6.973	1747	1752	1755	rVB	180	155	0.01%	0.001%
40	7.044	1769	1774	1779	rVV3	495	625	0.05%	0.006%
41	7.189	1809	1819	1826	rVV3	731	1161	0.09%	0.011%
42	7.417	1887	1890	1893	rBV	206	194	0.01%	0.002%
43	7.478	1905	1909	1912	rVB2	210	186	0.01%	0.002%
44	7.568	1924	1937	1955	rBV	185384	317404	23.32%	3.042%
45	7.687	1970	1974	1978	rBV3	342	317	0.02%	0.003%
46	7.793	2000	2007	2019	rVB4	1875	2843	0.21%	0.027%
47	7.902	2024	2041	2056	rBV	641596	1085559	79.77%	10.402%
48	7.973	2057	2063	2077	rVB2	9170	15464	1.14%	0.148%
49	8.182	2116	2128	2143	rBV	126917	211148	15.52%	2.023%
50	8.295	2161	2163	2169	rVB2	348	304	0.02%	0.003%
51	8.436	2204	2207	2211	rBV	156	185	0.01%	0.002%
52	8.639	2256	2270	2310	rVV	418258	747284	54.91%	7.161%
53	8.944	2359	2365	2367	rBV2	198	233	0.02%	0.002%
54	9.208	2443	2447	2451	rBV2	190	193	0.01%	0.002%
55	9.288	2467	2472	2477	rBV2	274	352	0.03%	0.003%
56	9.356	2487	2493	2496	rVB2	234	296	0.02%	0.003%
57	9.420	2500	2513	2536	rBV	573433	933520	68.60%	8.945%
58	9.574	2551	2561	2562	rBV2	431	569	0.04%	0.005%
59	9.700	2591	2600	2606	rVV2	1105	1650	0.12%	0.016%
60	9.767	2618	2621	2626	rBV2	222	205	0.02%	0.002%
61	9.835	2636	2642	2648	rBV2	163	282	0.02%	0.003%
62	10.115	2723	2729	2736	rVB5	796	1026	0.08%	0.010%
63	10.163	2741	2744	2747	rBV	291	219	0.02%	0.002%
64	10.414	2819	2822	2825	rBV2	216	198	0.01%	0.002%
65	10.674	2895	2903	2911	rVV3	4461	6275	0.46%	0.060%
66	10.761	2917	2930	2949	rBV	437384	702502	51.62%	6.732%
67	10.832	2950	2952	2955	rVB3	897	493	0.04%	0.005%
68	10.873	2955	2965	2968	rBV3	935	1311	0.10%	0.013%
69	11.153	3050	3052	3056	rVB2	563	399	0.03%	0.004%
70	11.372	3117	3120	3123	rVV2	237	203	0.01%	0.002%
71	11.391	3123	3126	3131	rVV2	304	271	0.02%	0.003%
72	11.459	3139	3147	3160	rVB4	3202	6029	0.44%	0.058%
73	11.578	3180	3184	3186	rBV3	579	493	0.04%	0.005%
74	11.623	3192	3198	3201	rBV2	274	319	0.02%	0.003%
75	11.700	3215	3222	3229	rVB3	1724	2344	0.17%	0.022%
76	11.751	3233	3238	3244	rVB2	1237	1452	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045217.D
 Acq On : 07 Oct 2021 18:24
 Operator : SY/MD
 Sample : VU1007WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

77	11.815	3245	3258	3277	rBV	553654	872731	64.13%	8.363%
78	11.912	3283	3288	3289	rBV4	307	235	0.02%	0.002%
79	11.947	3292	3299	3302	rBV3	1359	1726	0.13%	0.017%
80	12.041	3325	3328	3332	rVB	391	237	0.02%	0.002%
81	12.198	3361	3377	3397	rVV	579107	937937	68.92%	8.988%
82	12.282	3398	3403	3412	rVB4	815	1170	0.09%	0.011%
83	12.333	3412	3419	3420	rBV2	937	862	0.06%	0.008%
84	12.404	3435	3441	3443	rBV2	588	497	0.04%	0.005%
85	12.539	3480	3483	3490	rBV2	230	263	0.02%	0.003%
86	12.600	3500	3502	3507	rVB2	319	189	0.01%	0.002%
87	12.639	3507	3514	3517	rBV4	603	733	0.05%	0.007%
88	12.999	3619	3626	3627	rBV	618	539	0.04%	0.005%
89	13.153	3670	3674	3676	rBV	331	266	0.02%	0.003%
90	13.230	3690	3698	3705	rVB5	1661	2202	0.16%	0.021%
91	13.301	3716	3720	3726	rBV	264	344	0.03%	0.003%
92	13.844	3882	3889	3898	rVB5	3584	5186	0.38%	0.050%
93	13.883	3898	3901	3906	rVB2	245	206	0.02%	0.002%
94	13.912	3906	3910	3912	rBV	192	192	0.01%	0.002%
95	13.989	3931	3934	3937	rVB2	290	169	0.01%	0.002%
96	14.092	3958	3966	3978	rBV2	9879	15306	1.12%	0.147%
97	14.217	4000	4005	4011	rVB3	323	387	0.03%	0.004%
98	14.333	4034	4041	4054	rBV7	3934	6315	0.46%	0.061%
99	14.966	4235	4238	4241	rBV	244	194	0.01%	0.002%
100	15.114	4282	4284	4287	rBV	275	183	0.01%	0.002%




Sum of corrected areas: 10435678

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045217.D
Acq On : 07 Oct 2021 18:24
Operator : SY/MD
Sample : VU1007WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

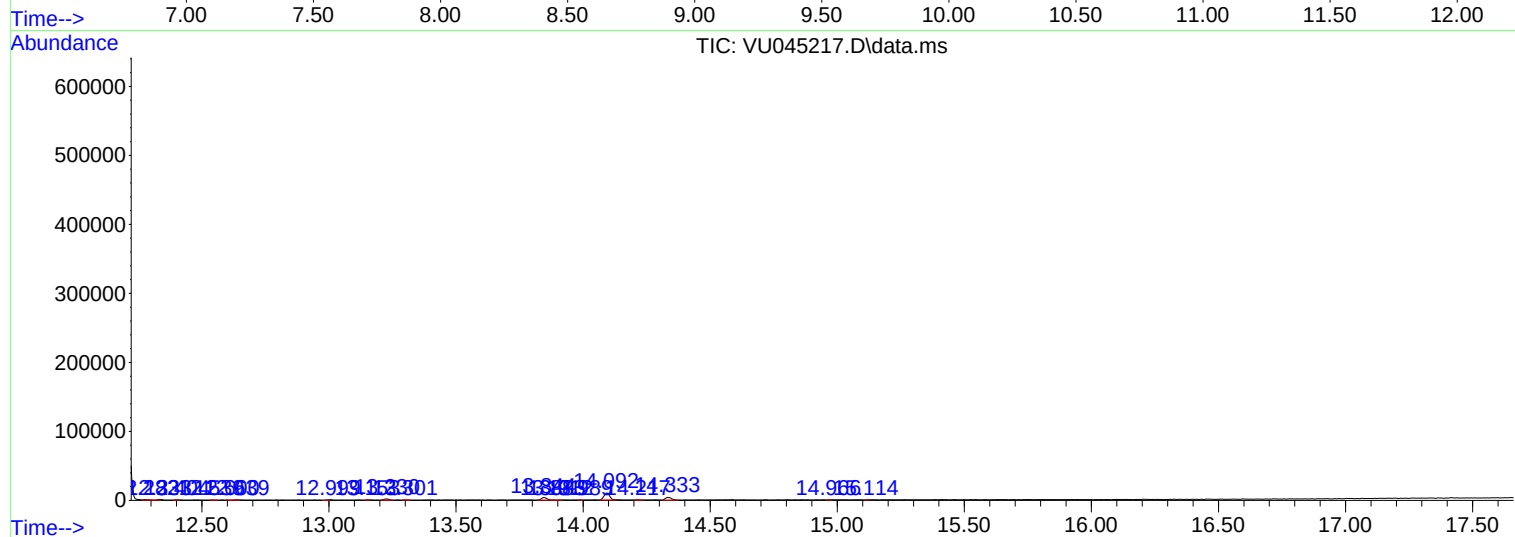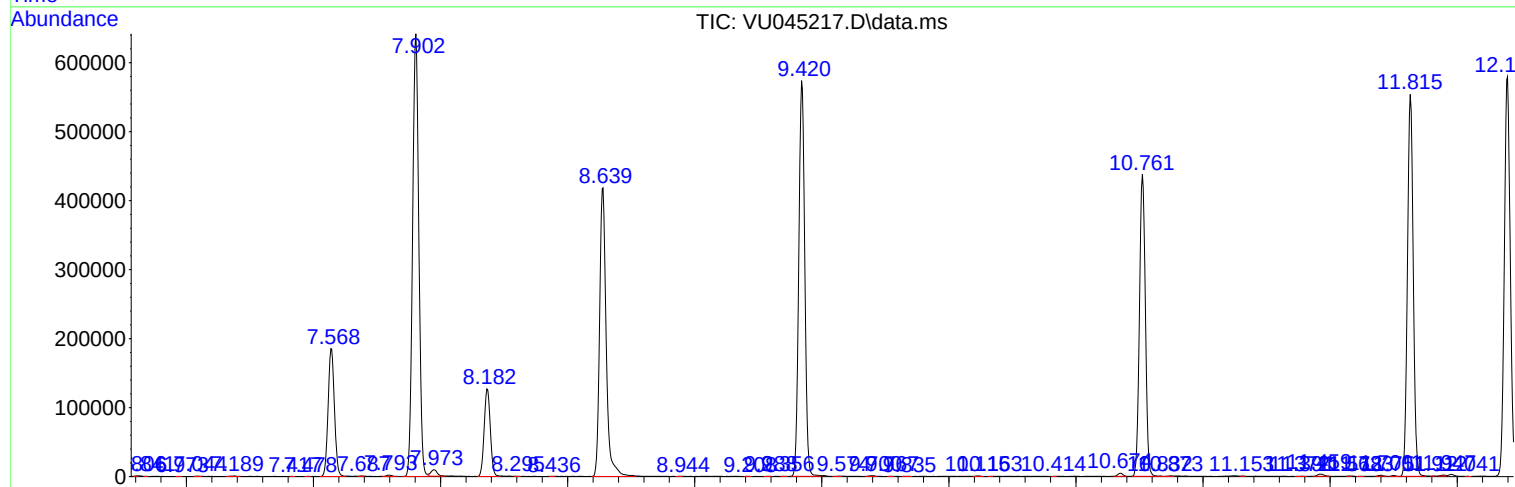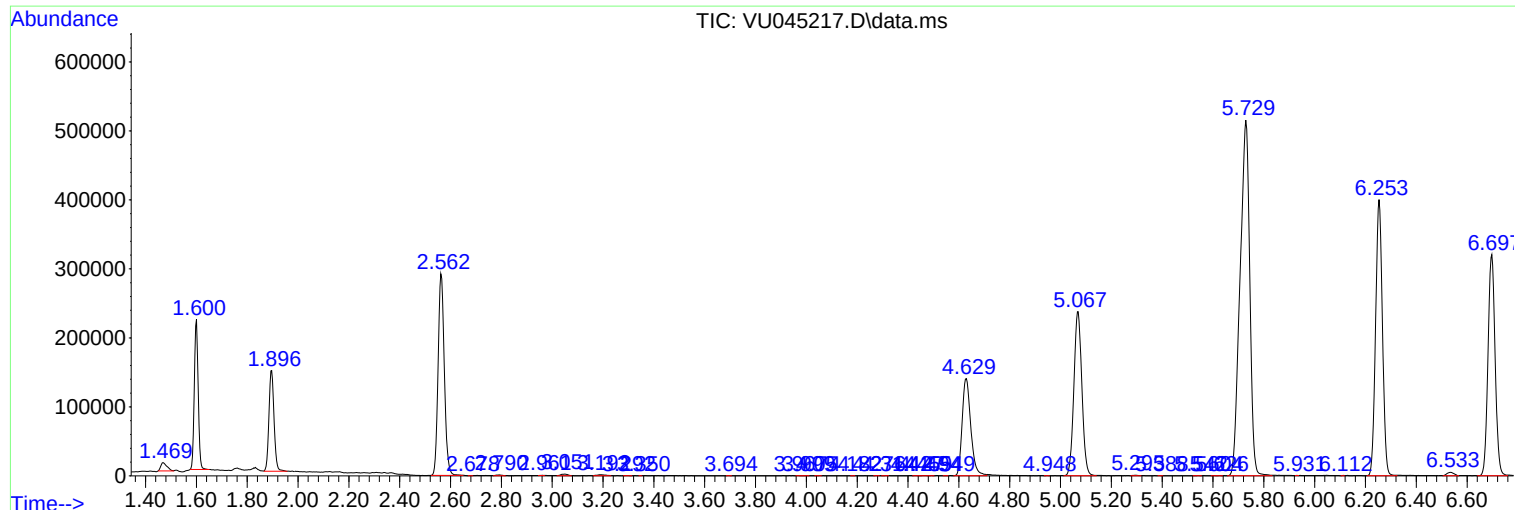

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045217.D
Acq On : 07 Oct 2021 18:24
Operator : SY/MD
Sample : VU1007WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045217.D
Acq On : 07 Oct 2021 18:24
Operator : SY/MD
Sample : VU1007WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------