

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045220.D
 Acq On : 07 Oct 2021 20:04
 Operator : SY/MD
 Sample : M4023-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	33	40	55	rBV	16805	31744	2.46%	0.327%
2	1.597	73	80	97	rBV	198954	214942	16.65%	2.211%
3	1.890	162	171	187	rVB	138701	190173	14.73%	1.956%
4	2.491	355	358	363	rVB2	296	193	0.01%	0.002%
5	2.559	367	379	400	rBV	264381	447162	34.63%	4.600%
6	2.697	420	422	426	rVV	225	168	0.01%	0.002%
7	2.735	429	434	438	rBV2	224	260	0.02%	0.003%
8	2.790	444	451	460	rVB4	923	1626	0.13%	0.017%
9	2.964	497	505	509	rVB2	269	401	0.03%	0.004%
10	3.022	519	523	524	rBV	209	156	0.01%	0.002%
11	3.038	524	528	529	rBV2	394	269	0.02%	0.003%
12	3.189	564	575	589	rVB2	3852	8859	0.69%	0.091%
13	3.375	630	633	637	rBV2	188	182	0.01%	0.002%
14	3.652	712	719	722	rBV	231	292	0.02%	0.003%
15	3.735	739	745	747	rVB2	217	177	0.01%	0.002%
16	3.896	793	795	800	rVB2	223	190	0.01%	0.002%
17	3.935	803	807	811	rBV2	188	154	0.01%	0.002%
18	4.215	889	894	896	rBV2	213	192	0.01%	0.002%
19	4.308	920	923	925	rBV2	255	201	0.02%	0.002%
20	4.469	968	973	979	rVV2	180	286	0.02%	0.003%
21	4.539	989	995	999	rVV2	181	220	0.02%	0.002%
22	4.629	1007	1023	1060	rBV	141448	334577	25.91%	3.442%
23	5.005	1133	1140	1142	rVB2	138	154	0.01%	0.002%
24	5.067	1142	1159	1190	rBV	226567	491037	38.03%	5.052%
25	5.192	1195	1198	1202	rBV	269	220	0.02%	0.002%
26	5.218	1205	1206	1210	rBV	285	156	0.01%	0.002%
27	5.295	1222	1230	1235	rVB3	601	976	0.08%	0.010%
28	5.378	1249	1256	1260	rBV2	452	613	0.05%	0.006%
29	5.565	1310	1314	1316	rBV	202	164	0.01%	0.002%
30	5.629	1330	1334	1338	rBV2	156	160	0.01%	0.002%
31	5.726	1341	1364	1390	rBV2	481398	1291243	100.00%	13.284%
32	5.980	1439	1443	1446	rVB3	271	234	0.02%	0.002%
33	5.999	1446	1449	1451	rBV	283	213	0.02%	0.002%
34	6.076	1471	1473	1479	rVB2	362	264	0.02%	0.003%
35	6.102	1479	1481	1482	rBV2	387	157	0.01%	0.002%
36	6.253	1512	1528	1546	rBV	376342	705248	54.62%	7.255%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045220.D
 Acq On : 07 Oct 2021 20:04
 Operator : SY/MD
 Sample : M4023-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.533	1605	1615	1627	rBV6	4612	9040	0.70%	0.093%
38	6.642	1645	1649	1651	rBV2	201	161	0.01%	0.002%
39	6.694	1651	1665	1689	rVV	302151	588796	45.60%	6.057%
40	6.809	1692	1701	1707	rVB4	1097	1692	0.13%	0.017%
41	6.935	1735	1740	1743	rBV2	211	241	0.02%	0.002%
42	7.047	1770	1775	1779	rBV2	627	625	0.05%	0.006%
43	7.185	1809	1818	1827	rVB6	1094	1828	0.14%	0.019%
44	7.375	1875	1877	1881	rBV	198	173	0.01%	0.002%
45	7.436	1892	1896	1900	rVB2	216	157	0.01%	0.002%
46	7.484	1906	1911	1913	rVB2	195	165	0.01%	0.002%
47	7.568	1923	1937	1956	rVV	145184	251536	19.48%	2.588%
48	7.681	1966	1972	1973	rBV2	402	323	0.03%	0.003%
49	7.738	1986	1990	1993	rBV2	160	179	0.01%	0.002%
50	7.819	2012	2015	2018	rBV	164	162	0.01%	0.002%
51	7.902	2026	2041	2056	rBV	586987	1006557	77.95%	10.355%
52	7.970	2056	2062	2073	rVB	8352	14004	1.08%	0.144%
53	8.182	2112	2128	2143	rBV	102975	170465	13.20%	1.754%
54	8.639	2256	2270	2309	rBV	422741	750531	58.12%	7.721%
55	8.902	2349	2352	2355	rBV	163	154	0.01%	0.002%
56	9.224	2447	2452	2455	rBV2	165	160	0.01%	0.002%
57	9.243	2455	2458	2461	rBV	203	179	0.01%	0.002%
58	9.420	2498	2513	2530	rBV	552485	886950	68.69%	9.125%
59	9.568	2556	2559	2560	rBV2	270	175	0.01%	0.002%
60	9.700	2592	2600	2604	rBV3	790	1183	0.09%	0.012%
61	9.783	2622	2626	2631	rBV2	235	236	0.02%	0.002%
62	9.819	2631	2637	2643	rBV2	198	352	0.03%	0.004%
63	9.928	2666	2671	2675	rVV2	473	546	0.04%	0.006%
64	10.333	2788	2797	2799	rBV	211	268	0.02%	0.003%
65	10.674	2898	2903	2909	rVB3	1493	1578	0.12%	0.016%
66	10.761	2917	2930	2951	rVB	423654	681407	52.77%	7.010%
67	10.867	2960	2963	2964	rBV	348	180	0.01%	0.002%
68	10.983	2994	2999	3001	rBV2	215	191	0.01%	0.002%
69	10.999	3002	3004	3007	rVV2	289	185	0.01%	0.002%
70	11.089	3029	3032	3037	rVB2	404	338	0.03%	0.003%
71	11.121	3038	3042	3046	rBV2	216	172	0.01%	0.002%
72	11.237	3073	3078	3079	rBV	234	212	0.02%	0.002%
73	11.259	3079	3085	3088	rVV2	265	323	0.03%	0.003%
74	11.298	3094	3097	3102	rVV2	189	228	0.02%	0.002%
75	11.433	3133	3139	3142	rBV	288	318	0.02%	0.003%
76	11.513	3161	3164	3169	rBV2	197	163	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045220.D
 Acq On : 07 Oct 2021 20:04
 Operator : SY/MD
 Sample : M4023-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.584	3181	3186	3191	rVB3	305	270	0.02%	0.003%
78	11.635	3195	3202	3208	rBV2	533	907	0.07%	0.009%
79	11.697	3219	3221	3226	rVB3	303	266	0.02%	0.003%
80	11.816	3245	3258	3278	rVV	491543	771093	59.72%	7.933%
81	11.915	3287	3289	3293	rBV	304	283	0.02%	0.003%
82	12.195	3364	3376	3396	rBV	521853	846791	65.58%	8.712%
83	12.430	3445	3449	3459	rVB2	365	506	0.04%	0.005%
84	12.491	3463	3468	3470	rBV2	218	203	0.02%	0.002%
85	12.828	3569	3573	3576	rBV	212	244	0.02%	0.003%
86	12.873	3584	3587	3590	rVB2	243	173	0.01%	0.002%
87	12.996	3619	3625	3628	rVB	249	254	0.02%	0.003%
88	13.015	3628	3631	3635	rBV2	226	194	0.02%	0.002%
89	13.307	3715	3722	3726	rBV2	272	406	0.03%	0.004%
90	13.343	3730	3733	3737	rBV	194	205	0.02%	0.002%
91	13.520	3785	3788	3791	rBV2	182	171	0.01%	0.002%
92	13.565	3798	3802	3804	rBV	330	304	0.02%	0.003%
93	13.851	3887	3891	3894	rBV2	355	259	0.02%	0.003%
94	14.095	3962	3967	3977	rVB2	757	1300	0.10%	0.013%
95	14.330	4039	4040	4044	rBV3	225	182	0.01%	0.002%
96	14.629	4131	4133	4136	rVB	338	167	0.01%	0.002%
97	14.812	4187	4190	4193	rBV2	282	214	0.02%	0.002%
98	14.992	4243	4246	4248	rVB2	347	185	0.01%	0.002%
99	15.008	4248	4251	4252	rBV	352	189	0.01%	0.002%
100	15.606	4435	4437	4441	rBV2	261	155	0.01%	0.002%




Sum of corrected areas: 9720317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045220.D
Acq On : 07 Oct 2021 20:04
Operator : SY/MD
Sample : M4023-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

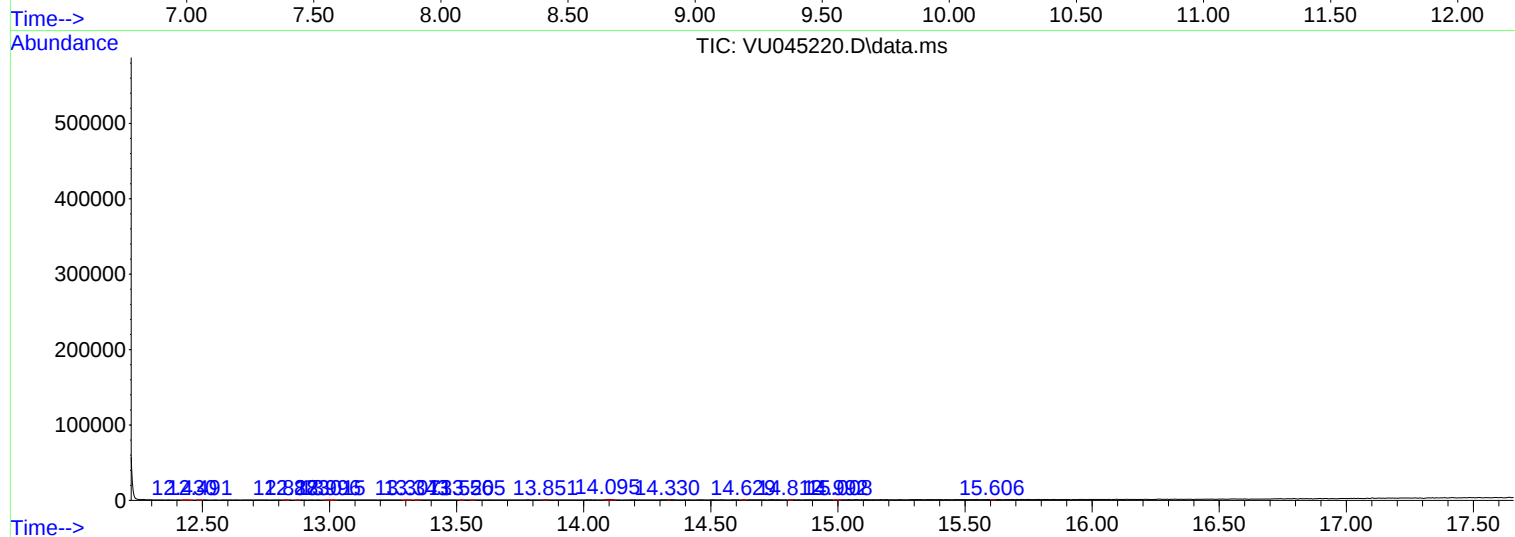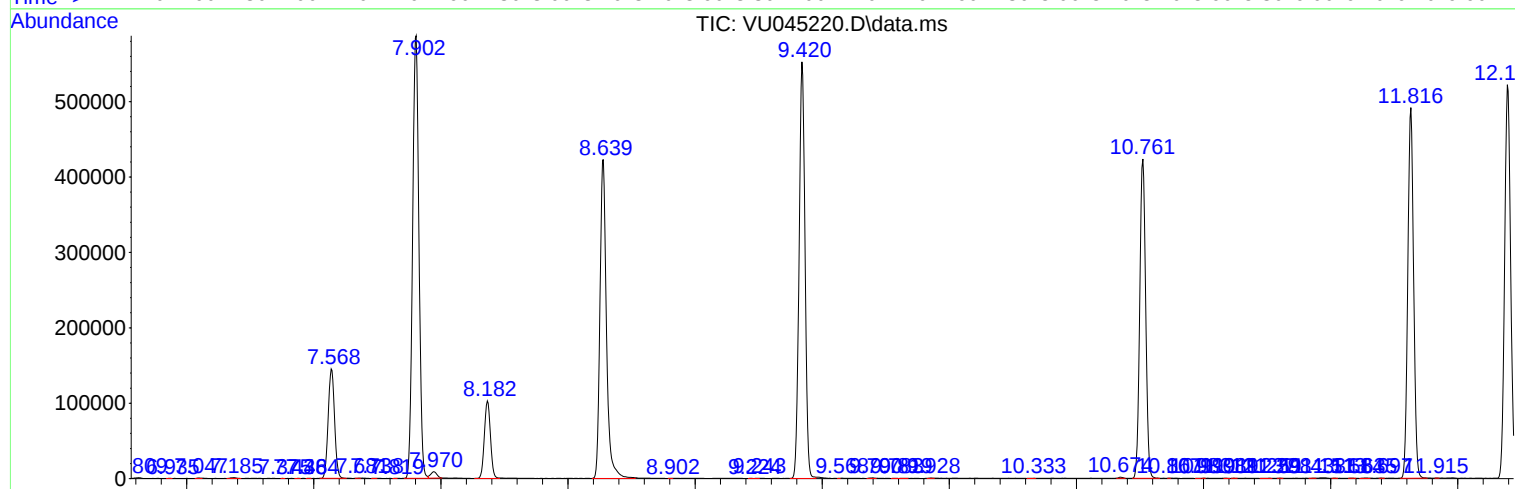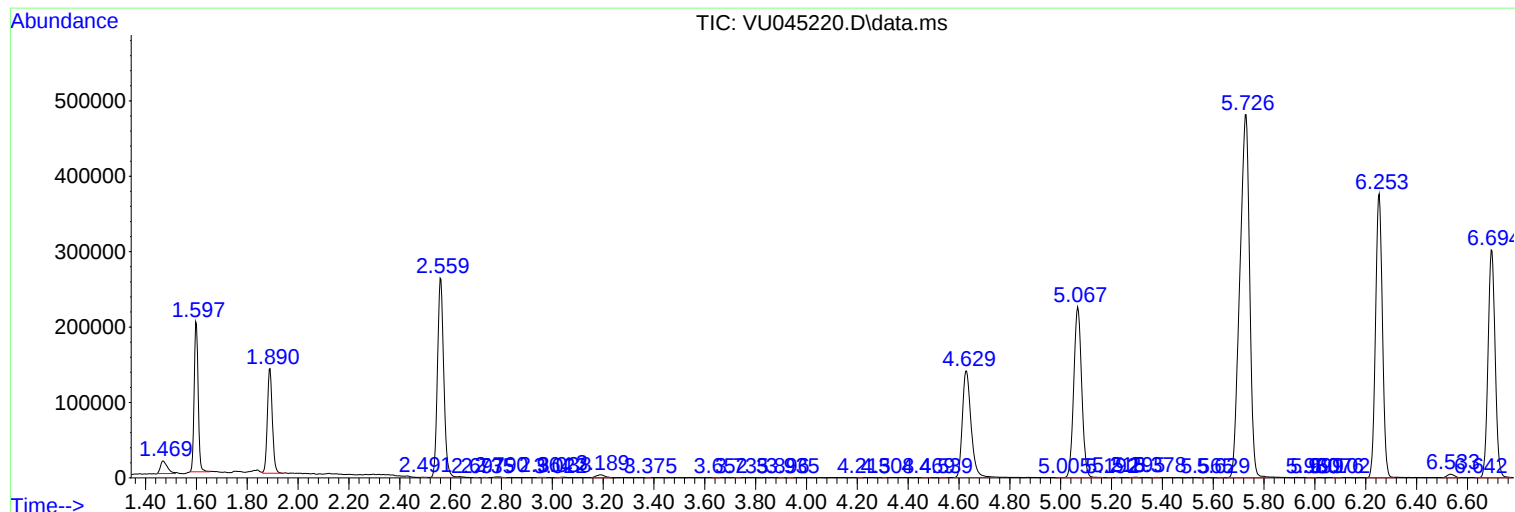

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045220.D
Acq On : 07 Oct 2021 20:04
Operator : SY/MD
Sample : M4023-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045220.D
Acq On : 07 Oct 2021 20:04
Operator : SY/MD
Sample : M4023-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
