

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045222.D
 Acq On : 07 Oct 2021 20:52
 Operator : SY/MD
 Sample : M4023-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	54	rBV	14164	24923	1.97%	0.259%
2	1.600	73	81	92	rBV	196938	212198	16.78%	2.209%
3	1.893	163	172	185	rVB	136805	183642	14.52%	1.912%
4	2.562	366	380	397	rBV	259987	439172	34.73%	4.571%
5	2.636	397	403	415	rVB	3131	5217	0.41%	0.054%
6	2.777	436	447	464	rBV	17553	34091	2.70%	0.355%
7	2.903	483	486	489	rBV2	187	148	0.01%	0.002%
8	2.957	498	503	511	rVV3	423	694	0.05%	0.007%
9	3.006	515	518	525	rBV2	183	238	0.02%	0.002%
10	3.047	525	531	537	rVV3	781	1043	0.08%	0.011%
11	3.121	551	554	559	rBV2	168	214	0.02%	0.002%
12	3.189	559	575	594	rVV	48329	112157	8.87%	1.167%
13	3.346	619	624	629	rBV2	214	273	0.02%	0.003%
14	3.398	634	640	645	rVB2	252	324	0.03%	0.003%
15	3.745	744	748	751	rVB2	180	172	0.01%	0.002%
16	3.768	751	755	760	rBV	194	150	0.01%	0.002%
17	3.797	760	764	767	rVB2	230	185	0.01%	0.002%
18	3.874	782	788	790	rBV2	185	168	0.01%	0.002%
19	4.060	843	846	850	rBV2	226	170	0.01%	0.002%
20	4.295	915	919	922	rBV2	180	166	0.01%	0.002%
21	4.420	955	958	960	rBV	198	166	0.01%	0.002%
22	4.501	979	983	988	rVB2	203	214	0.02%	0.002%
23	4.565	1000	1003	1008	rBV	183	173	0.01%	0.002%
24	4.629	1008	1023	1060	rBV	140832	342560	27.09%	3.566%
25	5.067	1143	1159	1178	rBV	222194	479076	37.88%	4.987%
26	5.301	1223	1232	1239	rBV4	742	1259	0.10%	0.013%
27	5.369	1249	1253	1256	rBV2	305	190	0.02%	0.002%
28	5.729	1343	1365	1390	rBV2	467692	1264680	100.00%	13.164%
29	5.944	1427	1432	1437	rBV3	533	766	0.06%	0.008%
30	6.253	1513	1528	1546	rBV	370264	690160	54.57%	7.184%
31	6.488	1596	1601	1606	rBV3	242	317	0.03%	0.003%
32	6.542	1606	1618	1630	rVV4	13949	28278	2.24%	0.294%
33	6.694	1651	1665	1686	rVV	297534	571883	45.22%	5.953%
34	6.767	1686	1688	1693	rVB3	532	367	0.03%	0.004%
35	6.806	1696	1700	1701	rBV3	632	453	0.04%	0.005%
36	7.047	1769	1775	1778	rBV2	365	441	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045222.D
 Acq On : 07 Oct 2021 20:52
 Operator : SY/MD
 Sample : M4023-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.298	1847	1853	1857	rBV2	256	370	0.03%	0.004%
38	7.520	1918	1922	1925	rVV	190	190	0.02%	0.002%
39	7.568	1925	1937	1962	rVV	143131	246251	19.47%	2.563%
40	7.658	1962	1965	1968	rVV2	204	165	0.01%	0.002%
41	7.690	1968	1975	1981	rVV3	784	1033	0.08%	0.011%
42	7.902	2026	2041	2055	rBV	579055	977894	77.32%	10.179%
43	7.976	2057	2064	2077	rVB2	8365	13560	1.07%	0.141%
44	8.182	2116	2128	2145	rBV	102005	165776	13.11%	1.726%
45	8.295	2161	2163	2169	rBV3	222	189	0.01%	0.002%
46	8.468	2213	2217	2226	rVB2	482	720	0.06%	0.007%
47	8.639	2256	2270	2304	rBV	400342	714310	56.48%	7.435%
48	8.787	2314	2316	2321	rVB2	485	400	0.03%	0.004%
49	9.066	2399	2403	2411	rVB2	156	218	0.02%	0.002%
50	9.218	2447	2450	2454	rVB	242	201	0.02%	0.002%
51	9.420	2499	2513	2548	rVB	535803	863652	68.29%	8.990%
52	9.697	2592	2599	2606	rBV4	936	1467	0.12%	0.015%
53	9.825	2635	2639	2643	rBV2	190	192	0.02%	0.002%
54	9.918	2664	2668	2672	rVB	173	202	0.02%	0.002%
55	9.973	2679	2685	2687	rBV	236	266	0.02%	0.003%
56	10.102	2720	2725	2732	rBV3	552	687	0.05%	0.007%
57	10.246	2766	2770	2776	rVB2	246	282	0.02%	0.003%
58	10.282	2776	2781	2784	rBV2	181	225	0.02%	0.002%
59	10.327	2791	2795	2797	rBV2	175	167	0.01%	0.002%
60	10.365	2804	2807	2810	rBV	157	158	0.01%	0.002%
61	10.472	2838	2840	2844	rVB	288	185	0.01%	0.002%
62	10.497	2844	2848	2850	rBV	198	164	0.01%	0.002%
63	10.639	2890	2892	2896	rBV	315	229	0.02%	0.002%
64	10.674	2896	2903	2912	rVB3	1452	1895	0.15%	0.020%
65	10.761	2913	2930	2951	rBV	409555	653835	51.70%	6.806%
66	10.938	2981	2985	2991	rVB2	312	322	0.03%	0.003%
67	10.980	2995	2998	3000	rBV	194	158	0.01%	0.002%
68	11.008	3004	3007	3009	rBV	195	151	0.01%	0.002%
69	11.205	3065	3068	3071	rBV	236	203	0.02%	0.002%
70	11.353	3111	3114	3116	rBV	241	197	0.02%	0.002%
71	11.398	3125	3128	3131	rBV	201	167	0.01%	0.002%
72	11.462	3144	3148	3157	rVB2	983	1557	0.12%	0.016%
73	11.578	3180	3184	3188	rBV	219	172	0.01%	0.002%
74	11.639	3197	3203	3207	rBV2	543	552	0.04%	0.006%
75	11.700	3214	3222	3226	rBV4	635	753	0.06%	0.008%
76	11.816	3245	3258	3278	rBV	472001	744274	58.85%	7.747%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045222.D
 Acq On : 07 Oct 2021 20:52
 Operator : SY/MD
 Sample : M4023-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.976	3306	3308	3314	rVB2	505	342	0.03%	0.004%
78	12.195	3362	3376	3394	rBV	503975	811831	64.19%	8.450%
79	12.282	3400	3403	3407	rBV	354	300	0.02%	0.003%
80	12.369	3426	3430	3433	rBV2	175	197	0.02%	0.002%
81	12.426	3444	3448	3452	rBV2	222	218	0.02%	0.002%
82	12.603	3500	3503	3508	rBV	223	170	0.01%	0.002%
83	12.889	3589	3592	3594	rBV2	182	159	0.01%	0.002%
84	12.954	3609	3612	3617	rVB	181	201	0.02%	0.002%
85	13.217	3692	3694	3698	rBV2	234	197	0.02%	0.002%
86	13.262	3705	3708	3710	rBV2	307	197	0.02%	0.002%
87	13.462	3764	3770	3772	rBV2	316	343	0.03%	0.004%
88	13.780	3866	3869	3874	rVB	293	234	0.02%	0.002%
89	13.812	3874	3879	3881	rBV2	313	318	0.03%	0.003%
90	13.828	3881	3884	3889	rVV2	192	202	0.02%	0.002%
91	14.005	3936	3939	3940	rBV	284	169	0.01%	0.002%
92	14.095	3962	3967	3970	rBV3	438	598	0.05%	0.006%
93	14.137	3977	3980	3983	rBV	213	185	0.01%	0.002%
94	14.227	4005	4008	4011	rBV2	329	180	0.01%	0.002%
95	14.246	4012	4014	4017	rVB2	361	165	0.01%	0.002%
96	14.266	4017	4020	4023	rBV	326	264	0.02%	0.003%
97	14.539	4102	4105	4108	rBV2	251	161	0.01%	0.002%
98	14.648	4136	4139	4141	rBV2	237	152	0.01%	0.002%
99	14.970	4235	4239	4242	rBV2	301	274	0.02%	0.003%
100	15.655	4449	4452	4455	rBV	344	265	0.02%	0.003%




Sum of corrected areas: 9607039

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045222.D
Acq On : 07 Oct 2021 20:52
Operator : SY/MD
Sample : M4023-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

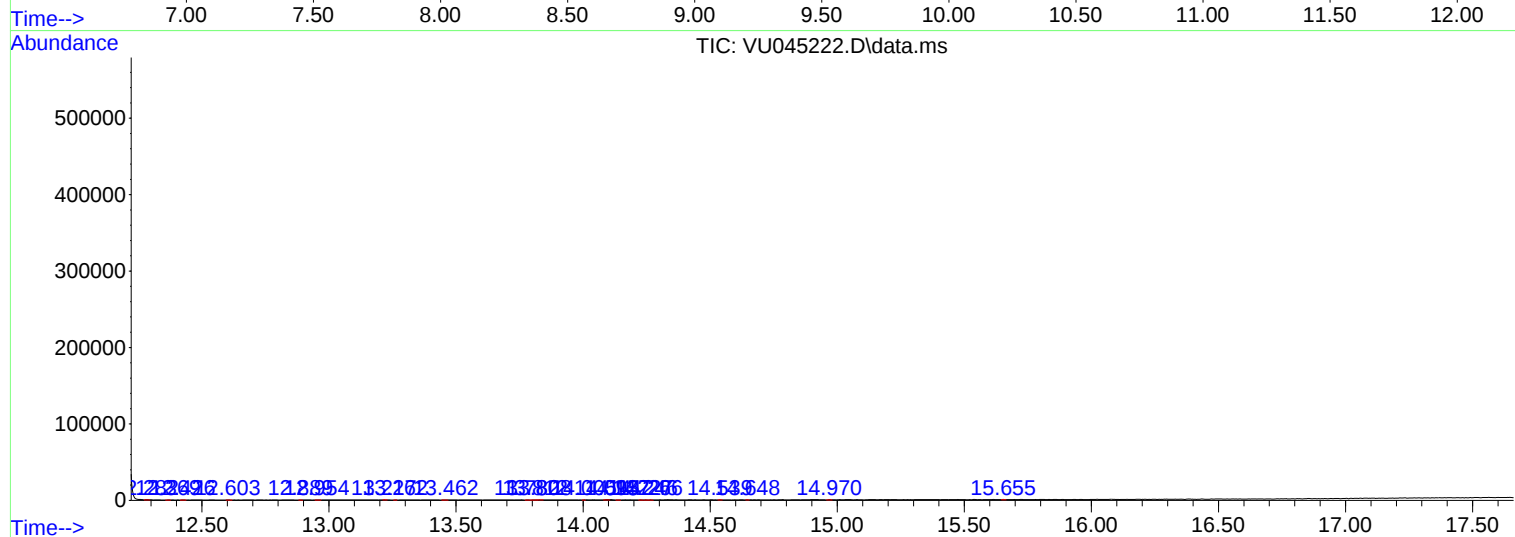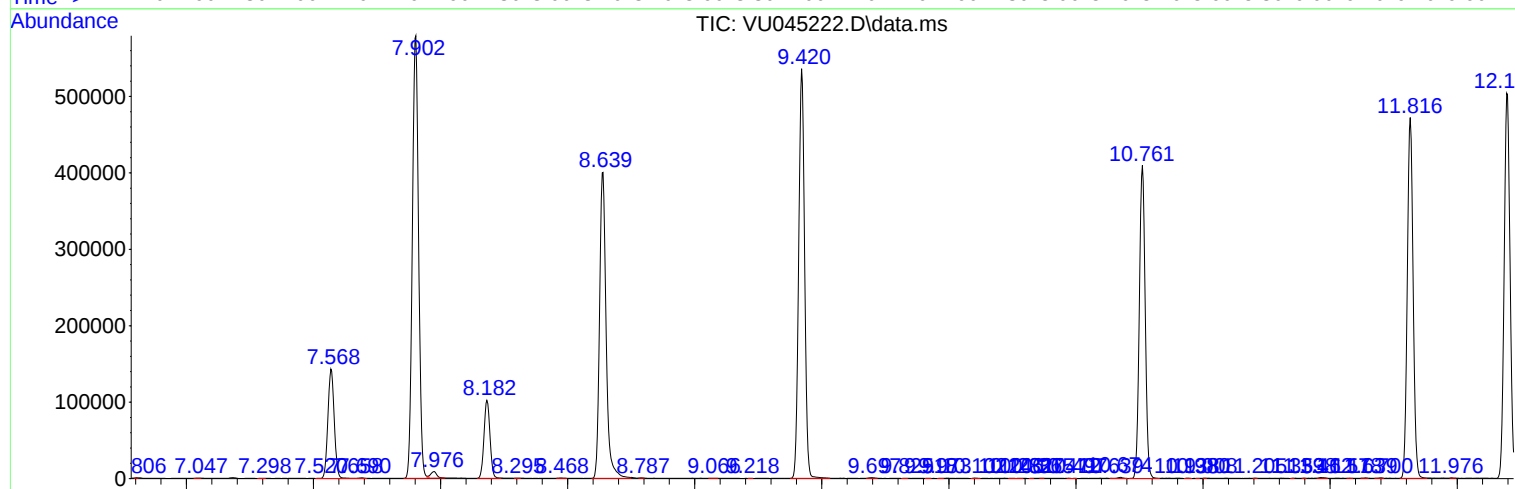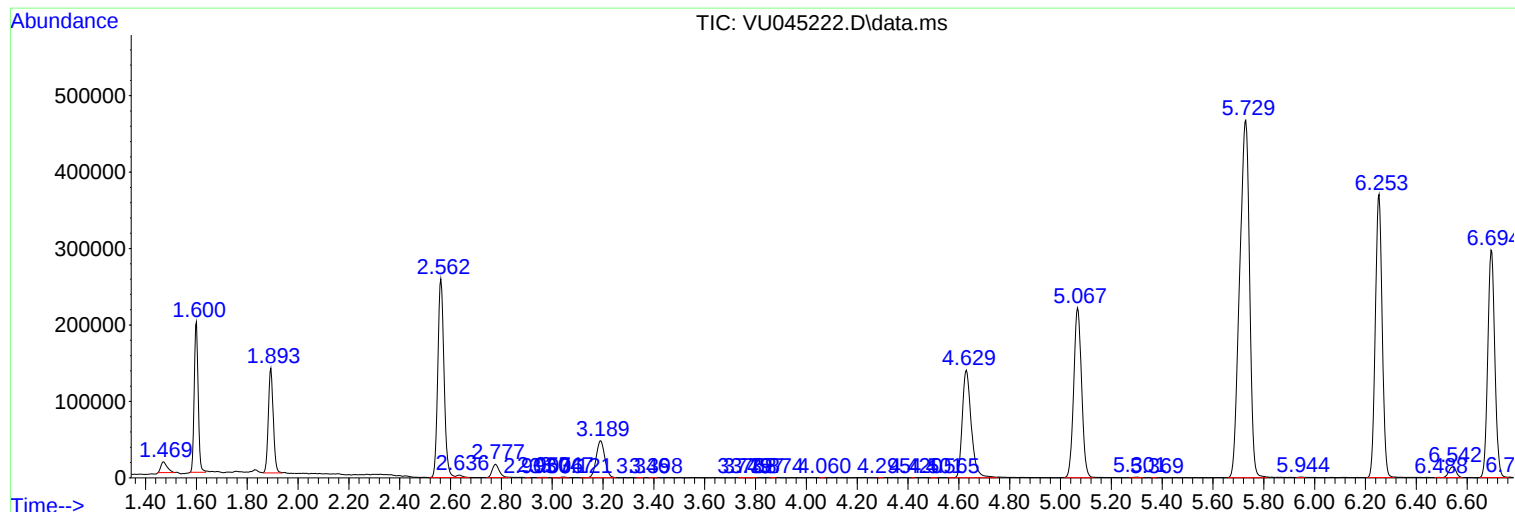

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045222.D
Acq On : 07 Oct 2021 20:52
Operator : SY/MD
Sample : M4023-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045222.D
Acq On : 07 Oct 2021 20:52
Operator : SY/MD
Sample : M4023-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
