

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045224.D
 Acq On : 07 Oct 2021 21:52
 Operator : SY/MD
 Sample : M4023-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	53	rBV	13140	23899	1.88%	0.206%
2	1.597	73	80	93	rBV	198706	213864	16.83%	1.844%
3	1.893	163	172	183	rVB	137726	184457	14.52%	1.591%
4	2.562	367	380	404	rBV2	290316	534558	42.07%	4.610%
5	2.768	439	444	445	rBV2	343	226	0.02%	0.002%
6	2.781	445	448	458	rVB4	1042	1310	0.10%	0.011%
7	2.900	481	485	489	rBV2	254	237	0.02%	0.002%
8	2.961	498	504	515	rBV3	556	954	0.08%	0.008%
9	3.047	521	531	541	rVB3	2275	4063	0.32%	0.035%
10	3.189	563	575	588	rBV2	2285	4892	0.38%	0.042%
11	3.256	592	596	601	rBV2	216	216	0.02%	0.002%
12	3.353	614	626	641	rVB2	8858	16438	1.29%	0.142%
13	3.417	641	646	648	rBV2	166	183	0.01%	0.002%
14	3.478	664	665	673	rVV	133	171	0.01%	0.001%
15	3.774	752	757	763	rBV2	139	201	0.02%	0.002%
16	3.871	774	787	803	rVB2	6187	13841	1.09%	0.119%
17	4.057	840	845	847	rBV2	191	172	0.01%	0.001%
18	4.189	881	886	892	rBV2	226	309	0.02%	0.003%
19	4.437	961	963	970	rVB2	196	247	0.02%	0.002%
20	4.668	1007	1035	1057	rBV2	368013	1124191	88.47%	9.695%
21	4.835	1084	1087	1090	rVB3	299	188	0.01%	0.002%
22	5.067	1139	1159	1181	rBV	224331	498533	39.23%	4.300%
23	5.205	1198	1202	1204	rBV	272	215	0.02%	0.002%
24	5.321	1219	1238	1254	rBV	67548	153154	12.05%	1.321%
25	5.481	1281	1288	1290	rBV2	327	282	0.02%	0.002%
26	5.729	1340	1365	1387	rBV2	475340	1270768	100.00%	10.960%
27	6.202	1506	1512	1513	rBV	217	243	0.02%	0.002%
28	6.253	1513	1528	1549	rVV	379135	709218	55.81%	6.117%
29	6.465	1591	1594	1600	rBV3	201	183	0.01%	0.002%
30	6.546	1604	1619	1641	rBV	509217	963124	75.79%	8.306%
31	6.694	1651	1665	1688	rVB	294304	573867	45.16%	4.949%
32	6.809	1696	1701	1702	rBV2	517	507	0.04%	0.004%
33	7.044	1760	1774	1777	rBV3	506	859	0.07%	0.007%
34	7.176	1811	1815	1817	rBV	712	615	0.05%	0.005%
35	7.472	1905	1907	1916	rVB2	202	215	0.02%	0.002%
36	7.568	1925	1937	1960	rBV	145373	252495	19.87%	2.178%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045224.D
 Acq On : 07 Oct 2021 21:52
 Operator : SY/MD
 Sample : M4023-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	7.684	1967	1973	1983	rVB5	666	1340	0.11%	0.012%
38	7.764	1992	1998	2001	rVB2	212	249	0.02%	0.002%
39	7.819	2011	2015	2018	rVB2	206	163	0.01%	0.001%
40	7.903	2026	2041	2056	rBV	571345	989313	77.85%	8.532%
41	7.973	2057	2063	2074	rVB2	8189	13184	1.04%	0.114%
42	8.124	2105	2110	2112	rBV	196	181	0.01%	0.002%
43	8.182	2116	2128	2150	rVV	101464	167905	13.21%	1.448%
44	8.333	2171	2175	2183	rVB3	398	537	0.04%	0.005%
45	8.404	2190	2197	2206	rVB4	1856	2657	0.21%	0.023%
46	8.478	2215	2220	2223	rVB2	398	417	0.03%	0.004%
47	8.565	2244	2247	2250	rVB	211	163	0.01%	0.001%
48	8.636	2255	2269	2304	rBV	409173	719968	56.66%	6.209%
49	8.864	2336	2340	2342	rBV2	234	210	0.02%	0.002%
50	8.903	2347	2352	2356	rVB2	166	184	0.01%	0.002%
51	8.941	2356	2364	2367	rBV2	248	363	0.03%	0.003%
52	9.012	2381	2386	2388	rBV2	205	219	0.02%	0.002%
53	9.086	2404	2409	2412	rBV	205	225	0.02%	0.002%
54	9.240	2453	2457	2461	rBV2	172	184	0.01%	0.002%
55	9.353	2488	2492	2498	rBV2	175	208	0.02%	0.002%
56	9.420	2498	2513	2549	rVV	539077	887117	69.81%	7.651%
57	9.575	2557	2561	2566	rVB2	288	333	0.03%	0.003%
58	9.620	2570	2575	2578	rBV2	189	176	0.01%	0.002%
59	9.700	2588	2600	2603	rBV4	1117	1497	0.12%	0.013%
60	9.796	2626	2630	2633	rBV2	216	206	0.02%	0.002%
61	9.996	2689	2692	2696	rBV	191	168	0.01%	0.001%
62	10.066	2709	2714	2717	rBV	228	277	0.02%	0.002%
63	10.144	2731	2738	2742	rBV2	214	295	0.02%	0.003%
64	10.330	2792	2796	2799	rBV	194	175	0.01%	0.002%
65	10.517	2850	2854	2858	rBV2	224	197	0.02%	0.002%
66	10.674	2892	2903	2911	rBV4	1223	1932	0.15%	0.017%
67	10.761	2917	2930	2950	rBV	417443	660973	52.01%	5.700%
68	10.867	2960	2963	2966	rVV2	245	189	0.01%	0.002%
69	10.896	2969	2972	2976	rVB2	261	191	0.02%	0.002%
70	11.156	3049	3053	3055	rBV	225	168	0.01%	0.001%
71	11.214	3068	3071	3076	rVB	234	217	0.02%	0.002%
72	11.240	3076	3079	3082	rBV2	193	185	0.01%	0.002%
73	11.414	3124	3133	3135	rBV	250	384	0.03%	0.003%
74	11.472	3147	3151	3160	rVV	805	941	0.07%	0.008%
75	11.552	3172	3176	3179	rBV2	184	161	0.01%	0.001%
76	11.632	3198	3201	3205	rBV	273	228	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045224.D
 Acq On : 07 Oct 2021 21:52
 Operator : SY/MD
 Sample : M4023-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.684	3214	3217	3219	rBV	205	164	0.01%	0.001%
78	11.816	3245	3258	3277	rVV	485920	767326	60.38%	6.618%
79	11.935	3292	3295	3297	rBV	282	174	0.01%	0.002%
80	12.021	3318	3322	3326	rBV2	167	199	0.02%	0.002%
81	12.057	3328	3333	3335	rBV2	178	163	0.01%	0.001%
82	12.153	3358	3363	3364	rBV	329	300	0.02%	0.003%
83	12.195	3364	3376	3396	rVV	507906	819579	64.49%	7.068%
84	12.317	3410	3414	3416	rBV	248	198	0.02%	0.002%
85	12.433	3447	3450	3458	rBV2	176	274	0.02%	0.002%
86	12.568	3486	3492	3496	rBV2	271	398	0.03%	0.003%
87	12.854	3575	3581	3586	rBV2	195	342	0.03%	0.003%
88	12.938	3605	3607	3612	rBV2	182	182	0.01%	0.002%
89	13.041	3635	3639	3645	rVB2	283	356	0.03%	0.003%
90	13.070	3645	3648	3652	rBV2	229	251	0.02%	0.002%
91	13.176	3678	3681	3684	rBV	402	351	0.03%	0.003%
92	13.478	3771	3775	3778	rBV	424	381	0.03%	0.003%
93	14.217	4002	4005	4010	rBV	246	223	0.02%	0.002%
94	14.266	4015	4020	4024	rBV	269	327	0.03%	0.003%
95	14.420	4065	4068	4072	rBV2	315	187	0.01%	0.002%
96	14.545	4105	4107	4110	rBV2	306	198	0.02%	0.002%
97	14.639	4133	4136	4137	rBV2	309	172	0.01%	0.001%
98	14.796	4182	4185	4187	rBV2	337	239	0.02%	0.002%
99	15.195	4306	4309	4311	rBV3	266	188	0.01%	0.002%
100	15.381	4362	4367	4369	rBV3	292	308	0.02%	0.003%




Sum of corrected areas: 11595055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045224.D
Acq On : 07 Oct 2021 21:52
Operator : SY/MD
Sample : M4023-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

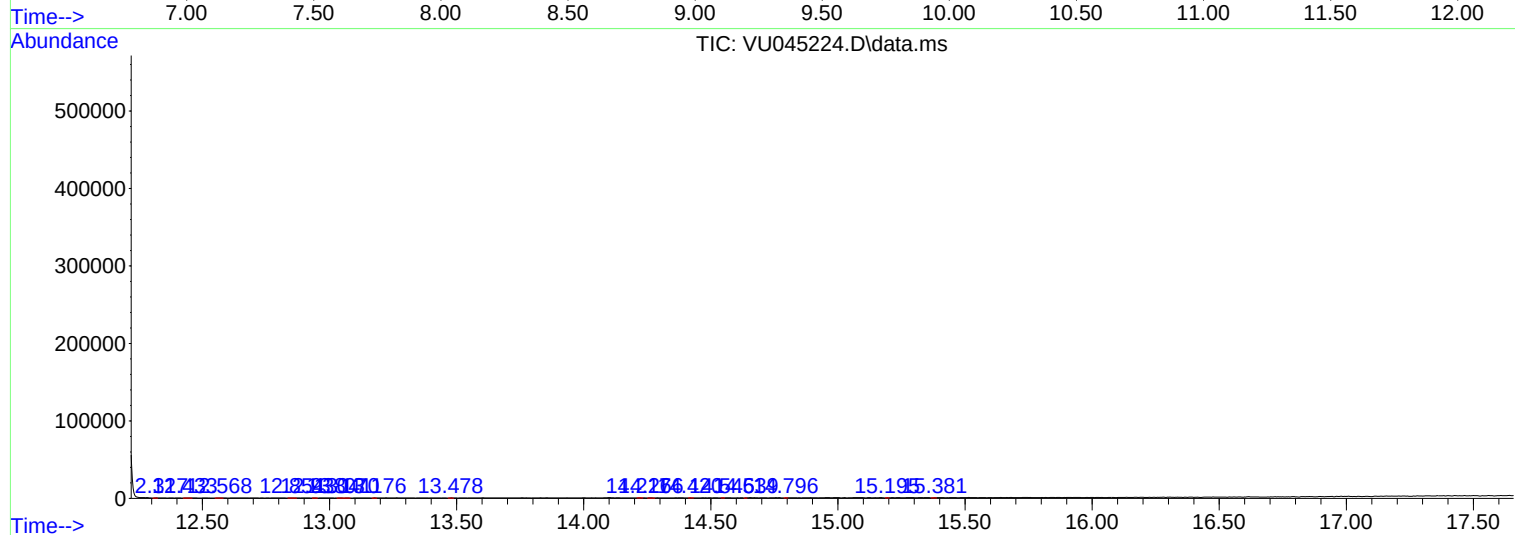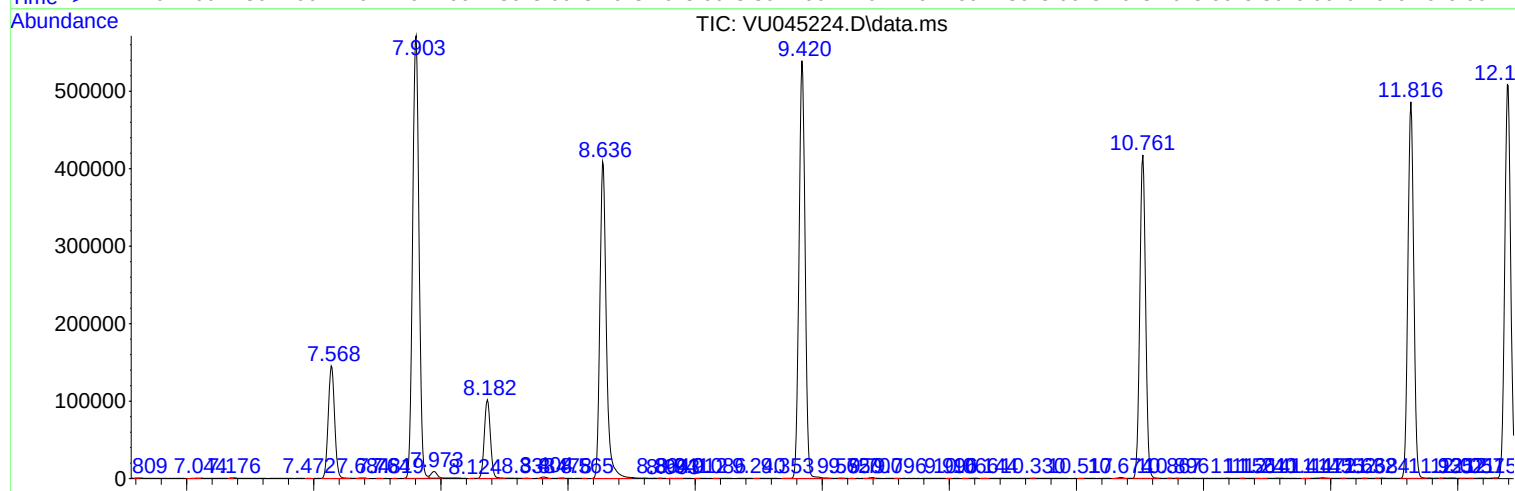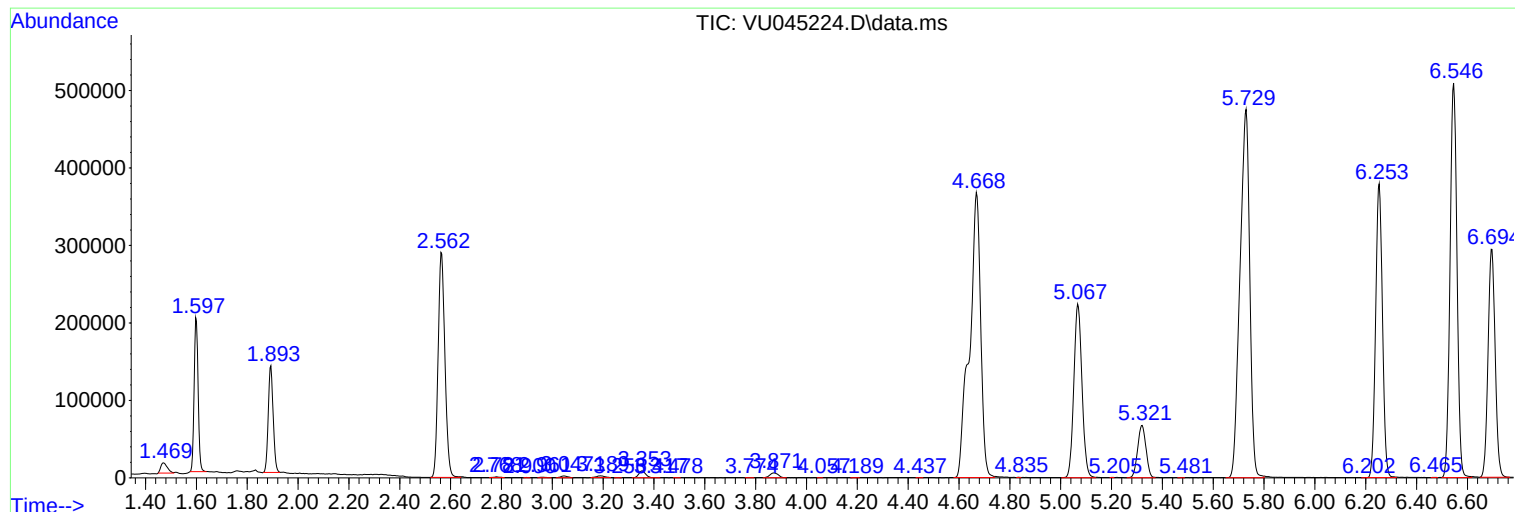

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045224.D
Acq On : 07 Oct 2021 21:52
Operator : SY/MD
Sample : M4023-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045224.D
Acq On : 07 Oct 2021 21:52
Operator : SY/MD
Sample : M4023-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------