

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045225.D
 Acq On : 07 Oct 2021 22:16
 Operator : SY/MD
 Sample : M4023-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.469	34	40	52	rBV2	12584	22591	1.74%	0.206%
2	1.597	73	80	96	rBV	201296	219783	16.98%	2.000%
3	1.887	162	170	190	rVB	141650	194598	15.03%	1.770%
4	2.562	367	380	399	rBV2	277531	490114	37.86%	4.459%
5	2.787	440	450	460	rVB3	1327	2369	0.18%	0.022%
6	2.925	489	493	495	rBV2	199	183	0.01%	0.002%
7	3.044	518	530	547	rBV	31646	61182	4.73%	0.557%
8	3.192	563	576	589	rVB3	2877	6893	0.53%	0.063%
9	3.350	617	625	628	rBV3	588	701	0.05%	0.006%
10	3.411	636	644	647	rBV	317	441	0.03%	0.004%
11	3.559	687	690	692	rBV	198	165	0.01%	0.002%
12	3.793	757	763	765	rBV	184	241	0.02%	0.002%
13	3.871	773	787	802	rBV	3145	7220	0.56%	0.066%
14	3.925	802	804	808	rVB2	226	183	0.01%	0.002%
15	4.018	829	833	835	rBV2	217	198	0.02%	0.002%
16	4.099	856	858	862	rBV2	183	135	0.01%	0.001%
17	4.192	883	887	891	rBV2	224	220	0.02%	0.002%
18	4.305	918	922	927	rBV	171	186	0.01%	0.002%
19	4.629	1007	1023	1056	rBV2	141024	432547	33.41%	3.935%
20	5.067	1142	1159	1181	rBV	225828	496402	38.34%	4.516%
21	5.192	1195	1198	1203	rBV2	241	284	0.02%	0.003%
22	5.321	1222	1238	1253	rVB2	25414	56516	4.37%	0.514%
23	5.430	1265	1272	1275	rBV2	202	282	0.02%	0.003%
24	5.591	1317	1322	1324	rBV	153	134	0.01%	0.001%
25	5.729	1343	1365	1391	rBV2	483584	1294640	100.00%	11.778%
26	5.967	1436	1439	1444	rBV2	263	252	0.02%	0.002%
27	6.044	1460	1463	1466	rVB2	269	192	0.01%	0.002%
28	6.076	1470	1473	1476	rVB2	256	175	0.01%	0.002%
29	6.115	1480	1485	1489	rBV2	490	480	0.04%	0.004%
30	6.144	1491	1494	1497	rVB	270	194	0.01%	0.002%
31	6.253	1513	1528	1546	rBV	378587	704664	54.43%	6.411%
32	6.462	1589	1593	1596	rVB3	324	227	0.02%	0.002%
33	6.481	1596	1599	1603	rBV2	256	172	0.01%	0.002%
34	6.546	1603	1619	1637	rBV	545453	1019034	78.71%	9.271%
35	6.694	1651	1665	1686	rBV	305604	586879	45.33%	5.339%
36	6.780	1691	1692	1695	rVB2	408	200	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045225.D
 Acq On : 07 Oct 2021 22:16
 Operator : SY/MD
 Sample : M4023-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.809	1695	1701	1707	rBV3	1091	1254	0.10%	0.011%
38	6.896	1722	1728	1731	rBV	221	280	0.02%	0.003%
39	7.047	1771	1775	1776	rVV	354	238	0.02%	0.002%
40	7.060	1776	1779	1784	rVB	349	298	0.02%	0.003%
41	7.108	1791	1794	1800	rVB2	242	283	0.02%	0.003%
42	7.144	1800	1805	1808	rBV	294	308	0.02%	0.003%
43	7.173	1811	1814	1815	rBV	697	380	0.03%	0.003%
44	7.247	1833	1837	1839	rBV2	226	159	0.01%	0.001%
45	7.259	1839	1841	1845	rVB2	178	135	0.01%	0.001%
46	7.285	1845	1849	1852	rBV2	209	170	0.01%	0.002%
47	7.356	1864	1871	1874	rBV	145	165	0.01%	0.002%
48	7.382	1874	1879	1883	rBV2	243	265	0.02%	0.002%
49	7.462	1899	1904	1910	rBV2	207	319	0.02%	0.003%
50	7.494	1910	1914	1919	rVB2	211	173	0.01%	0.002%
51	7.568	1924	1937	1957	rVV	145787	251839	19.45%	2.291%
52	7.649	1960	1962	1965	rVB3	235	137	0.01%	0.001%
53	7.684	1970	1973	1985	rVB3	673	999	0.08%	0.009%
54	7.819	2011	2015	2017	rBV	165	168	0.01%	0.002%
55	7.903	2026	2041	2056	rBV	592579	1001501	77.36%	9.112%
56	7.970	2056	2062	2076	rVB2	8352	14314	1.11%	0.130%
57	8.079	2093	2096	2099	rVB	310	170	0.01%	0.002%
58	8.182	2116	2128	2141	rVV	103228	169940	13.13%	1.546%
59	8.404	2188	2197	2204	rBV3	1808	2255	0.17%	0.021%
60	8.485	2218	2222	2227	rBV4	395	379	0.03%	0.003%
61	8.578	2247	2251	2256	rBV2	203	246	0.02%	0.002%
62	8.639	2256	2270	2301	rBV	417893	743691	57.44%	6.766%
63	8.957	2366	2369	2372	rVB2	224	153	0.01%	0.001%
64	8.983	2372	2377	2379	rBV	187	159	0.01%	0.001%
65	9.060	2393	2401	2407	rVV2	206	381	0.03%	0.003%
66	9.086	2407	2409	2413	rVB2	179	150	0.01%	0.001%
67	9.179	2435	2438	2444	rBV	235	187	0.01%	0.002%
68	9.420	2499	2513	2537	rBV	544971	885536	68.40%	8.057%
69	9.575	2555	2561	2567	rVB3	766	1096	0.08%	0.010%
70	9.603	2567	2570	2573	rBV2	185	166	0.01%	0.002%
71	9.697	2587	2599	2611	rVB2	3912	5820	0.45%	0.053%
72	9.819	2631	2637	2640	rBV2	260	336	0.03%	0.003%
73	9.867	2649	2652	2660	rBV2	156	159	0.01%	0.001%
74	9.912	2661	2666	2667	rBV2	399	304	0.02%	0.003%
75	10.105	2719	2726	2733	rVB3	1466	1821	0.14%	0.017%
76	10.288	2775	2783	2784	rBV	255	327	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045225.D
 Acq On : 07 Oct 2021 22:16
 Operator : SY/MD
 Sample : M4023-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.365	2802	2807	2808	rBV2	152	132	0.01%	0.001%
78	10.510	2849	2852	2859	rVB2	180	183	0.01%	0.002%
79	10.645	2890	2894	2896	rBV2	151	144	0.01%	0.001%
80	10.674	2896	2903	2910	rVV3	1374	1672	0.13%	0.015%
81	10.761	2917	2930	2955	rVB	432429	684907	52.90%	6.231%
82	11.291	3091	3095	3097	rBV2	175	172	0.01%	0.002%
83	11.462	3141	3148	3149	rBV2	615	613	0.05%	0.006%
84	11.636	3194	3202	3210	rVB3	1686	2297	0.18%	0.021%
85	11.816	3245	3258	3278	rBV	496411	768983	59.40%	6.996%
86	11.938	3291	3296	3297	rBV3	435	403	0.03%	0.004%
87	11.976	3305	3308	3315	rVB3	648	666	0.05%	0.006%
88	12.041	3323	3328	3331	rBV2	213	195	0.02%	0.002%
89	12.195	3363	3376	3400	rBV	517252	841449	64.99%	7.655%
90	12.677	3522	3526	3528	rBV2	261	229	0.02%	0.002%
91	12.722	3538	3540	3543	rBV	208	132	0.01%	0.001%
92	13.057	3640	3644	3648	rBV	269	219	0.02%	0.002%
93	13.295	3715	3718	3720	rBV2	218	130	0.01%	0.001%
94	14.008	3936	3940	3946	rBV2	245	298	0.02%	0.003%
95	14.314	4032	4035	4038	rBV2	204	149	0.01%	0.001%
96	14.401	4060	4062	4066	rBV	247	148	0.01%	0.001%
97	14.497	4089	4092	4094	rBV	234	178	0.01%	0.002%
98	14.539	4102	4105	4107	rBV	183	138	0.01%	0.001%
99	14.555	4107	4110	4113	rVV2	399	294	0.02%	0.003%
100	16.076	4581	4583	4590	rBV3	474	488	0.04%	0.004%



Sum of corrected areas: 10991557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045225.D
Acq On : 07 Oct 2021 22:16
Operator : SY/MD
Sample : M4023-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

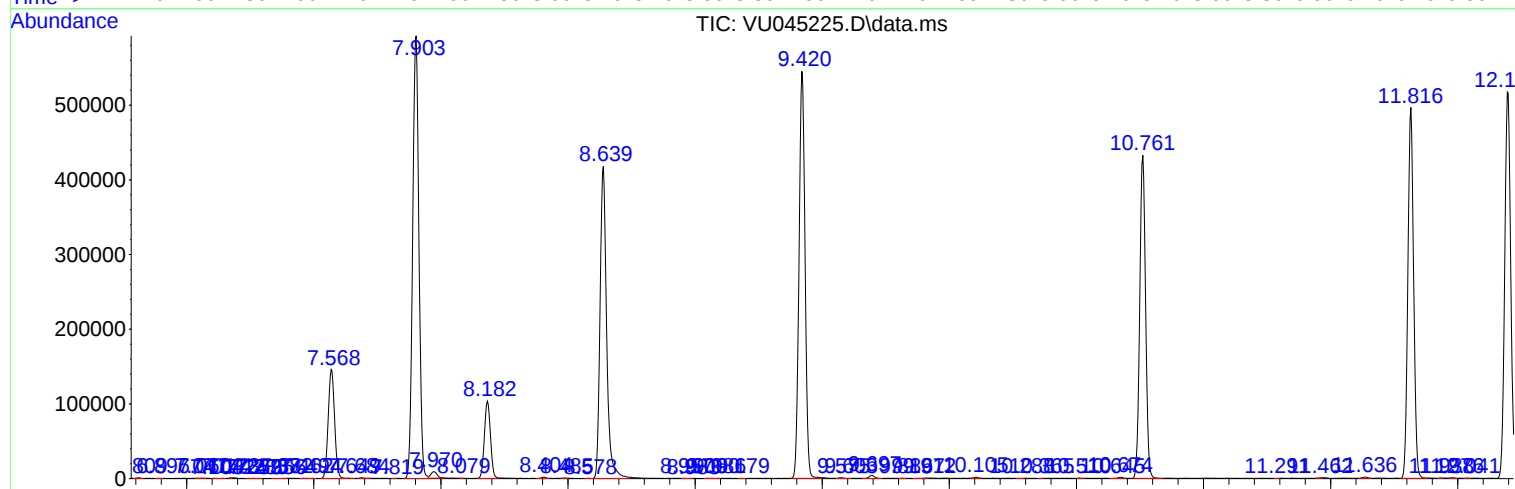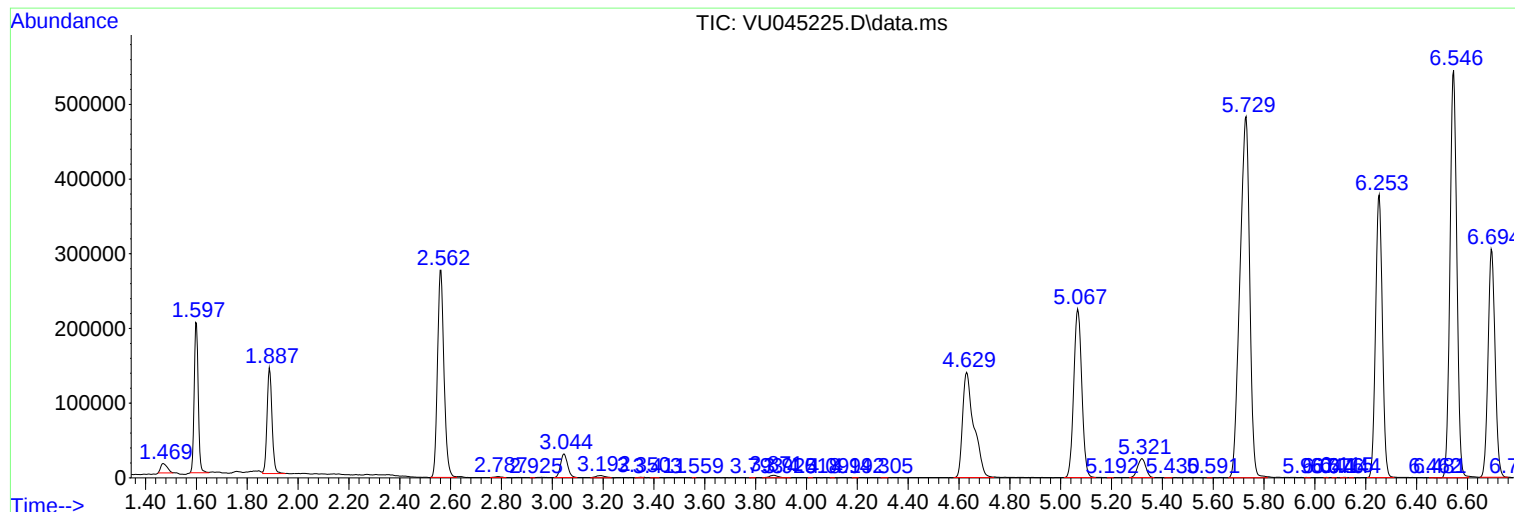

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045225.D
Acq On : 07 Oct 2021 22:16
Operator : SY/MD
Sample : M4023-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045225.D
Acq On : 07 Oct 2021 22:16
Operator : SY/MD
Sample : M4023-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
