

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045226.D
 Acq On : 07 Oct 2021 22:40
 Operator : SY/MD
 Sample : M4138-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	34	41	52	rBV	11452	20398	1.57%	0.208%
2	1.597	73	80	98	rVB	182436	197200	15.16%	2.009%
3	1.893	164	172	185	rBV	134167	178667	13.73%	1.821%
4	2.562	367	380	396	rVV	253974	429292	32.99%	4.374%
5	2.636	397	403	420	rVB3	5795	10437	0.80%	0.106%
6	2.777	435	447	464	rBV2	6830	14009	1.08%	0.143%
7	2.893	480	483	487	rBV	209	164	0.01%	0.002%
8	2.961	497	504	515	rVB4	650	1154	0.09%	0.012%
9	3.047	525	531	536	rVB2	784	878	0.07%	0.009%
10	3.195	562	577	588	rVV2	3124	6684	0.51%	0.068%
11	3.308	609	612	616	rBV2	190	183	0.01%	0.002%
12	3.433	645	651	653	rBV	215	181	0.01%	0.002%
13	3.453	653	657	662	rBV2	193	220	0.02%	0.002%
14	3.514	673	676	680	rBV2	187	214	0.02%	0.002%
15	3.565	688	692	695	rVV2	171	155	0.01%	0.002%
16	3.700	731	734	739	rVB2	153	167	0.01%	0.002%
17	3.755	747	751	760	rBV2	120	188	0.01%	0.002%
18	3.822	768	772	780	rBV2	172	301	0.02%	0.003%
19	3.951	810	812	817	rVB	253	172	0.01%	0.002%
20	3.986	817	823	826	rBV2	216	281	0.02%	0.003%
21	4.298	917	920	925	rVB	146	172	0.01%	0.002%
22	4.395	943	950	953	rBV2	139	191	0.01%	0.002%
23	4.568	997	1004	1007	rBV2	189	309	0.02%	0.003%
24	4.629	1007	1023	1057	rBV	147542	350501	26.94%	3.571%
25	4.816	1072	1081	1094	rVB2	4604	9887	0.76%	0.101%
26	5.012	1135	1142	1143	rBV2	257	277	0.02%	0.003%
27	5.067	1143	1159	1183	rVV	230143	499865	38.42%	5.093%
28	5.150	1183	1185	1193	rVV2	328	402	0.03%	0.004%
29	5.289	1222	1228	1230	rBV2	678	818	0.06%	0.008%
30	5.382	1252	1257	1260	rBV2	184	185	0.01%	0.002%
31	5.417	1264	1268	1274	rBV2	163	210	0.02%	0.002%
32	5.507	1289	1296	1298	rBV2	195	245	0.02%	0.002%
33	5.543	1305	1307	1310	rBV	208	152	0.01%	0.002%
34	5.568	1310	1315	1317	rVV	153	145	0.01%	0.001%
35	5.729	1343	1365	1392	rBV2	485796	1301118	100.00%	13.258%
36	6.118	1481	1486	1487	rBV2	394	325	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045226.D
 Acq On : 07 Oct 2021 22:40
 Operator : SY/MD
 Sample : M4138-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.163	1496	1500	1505	rVB3	591	595	0.05%	0.006%
38	6.253	1513	1528	1545	rBV	375789	701350	53.90%	7.146%
39	6.417	1576	1579	1582	rBV2	197	144	0.01%	0.001%
40	6.533	1605	1615	1627	rVB5	8378	15569	1.20%	0.159%
41	6.694	1651	1665	1685	rBV	310182	598851	46.03%	6.102%
42	6.819	1694	1704	1707	rBV5	791	1232	0.09%	0.013%
43	6.957	1740	1747	1751	rBV2	205	298	0.02%	0.003%
44	6.980	1751	1754	1761	rVV	201	229	0.02%	0.002%
45	7.009	1761	1763	1768	rVV2	156	156	0.01%	0.002%
46	7.047	1768	1775	1784	rVB3	644	1005	0.08%	0.010%
47	7.089	1786	1788	1792	rBV	162	148	0.01%	0.002%
48	7.153	1805	1808	1810	rBV	189	152	0.01%	0.002%
49	7.179	1810	1816	1823	rVV5	1530	2592	0.20%	0.026%
50	7.269	1841	1844	1852	rVB2	222	322	0.02%	0.003%
51	7.340	1862	1866	1871	rBV2	195	230	0.02%	0.002%
52	7.472	1902	1907	1913	rVB	192	263	0.02%	0.003%
53	7.568	1924	1937	1958	rBV	165830	289096	22.22%	2.946%
54	7.642	1958	1960	1964	rVB3	275	159	0.01%	0.002%
55	7.681	1968	1972	1973	rBV	475	302	0.02%	0.003%
56	7.716	1980	1983	1990	rVB4	797	933	0.07%	0.010%
57	7.845	2019	2023	2027	rBV2	202	246	0.02%	0.003%
58	7.903	2027	2041	2056	rVV	595498	1003520	77.13%	10.225%
59	7.973	2056	2063	2078	rVB2	9226	15486	1.19%	0.158%
60	8.118	2104	2108	2111	rBV	175	185	0.01%	0.002%
61	8.182	2116	2128	2143	rBV	118402	193233	14.85%	1.969%
62	8.263	2147	2153	2165	rVB2	2833	4963	0.38%	0.051%
63	8.340	2174	2177	2182	rVB2	394	361	0.03%	0.004%
64	8.475	2213	2219	2228	rVB3	1015	1511	0.12%	0.015%
65	8.636	2255	2269	2312	rBV	434336	764335	58.74%	7.788%
66	8.829	2327	2329	2335	rVB	410	341	0.03%	0.003%
67	8.854	2335	2337	2340	rBV	274	152	0.01%	0.002%
68	8.960	2364	2370	2375	rBV2	263	336	0.03%	0.003%
69	8.989	2375	2379	2382	rVB	184	154	0.01%	0.002%
70	9.066	2399	2403	2412	rBV2	589	925	0.07%	0.009%
71	9.346	2482	2490	2499	rBV2	2701	4155	0.32%	0.042%
72	9.420	2499	2513	2538	rBV	539647	872666	67.07%	8.892%
73	9.565	2555	2558	2560	rBV2	207	149	0.01%	0.002%
74	9.629	2572	2578	2582	rBV2	175	293	0.02%	0.003%
75	9.697	2593	2599	2606	rVB2	704	1039	0.08%	0.011%
76	9.922	2665	2669	2675	rVB2	565	687	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
 Data File : VU045226.D
 Acq On : 07 Oct 2021 22:40
 Operator : SY/MD
 Sample : M4138-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW7F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	10.095	2719	2723	2726	rBV2	300	279	0.02%	0.003%
78	10.275	2776	2779	2785	rVB	216	180	0.01%	0.002%
79	10.636	2888	2891	2893	rBV	197	145	0.01%	0.001%
80	10.674	2896	2903	2910	rVV3	2524	3340	0.26%	0.034%
81	10.761	2916	2930	2946	rBV	432835	688284	52.90%	7.013%
82	10.867	2959	2963	2968	rBV3	608	753	0.06%	0.008%
83	10.896	2968	2972	2980	rVV2	470	735	0.06%	0.007%
84	10.935	2981	2984	2988	rVV2	265	177	0.01%	0.002%
85	11.124	3038	3043	3046	rBV4	555	661	0.05%	0.007%
86	11.288	3090	3094	3097	rVV2	201	174	0.01%	0.002%
87	11.462	3139	3148	3161	rBV5	1759	3054	0.23%	0.031%
88	11.700	3214	3222	3227	rBV3	1026	1171	0.09%	0.012%
89	11.816	3245	3258	3274	rBV	484516	755836	58.09%	7.702%
90	11.976	3303	3308	3317	rVB4	1561	2314	0.18%	0.024%
91	12.066	3329	3336	3347	rVV6	1400	2608	0.20%	0.027%
92	12.195	3363	3376	3395	rBV	528436	847566	65.14%	8.636%
93	12.336	3415	3420	3429	rVB5	698	879	0.07%	0.009%
94	12.404	3439	3441	3443	rBV	309	197	0.02%	0.002%
95	13.336	3726	3731	3734	rBV2	223	233	0.02%	0.002%
96	13.574	3800	3805	3808	rBV	271	315	0.02%	0.003%
97	14.372	4050	4053	4058	rBV2	221	252	0.02%	0.003%
98	14.555	4107	4110	4113	rBV	315	222	0.02%	0.002%
99	14.809	4185	4189	4191	rBV2	337	265	0.02%	0.003%
100	14.967	4235	4238	4241	rBV2	328	224	0.02%	0.002%


Sum of corrected areas: 9813974

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045226.D
Acq On : 07 Oct 2021 22:40
Operator : SY/MD
Sample : M4138-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

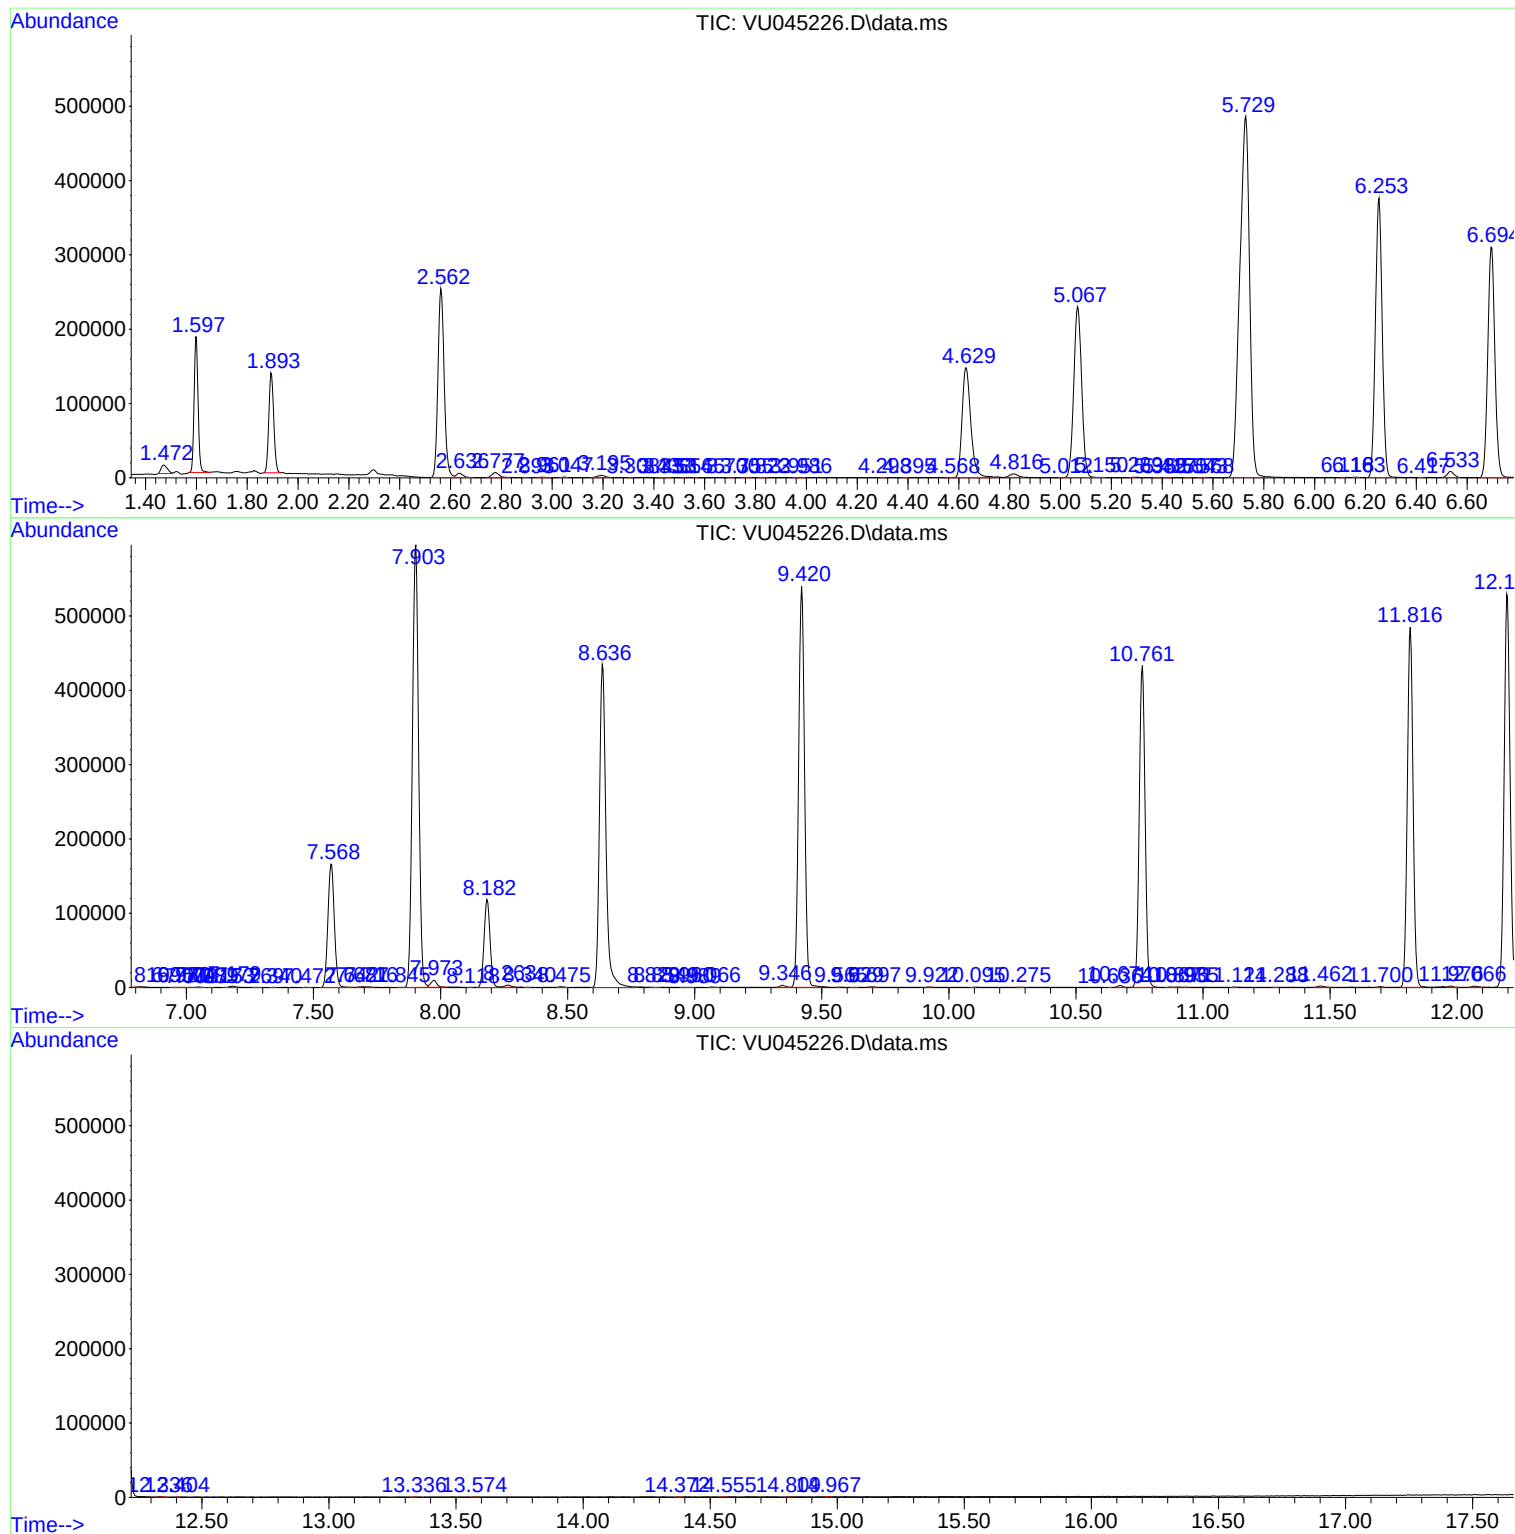

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045226.D
Acq On : 07 Oct 2021 22:40
Operator : SY/MD
Sample : M4138-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100721\
Data File : VU045226.D
Acq On : 07 Oct 2021 22:40
Operator : SY/MD
Sample : M4138-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW7F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------