

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100818\
 Data File : VU027511.D
 Acq On : 08 Oct 2018 19:57
 Operator : MD/SY
 Sample : J5298-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E62W4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	65	70	81	rBV	84527	85174	12.51%	1.611%
2	1.681	152	158	175	rVB	68533	88062	12.94%	1.666%
3	2.273	332	342	355	rBV	133787	201800	29.64%	3.817%
4	2.443	388	395	413	rVB	3981	7326	1.08%	0.139%
5	2.624	447	451	454	rBV3	272	262	0.04%	0.005%
6	2.675	464	467	472	rBV	214	193	0.03%	0.004%
7	2.697	472	474	476	rBV	239	107	0.02%	0.002%
8	2.839	510	518	526	rVB	888	1565	0.23%	0.030%
9	2.919	540	543	549	rVB2	253	225	0.03%	0.004%
10	2.958	549	555	559	rBV	155	203	0.03%	0.004%
11	3.177	620	623	626	rBV3	423	345	0.05%	0.007%
12	3.472	710	715	717	rBV	127	121	0.02%	0.002%
13	3.572	743	746	747	rBV	90	51	0.01%	0.001%
14	3.617	758	760	761	rBV	106	41	0.01%	0.001%
15	3.714	783	790	796	rBV	131	206	0.03%	0.004%
16	3.765	803	806	808	rBV	92	50	0.01%	0.001%
17	3.906	848	850	852	rBV	131	43	0.01%	0.001%
18	3.993	875	877	879	rBV	135	57	0.01%	0.001%
19	4.054	894	896	900	rVB2	155	100	0.01%	0.002%
20	4.180	920	935	965	rBV	78579	211655	31.09%	4.003%
21	4.476	1024	1027	1029	rVB2	161	85	0.01%	0.002%
22	4.524	1037	1042	1047	rVB3	270	319	0.05%	0.006%
23	4.556	1049	1052	1055	rBV2	110	81	0.01%	0.002%
24	4.572	1055	1057	1059	rVB	142	76	0.01%	0.001%
25	4.591	1059	1063	1065	rBV	75	52	0.01%	0.001%
26	4.652	1065	1082	1110	rBV	112170	267969	39.36%	5.068%
27	4.794	1123	1126	1127	rBV	236	91	0.01%	0.002%
28	4.807	1127	1130	1132	rVB2	187	99	0.01%	0.002%
29	4.881	1149	1153	1154	rBV2	467	301	0.04%	0.006%
30	4.996	1187	1189	1190	rBV2	135	60	0.01%	0.001%
31	5.025	1194	1198	1202	rBV	85	76	0.01%	0.001%
32	5.157	1238	1239	1240	rBV	113	34	0.00%	0.001%
33	5.196	1247	1251	1255	rVB	134	108	0.02%	0.002%
34	5.218	1255	1258	1265	rBV	168	121	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100818\
 Data File : VU027511.D
 Acq On : 08 Oct 2018 19:57
 Operator : MD/SY
 Sample : J5298-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E62W4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

35	5.260	1267	1271	1273	rBV	75	61	0.01%	0.001%
36	5.344	1273	1297	1328	rBV2	221191	680758	100.00%	12.876%
37	5.546	1358	1360	1365	rVB	219	146	0.02%	0.003%
38	5.614	1379	1381	1385	rVB	195	115	0.02%	0.002%
39	5.636	1385	1388	1393	rBV	75	80	0.01%	0.002%
40	5.746	1420	1422	1426	rVB	83	49	0.01%	0.001%
41	5.794	1426	1437	1440	rBV2	1035	1599	0.23%	0.030%
42	5.890	1453	1467	1502	rBV	223043	447638	65.76%	8.466%
43	6.093	1527	1530	1531	rBV	166	89	0.01%	0.002%
44	6.167	1551	1553	1555	rBV	285	139	0.02%	0.003%
45	6.215	1567	1568	1572	rVB	142	41	0.01%	0.001%
46	6.250	1574	1579	1583	rBV2	409	433	0.06%	0.008%
47	6.334	1591	1605	1628	rBV	160342	329140	48.35%	6.225%
48	6.578	1679	1681	1683	rVB	177	77	0.01%	0.001%
49	6.591	1683	1685	1687	rBV	148	61	0.01%	0.001%
50	6.614	1687	1692	1698	rVV	106	135	0.02%	0.003%
51	6.639	1698	1700	1703	rVB	99	52	0.01%	0.001%
52	6.659	1703	1706	1707	rBV	62	37	0.01%	0.001%
53	6.778	1741	1743	1744	rVB	105	40	0.01%	0.001%
54	6.797	1745	1749	1750	rBV	268	162	0.02%	0.003%
55	6.829	1750	1759	1769	rBV3	5712	10026	1.47%	0.190%
56	6.897	1778	1780	1781	rBV3	98	39	0.01%	0.001%
57	6.935	1789	1792	1794	rBV	100	62	0.01%	0.001%
58	6.984	1799	1807	1810	rBV	144	163	0.02%	0.003%
59	7.022	1816	1819	1826	rVB	160	103	0.02%	0.002%
60	7.170	1863	1865	1866	rVB	111	41	0.01%	0.001%
61	7.231	1872	1884	1909	rBV	82688	153073	22.49%	2.895%
62	7.340	1917	1918	1922	rVB2	248	132	0.02%	0.002%
63	7.395	1926	1935	1947	rVB3	5034	9192	1.35%	0.174%
64	7.472	1955	1959	1961	rBV	142	80	0.01%	0.002%
65	7.569	1976	1989	2004	rBV	270545	477185	70.10%	9.025%
66	7.717	2034	2035	2039	rVB	162	58	0.01%	0.001%
67	7.736	2039	2041	2045	rBV	330	219	0.03%	0.004%
68	7.797	2057	2060	2062	rVB	162	66	0.01%	0.001%
69	7.810	2062	2064	2066	rVB	103	58	0.01%	0.001%
70	7.852	2066	2077	2096	rBV	59596	102941	15.12%	1.947%
71	7.951	2106	2108	2110	rBV	279	147	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100818\
 Data File : VU027511.D
 Acq On : 08 Oct 2018 19:57
 Operator : MD/SY
 Sample : J5298-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E62W4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis

72	8.051	2136	2139	2142	rBV2	179	119	0.02%	0.002%
73	8.102	2152	2155	2157	rBV	181	103	0.02%	0.002%
74	8.183	2168	2180	2188	rBV	4415	9782	1.44%	0.185%
75	8.311	2211	2220	2252	rVB	241584	425911	62.56%	8.055%
76	8.614	2310	2314	2316	rBV	246	152	0.02%	0.003%
77	8.871	2392	2394	2395	rBV	126	55	0.01%	0.001%
78	8.948	2416	2418	2424	rVB	143	93	0.01%	0.002%
79	9.003	2432	2435	2436	rBV	85	53	0.01%	0.001%
80	9.090	2450	2462	2485	rBV	322559	535706	78.69%	10.132%
81	9.308	2527	2530	2532	rBV	167	117	0.02%	0.002%
82	9.366	2542	2548	2553	rBV4	1674	2122	0.31%	0.040%
83	9.411	2560	2562	2565	rBV	134	113	0.02%	0.002%
84	9.562	2606	2609	2611	rBV	200	117	0.02%	0.002%
85	9.659	2636	2639	2645	rVB	284	205	0.03%	0.004%
86	9.697	2647	2651	2653	rBV2	162	111	0.02%	0.002%
87	9.826	2689	2691	2695	rBV	172	117	0.02%	0.002%
88	9.958	2731	2732	2734	rBV	93	39	0.01%	0.001%
89	9.987	2740	2741	2744	rBV	121	31	0.00%	0.001%
90	10.038	2753	2757	2758	rBV	222	152	0.02%	0.003%
91	10.093	2771	2774	2777	rBV	237	193	0.03%	0.004%
92	10.134	2785	2787	2788	rBV	160	64	0.01%	0.001%
93	10.434	2867	2880	2899	rBV	223287	352881	51.84%	6.674%
94	10.578	2921	2925	2927	rBV2	207	129	0.02%	0.002%
95	10.614	2927	2936	2948	rVB3	3647	7456	1.10%	0.141%
96	10.893	3020	3023	3026	rBV2	193	126	0.02%	0.002%
97	11.327	3155	3158	3163	rBV2	334	344	0.05%	0.007%
98	11.485	3194	3207	3225	rBV	283270	446650	65.61%	8.448%
99	11.668	3261	3264	3266	rBV	246	169	0.02%	0.003%
100	11.861	3311	3324	3342	rBV	264230	422604	62.08%	7.993%


Sum of corrected areas: 5287209

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100818\
Data File : VU027511.D
Acq On : 08 Oct 2018 19:57
Operator : MD/SY
Sample : J5298-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E62W4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

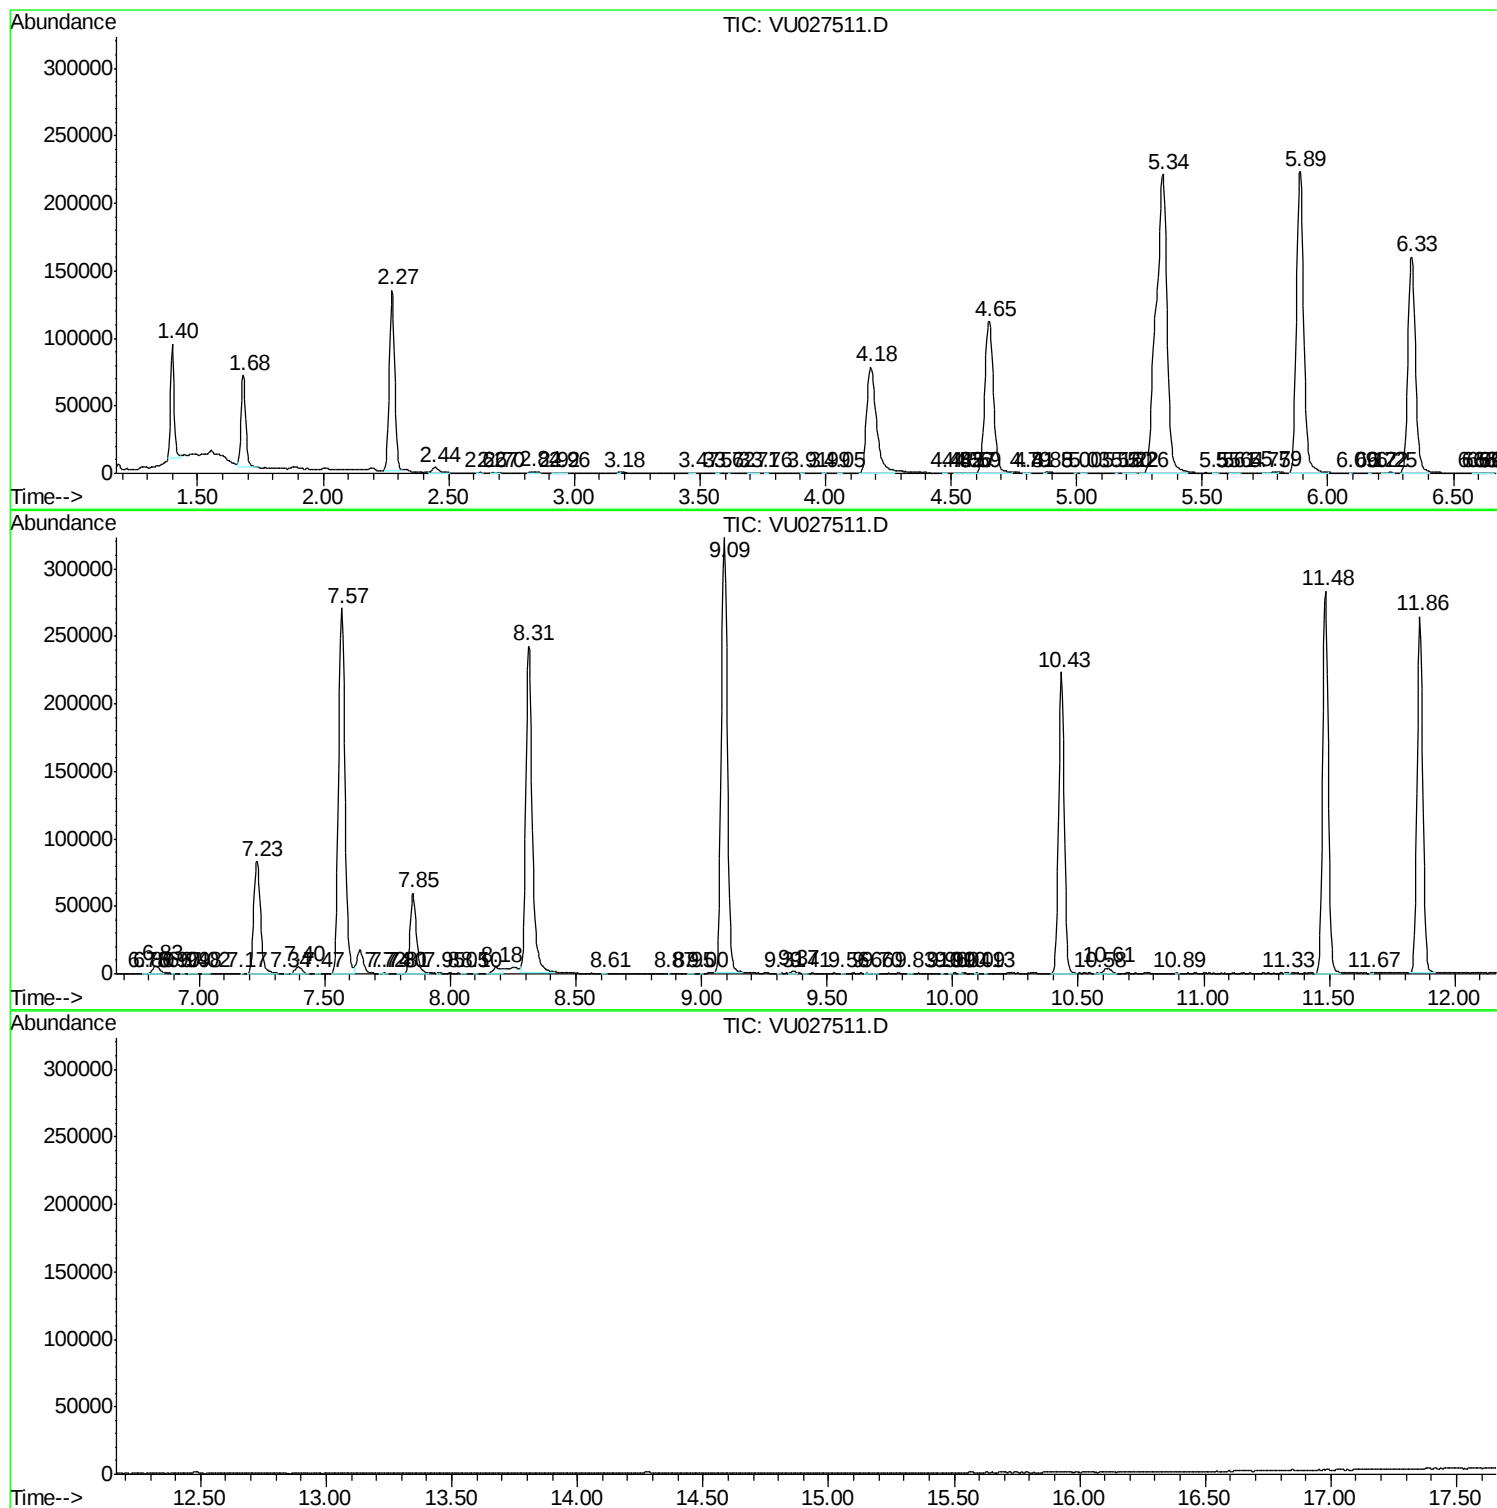

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100818\
Data File : VU027511.D
Acq On : 08 Oct 2018 19:57
Operator : MD/SY
Sample : J5298-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E62W4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU100818\
Data File : VU027511.D
Acq On : 08 Oct 2018 19:57
Operator : MD/SY
Sample : J5298-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E62W4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc