


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100818\
 Data File : VU027486.D
 Acq On : 08 Oct 2018 09:31
 Operator : MD/SY
 Sample : BFB40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 10 08:24:11 2018

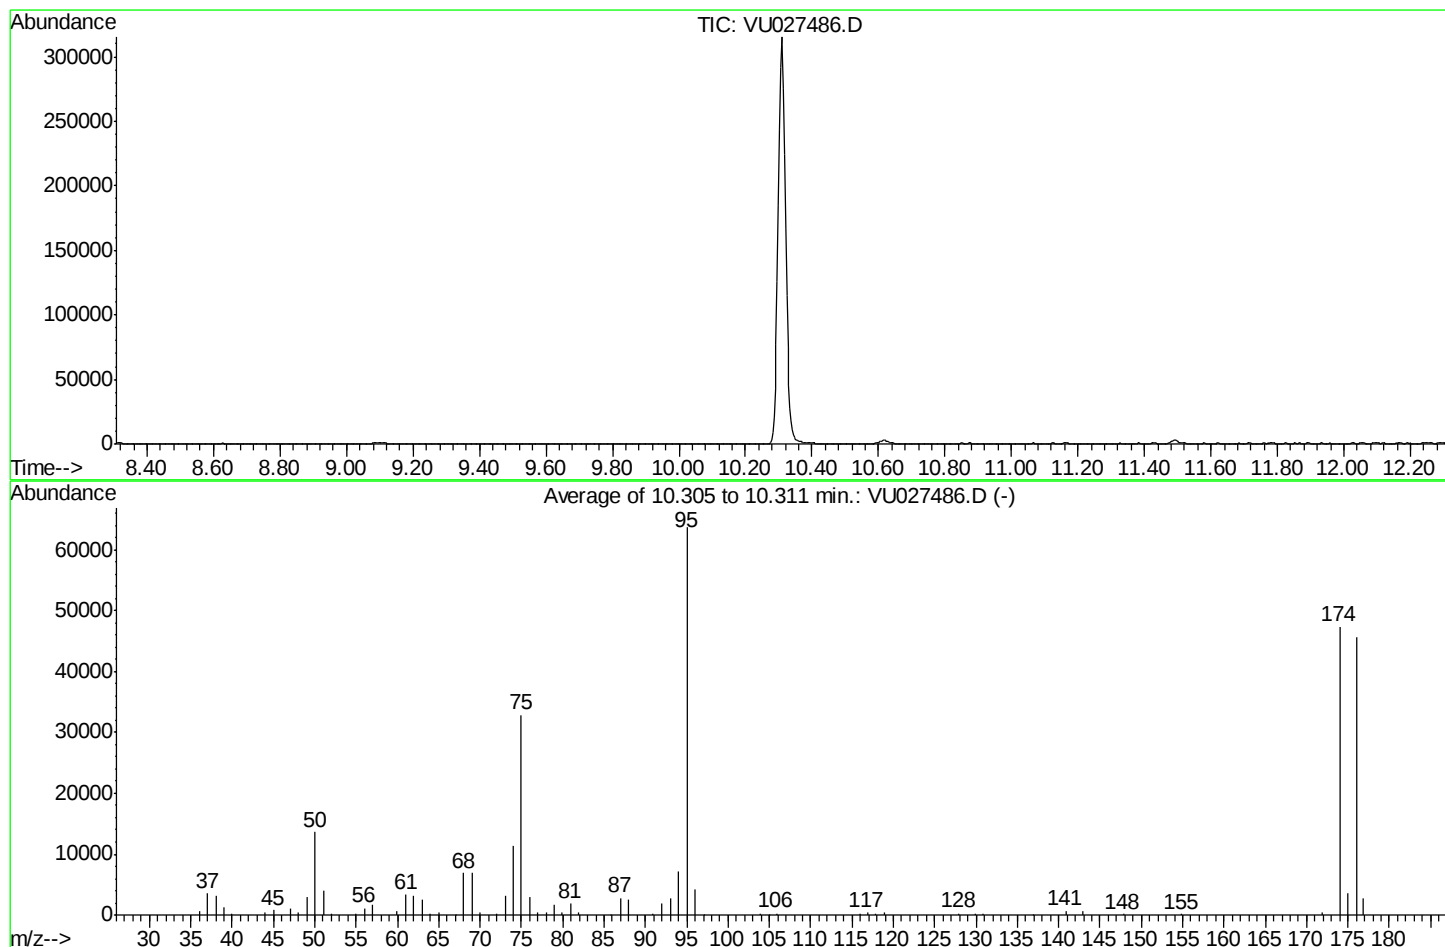

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	13585	PASS
75	95	30	80	51.6	32888	PASS
95	95	100	100	100.0	63725	PASS
96	95	5	9	6.5	4168	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.4	47410	PASS
175	174	5	9	7.6	3622	PASS
176	174	95	101	96.2	45600	PASS
177	176	5	9	6.1	2766	PASS

m/z	Abundance
44.00	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	540.0
37.00	3457.0
38.00	3102.0
39.00	1281.0
40.00	142.0
44.00	673.0
45.00	769.0
47.00	1095.0
48.00	512.0
49.00	2882.0
50.10	13299.0
51.10	3929.0
52.00	142.0
54.90	189.0
56.00	1061.0
57.00	1538.0
60.00	610.0
61.00	3144.0
62.00	3028.0
63.00	2468.0
64.00	333.0
65.00	380.0
67.00	163.0
68.00	6694.0
69.00	6724.0
70.00	463.0
72.00	301.0
73.00	3069.0
74.00	11186.0
75.00	31600.0
76.00	2845.0
77.00	462.0
78.00	325.0
78.90	1627.0
80.00	485.0
80.90	1728.0
81.90	431.0
87.00	2616.0
88.00	2543.0
90.90	209.0
92.00	1795.0
93.00	2656.0
94.00	7006.0
95.00	61432.0
96.00	4065.0
103.90	208.0
104.90	111.0
105.90	251.0
115.90	212.0
116.90	348.0
117.90	214.0
118.90	355.0
127.90	227.0
129.90	142.0
130.80	121.0
140.90	669.0
142.90	600.0
147.90	162.0
154.90	161.0
171.90	527.0
174.00	43976.0
175.00	3483.0
176.00	42600.0
176.90	2549.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	551.0
37.00	3630.0
38.10	3242.0
39.00	1365.0
40.00	149.0
44.00	736.0
45.00	808.0
47.00	1149.0
47.90	536.0
49.00	2950.0
50.10	14001.0
51.00	4191.0
52.00	193.0
55.00	187.0
56.00	1165.0
57.00	1830.0
60.00	672.0
61.00	3437.0
62.00	3189.0
63.00	2616.0
63.90	330.0
65.00	391.0
67.10	144.0
68.00	7126.0
69.00	7083.0
70.00	488.0
72.00	283.0
73.10	3299.0
74.00	11806.0
75.00	33880.0
76.00	3002.0
77.00	471.0
78.00	367.0
78.90	1766.0
80.00	518.0
80.90	1880.0
81.90	438.0
87.00	2871.0
88.00	2719.0
90.90	239.0
92.00	1976.0
93.00	2795.0
94.00	7409.0
95.00	65840.0
96.00	4311.0
97.00	114.0
103.90	221.0
104.90	102.0
105.90	263.0
115.90	252.0
116.90	396.0
117.90	246.0
118.90	370.0
127.90	250.0
129.90	161.0
130.80	117.0
140.80	731.0
142.90	628.0
147.80	175.0
154.90	152.0
171.90	556.0
174.00	48936.0
175.00	3718.0
176.00	47080.0
176.90	2840.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	529.0
37.00	3448.0
38.10	3031.0
39.00	1282.0
40.00	138.0
44.00	726.0
45.00	776.0
47.00	1096.0
47.90	486.0
49.00	2739.0
50.00	13456.0
51.00	4061.0
52.00	212.0
55.00	180.0
56.00	1068.0
57.00	1940.0
59.90	671.0
61.00	3335.0
62.00	3134.0
63.00	2480.0
63.90	304.0
65.00	367.0
68.00	6916.0
69.00	6827.0
70.00	452.0
72.00	295.0
73.00	3140.0
74.00	11209.0
75.00	33184.0
76.00	2879.0
77.00	418.0
78.00	399.0
78.90	1733.0
79.90	517.0
80.90	1855.0
81.90	402.0
85.80	106.0
87.00	2889.0
88.00	2621.0
90.90	228.0
92.00	1942.0
93.00	2715.0
94.00	7288.0
95.00	63904.0
96.00	4129.0
97.00	126.0
103.90	244.0
105.80	260.0
115.90	234.0
116.90	393.0
117.90	260.0
119.00	352.0
127.90	211.0
130.00	198.0
130.80	108.0
136.90	136.0
140.80	683.0
142.90	597.0
147.80	144.0
154.90	145.0
171.90	514.0
174.00	49320.0
175.00	3667.0
176.00	47120.0
176.90	2911.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40