

Data File : VU034985.D

Acq On : 08 Oct 2019 11:51

Operator : JC/SP

Sample : MDL03

Misc : 25.0mL/MSVOA_U/WATER

ALS Vial : 9 Sample Multiplier: 1




Quant Time: Oct 09 07:20:06 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Wed Oct 09 07:15:09 2019

Response via : Initial Calibration

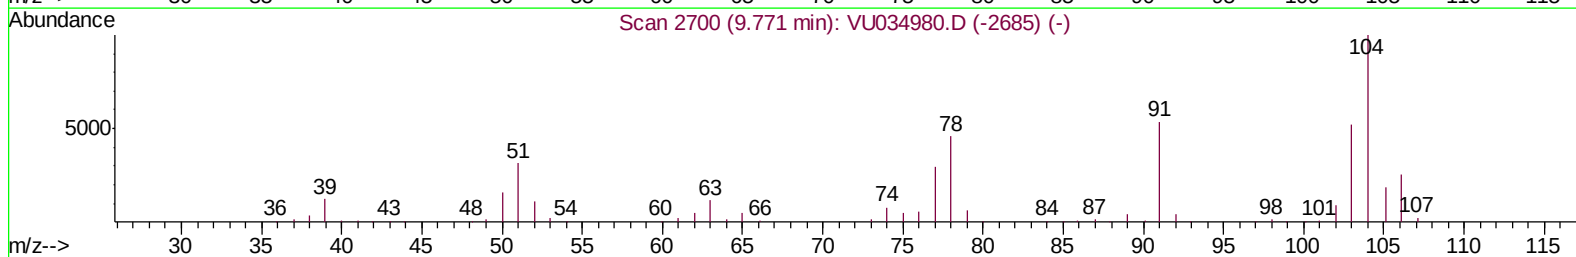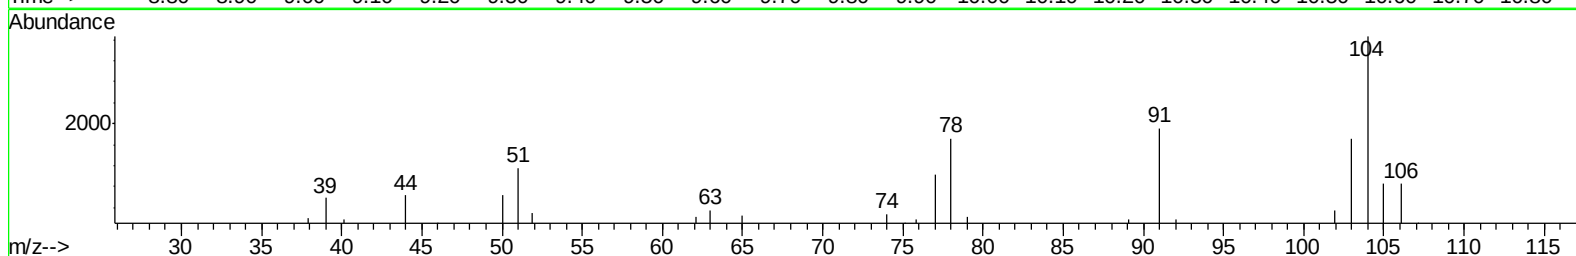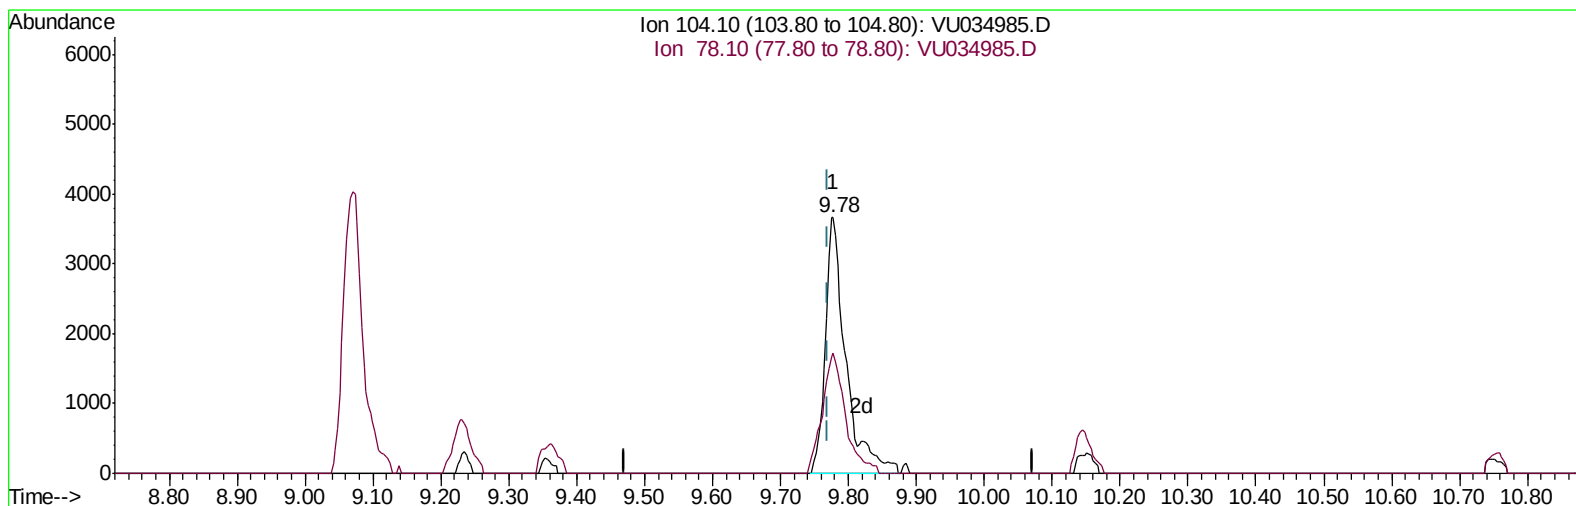

TIC: VU034985.D

(55) Styrene (T)

9.778min (+0.006) 0.21ug/L m

response 7652

Ion	Exp%	Act%
104.10	100	100
78.10	46.80	46.93
0.00	0.00	0.00
0.00	0.00	0.00