


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100819\
 Data File : VU034979.D
 Acq On : 08 Oct 2019 08:26
 Operator : JC/SP
 Sample : BFB15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB15

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Oct 09 07:15:09 2019

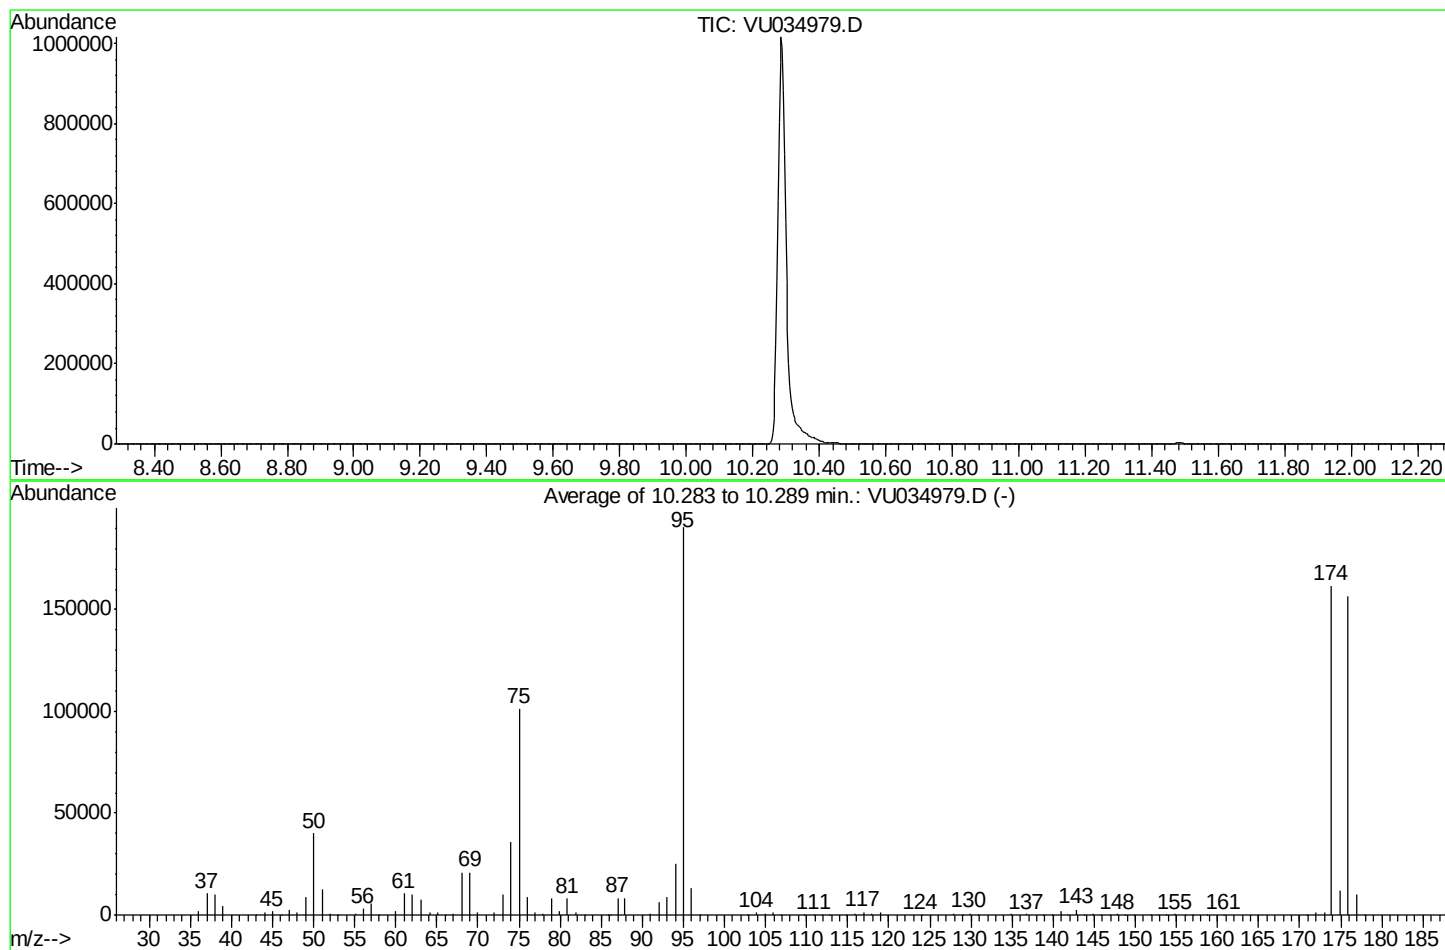

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	39997	PASS
75	95	30	80	53.3	101408	PASS
95	95	100	100	100.0	190400	PASS
96	95	5	9	6.8	13003	PASS
173	174	0.00	2	0.8	1360	PASS
174	95	50	120	84.9	161621	PASS
175	174	5	9	7.4	11995	PASS
176	174	95	101	97.0	156693	PASS
177	176	5	9	6.6	10357	PASS

m/z	Abundance
36.00	1908.0
37.00	10382.0
38.00	9961.0
39.00	4213.0
39.90	260.0
44.00	1804.0
45.00	1719.0
46.10	170.0
47.00	2436.0
48.00	1399.0
49.00	8719.0
50.00	39480.0
51.00	12227.0
52.00	522.0
52.90	180.0
55.10	641.0
56.00	2934.0
57.00	5002.0
58.00	287.0
60.00	2213.0
61.00	10406.0
62.00	10005.0
63.00	7698.0
64.10	1166.0
65.10	1029.0
66.00	141.0
67.00	517.0
68.00	19824.0
69.00	20568.0
70.00	1534.0
72.00	1130.0
73.00	10024.0
74.00	34640.0
75.00	100112.0
76.00	8874.0
76.90	1348.0
77.80	796.0
78.90	7565.0
79.90	1917.0
80.90	7661.0
81.90	1541.0
82.90	210.0
85.80	223.0
87.00	7938.0
87.90	7817.0
91.00	882.0
92.00	5992.0
93.00	8586.0
94.00	23696.0
95.00	184064.0
96.00	13059.0
97.10	337.0
103.90	1054.0
104.90	418.0
105.90	994.0
106.80	147.0
109.70	103.0
110.90	200.0
111.90	164.0
112.80	179.0
114.90	142.0
115.80	642.0
116.90	1284.0
117.90	736.0
118.90	999.0
123.90	106.0
127.80	676.0
128.90	255.0
129.90	789.0
130.90	270.0
134.90	479.0
136.80	491.0
138.70	186.0
139.90	126.0
140.90	2032.0
141.80	141.0
142.90	2649.0
143.80	199.0
144.90	458.0
145.80	348.0
146.90	108.0
147.90	440.0
149.80	155.0
151.90	128.0
152.80	205.0
154.90	379.0
155.90	120.0
156.90	286.0
158.80	195.0
160.80	141.0
170.90	226.0
171.90	1412.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

173.00	1975.0
173.90	152768.0
175.00	11297.0
175.90	146560.0
176.90	10107.0
177.90	218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	1978.0
37.00	10747.0
38.00	10461.0
39.00	4291.0
40.00	240.0
43.00	103.0
44.00	1944.0
45.00	1843.0
46.10	219.0
47.00	2695.0
48.00	1446.0
49.00	9017.0
50.00	41152.0
51.00	12843.0
52.00	476.0
53.00	197.0
55.10	630.0
56.00	3174.0
57.00	5599.0
58.00	274.0
60.00	2332.0
61.00	10983.0
62.00	10424.0
63.00	8109.0
64.10	1202.0
65.10	1063.0
66.00	131.0
67.00	642.0
68.00	21456.0
69.00	21600.0
70.00	1592.0
72.00	1144.0
73.00	10321.0
74.00	36648.0
75.00	104920.0
76.00	9087.0
77.00	1389.0
77.80	859.0
78.90	8234.0
79.90	2058.0
80.90	8106.0
81.90	1587.0
82.90	203.0
85.80	274.0
87.00	8645.0
87.90	8208.0
91.00	954.0
92.00	6300.0
93.00	9004.0
94.00	25824.0
95.00	196352.0
96.00	13381.0
97.10	320.0
103.90	1037.0
104.90	422.0
105.90	1001.0
106.80	152.0
110.90	284.0
111.90	212.0
112.70	194.0
114.80	204.0
115.80	789.0
116.90	1419.0
117.90	716.0
119.00	1167.0
127.80	707.0
128.90	307.0
129.90	838.0
130.90	263.0
134.90	468.0
136.80	556.0
138.80	190.0
139.90	136.0
140.90	2152.0
141.80	184.0
142.90	2657.0
143.80	225.0
144.90	533.0
145.80	299.0
147.80	465.0
149.80	137.0
151.90	128.0
152.90	229.0
153.80	125.0
154.90	362.0
156.00	105.0
156.90	257.0
158.70	224.0
160.80	189.0
170.90	226.0
172.00	1472.0
173.90	166912.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

175.00	12311.0
175.90	161792.0
176.90	10772.0
177.90	281.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

m/z	Abundance
36.00	1836.0
37.00	10126.0
38.00	9672.0
39.00	3853.0
40.00	228.0
42.90	135.0
44.00	1865.0
45.00	1833.0
46.00	247.0
47.00	2589.0
48.00	1329.0
49.00	8478.0
50.00	39360.0
51.00	12386.0
52.00	436.0
53.00	191.0
55.00	599.0
56.00	3124.0
57.00	5770.0
58.00	236.0
60.00	2106.0
61.00	10564.0
62.00	9933.0
63.00	7663.0
64.10	1056.0
65.10	1003.0
66.00	156.0
67.00	685.0
68.00	21120.0
69.00	20896.0
70.00	1433.0
72.00	1046.0
73.00	9675.0
74.00	35800.0
75.00	99192.0
76.00	8627.0
77.00	1260.0
77.90	847.0
78.90	8104.0
79.90	1993.0
80.90	7873.0
81.90	1591.0
83.00	197.0
86.10	270.0
87.00	8615.0
87.90	7939.0
90.90	919.0
92.00	5946.0
93.00	8675.0
94.00	25280.0
95.00	190784.0
96.00	12571.0
97.00	269.0
102.80	101.0
103.90	952.0
104.90	334.0
105.90	923.0
106.80	165.0
110.90	300.0
111.90	211.0
112.80	202.0
114.90	280.0
115.80	932.0
116.90	1423.0
117.90	673.0
119.00	1211.0
127.80	624.0
128.90	309.0
129.90	733.0
130.90	247.0
134.90	375.0
136.80	448.0
138.80	136.0
139.90	147.0
140.90	2089.0
141.80	189.0
142.90	2439.0
143.80	220.0
144.90	531.0
145.80	254.0
147.80	429.0
148.80	113.0
149.80	123.0
151.90	121.0
152.90	272.0
153.80	158.0
154.80	355.0
156.10	110.0
157.00	243.0
158.80	228.0
160.70	196.0
170.90	232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

171.90	1537.0
173.00	2106.0
173.90	165184.0
174.90	12379.0
175.90	161728.0
176.90	10192.0
177.80	347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15

Scan 2846 (10.241 min): VU034979.D
BFB15

m/z	Abundance
39.90	246.0
44.00	547.0

Instrument :
MSVOA_U
ClientSampleId :
BFB15