
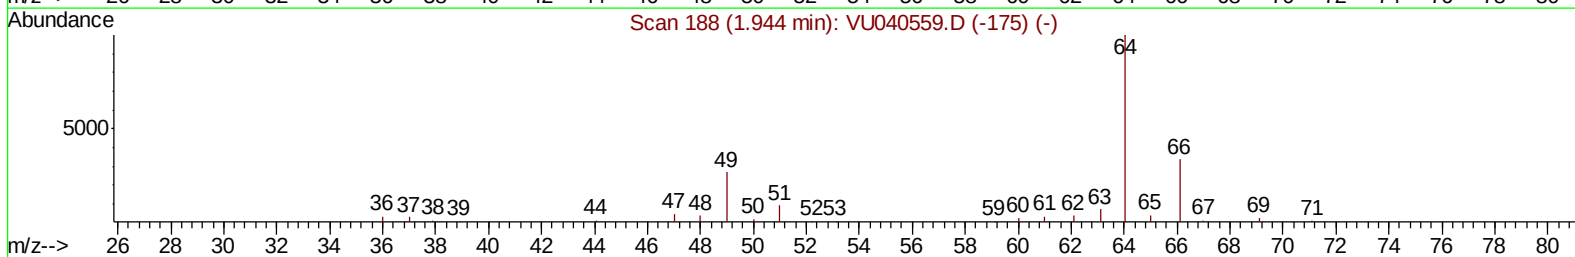
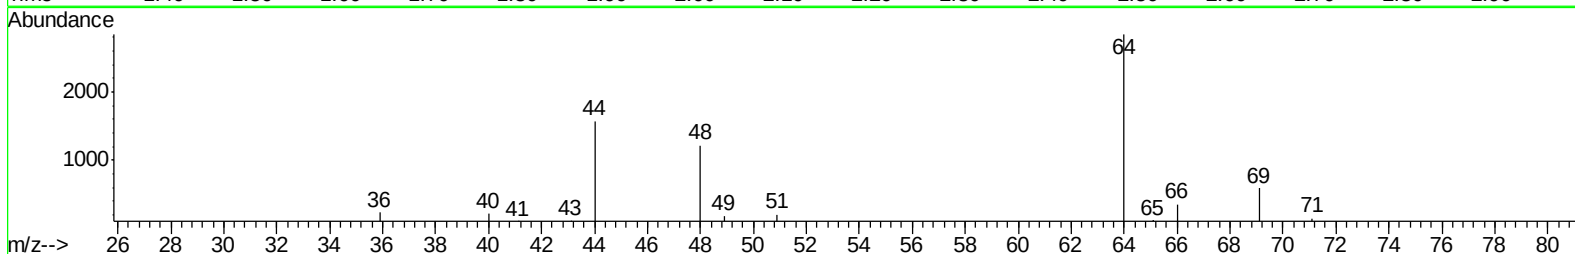


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100820\
Data File : VU040566.D
Acq On : 08 Oct 2020 17:10
Operator : SY/MD
Sample : L4240-08DL 20X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 09 02:56:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 09 01:55:27 2020
Response via : Initial Calibration

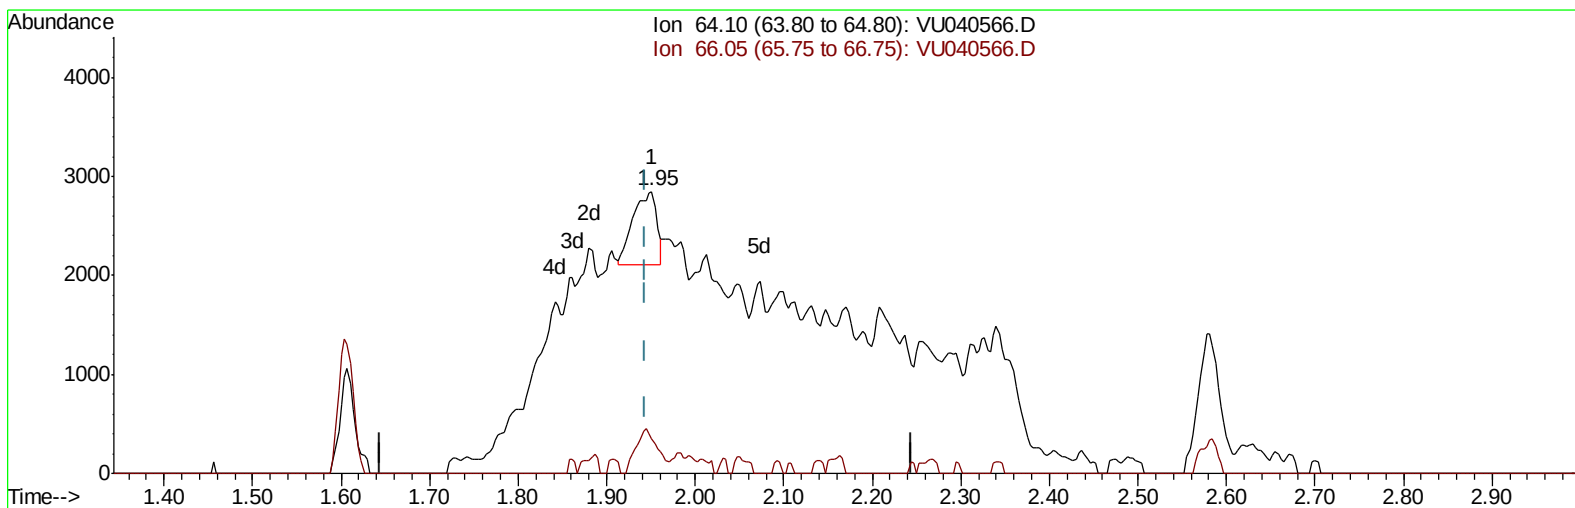

TIC: VU040566.D

(8) Chloroethane (T)

1.951min (+0.006) 0.16ug/L m

response 1350

Ion	Exp%	Act%
64.10	100	100
66.05	33.30	12.33#
0.00	0.00	0.00
0.00	0.00	0.00