
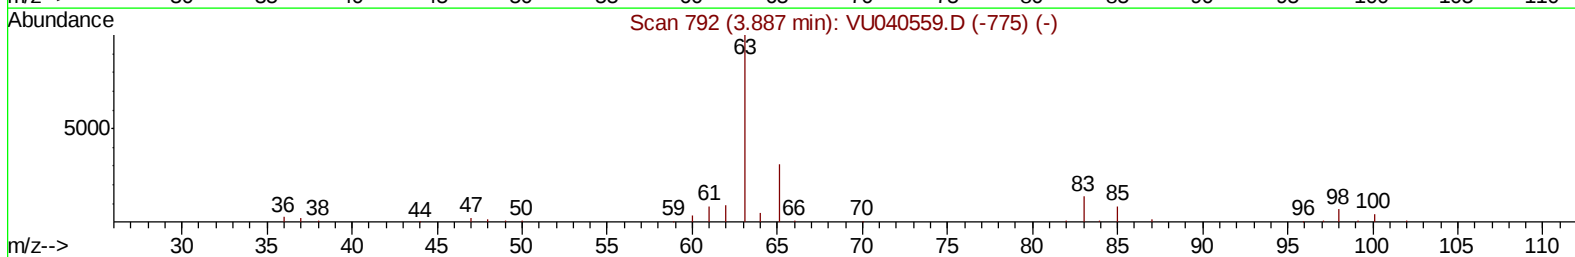
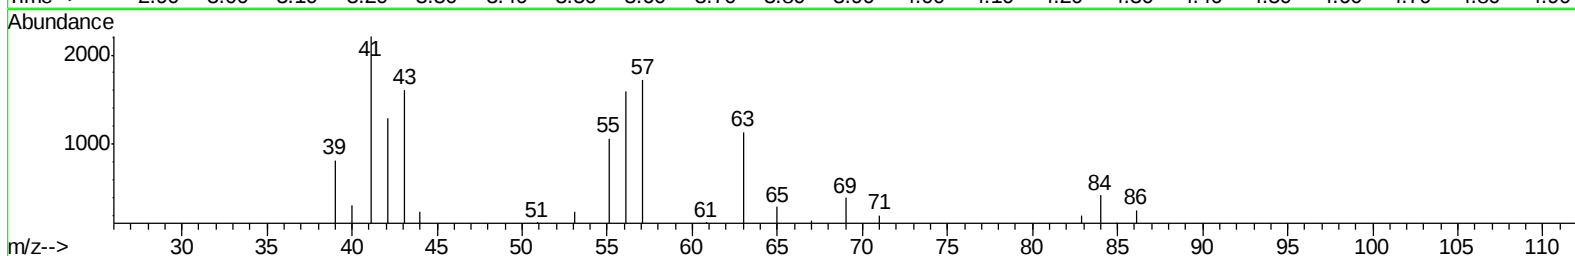


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU100820\
 Data File : VU040566.D
 Acq On : 08 Oct 2020 17:10
 Operator : SY/MD
 Sample : L4240-08DL 20X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 09 02:56:28 2020
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 09 01:55:27 2020
 Response via : Initial Calibration

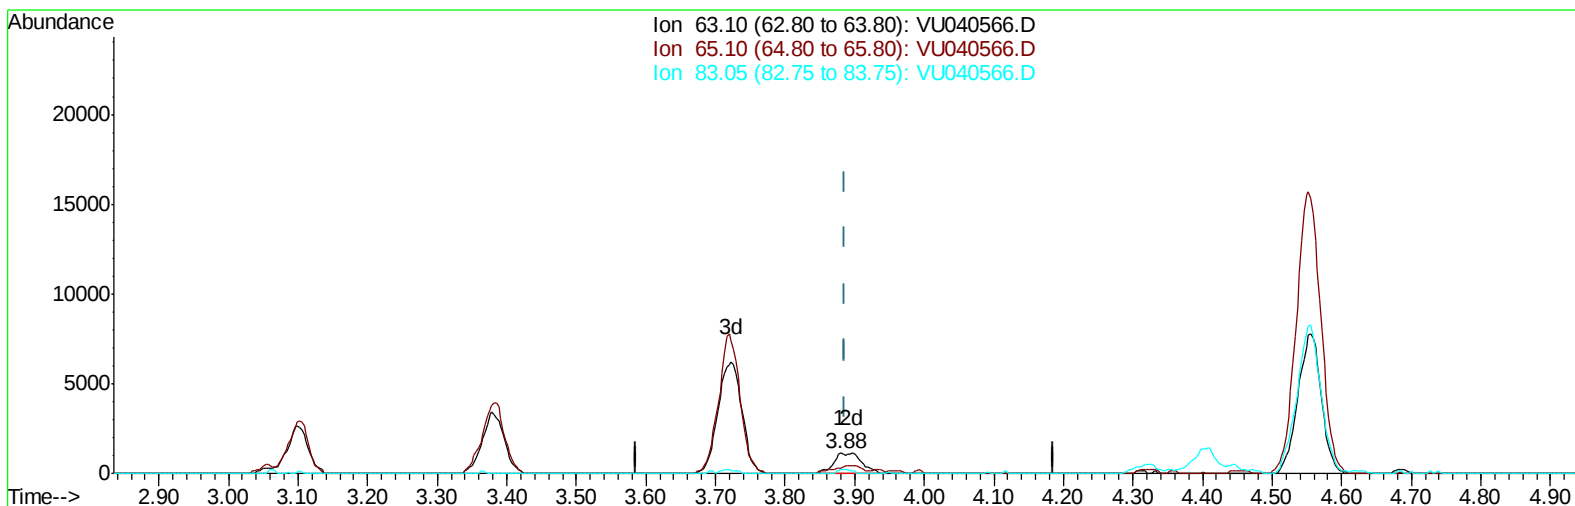

TIC: VU040566.D

(19) 1,1-Dichloroethane (T)

3.880min (-0.006) 0.14ug/L m

response 3104

Ion	Exp%	Act%
63.10	100	100
65.10	31.30	25.93
83.05	13.70	17.37
0.00	0.00	0.00