

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U100820\
 Data File : VU040566.D
 Acq On : 08 Oct 2020 17:10
 Operator : SY/MD
 Sample : L4240-08DL 20X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3S5DL

Quant Time: Oct 09 02:04:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 09 01:55:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	144806	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	140882	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	72377	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	57389	4.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.60%
7) Chloroethane-d5	1.92	69	45919	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	2.58	63	85316	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	4.66	46	205269	53.46	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.92%
24) Chloroform-d	5.08	84	100873	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.72	65	63478	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.00%
32) Benzene-d6	5.74	84	193863	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.70	67	63996	5.07	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.40%
41) Toluene-d8	7.91	98	161765	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
43) trans-1,3-Dichloropropene-	8.19	79	26187	4.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.00%
46) 2-Hexanone-d5	8.64	63	142204	51.64	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.28%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	55099	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	70673	5.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.40%

Target Compounds

					Ovalue
5) Vinyl chloride	1.61	62	727	0.056 ug/L #	1
8) Chloroethane	1.95	64	987	0.120 ug/L #	63
10) 1,1,2-Trichloro-1,2,2-trif	2.58	101	639	0.053 ug/L #	20
12) 1,1-Dichloroethene	2.59	96	579	0.056 ug/L #	1
14) Carbon disulfide	2.81	76	1599	0.055 ug/L #	76
15) Methyl Acetate	3.10	43	1842421	271.093 ug/L #	56
16) Methylene chloride	3.06	84	11979	0.903 ug/L #	35
19) 1,1-Dichloroethane	3.88	63	1387	0.062 ug/L	90
21) 2-Butanone	4.55	43	208672	44.970 ug/L #	53
29) 1,1,1-Trichloroethane	5.34	97	4591	0.243 ug/L	97
30) Cyclohexane	5.41	56	90747	5.202 ug/L	99
35) Methylcyclohexane	6.77	83	1807	0.109 ug/L #	88
37) 1,2-Dichloropropane	6.70	63	7153	0.567 ug/L #	87
39) cis-1,3-Dichloropropene	7.57	75	1819	0.106 ug/L #	66
42) Toluene	7.98	91	18738	0.406 ug/L	97
44) trans-1,3-Dichloropropene	8.19	75	1319	0.083 ug/L	89
48) 2-Hexanone	8.69	43	3910	0.522 ug/L #	88

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100820\
 Data File : VU040566.D
 Acq On : 08 Oct 2020 17:10
 Operator : SY/MD
 Sample : L4240-08DL 20X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BG3S5DL

Quant Time: Oct 09 02:04:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Oct 09 01:55:27 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
52) Ethylbenzene	9.57	91	3928	0.079	ug/L	91
53) m,p-Xylene	9.69	106	3966	0.218	ug/L	91
56) Isopropylbenzene	10.48	105	8460	0.180	ug/L	98
59) 1,2,3-Trichloropropane	10.91	75	710	0.077	ug/L #	1
63) 1,4-Dichlorobenzene	11.83	146	1843	0.075	ug/L	93
67) 1,3,5-Trichlorobenzene	13.83	180	24628	1.465	ug/L	98
68) 1,2,4-trichlorobenzene	13.83	180	24628	1.896	ug/L	97
69) Naphthalene	14.08	128	2688	0.127	ug/L #	95
70) 1,2,3-Trichlorobenzene	14.32	180	5282	0.438	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100820\
Data File : VU040566.D
Acq On : 08 Oct 2020 17:10
Operator : SY/MD
Sample : L4240-08DL 20X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BG3S5DL

Quant Time: Oct 09 02:04:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Oct 09 01:55:27 2020
Response via : Initial Calibration

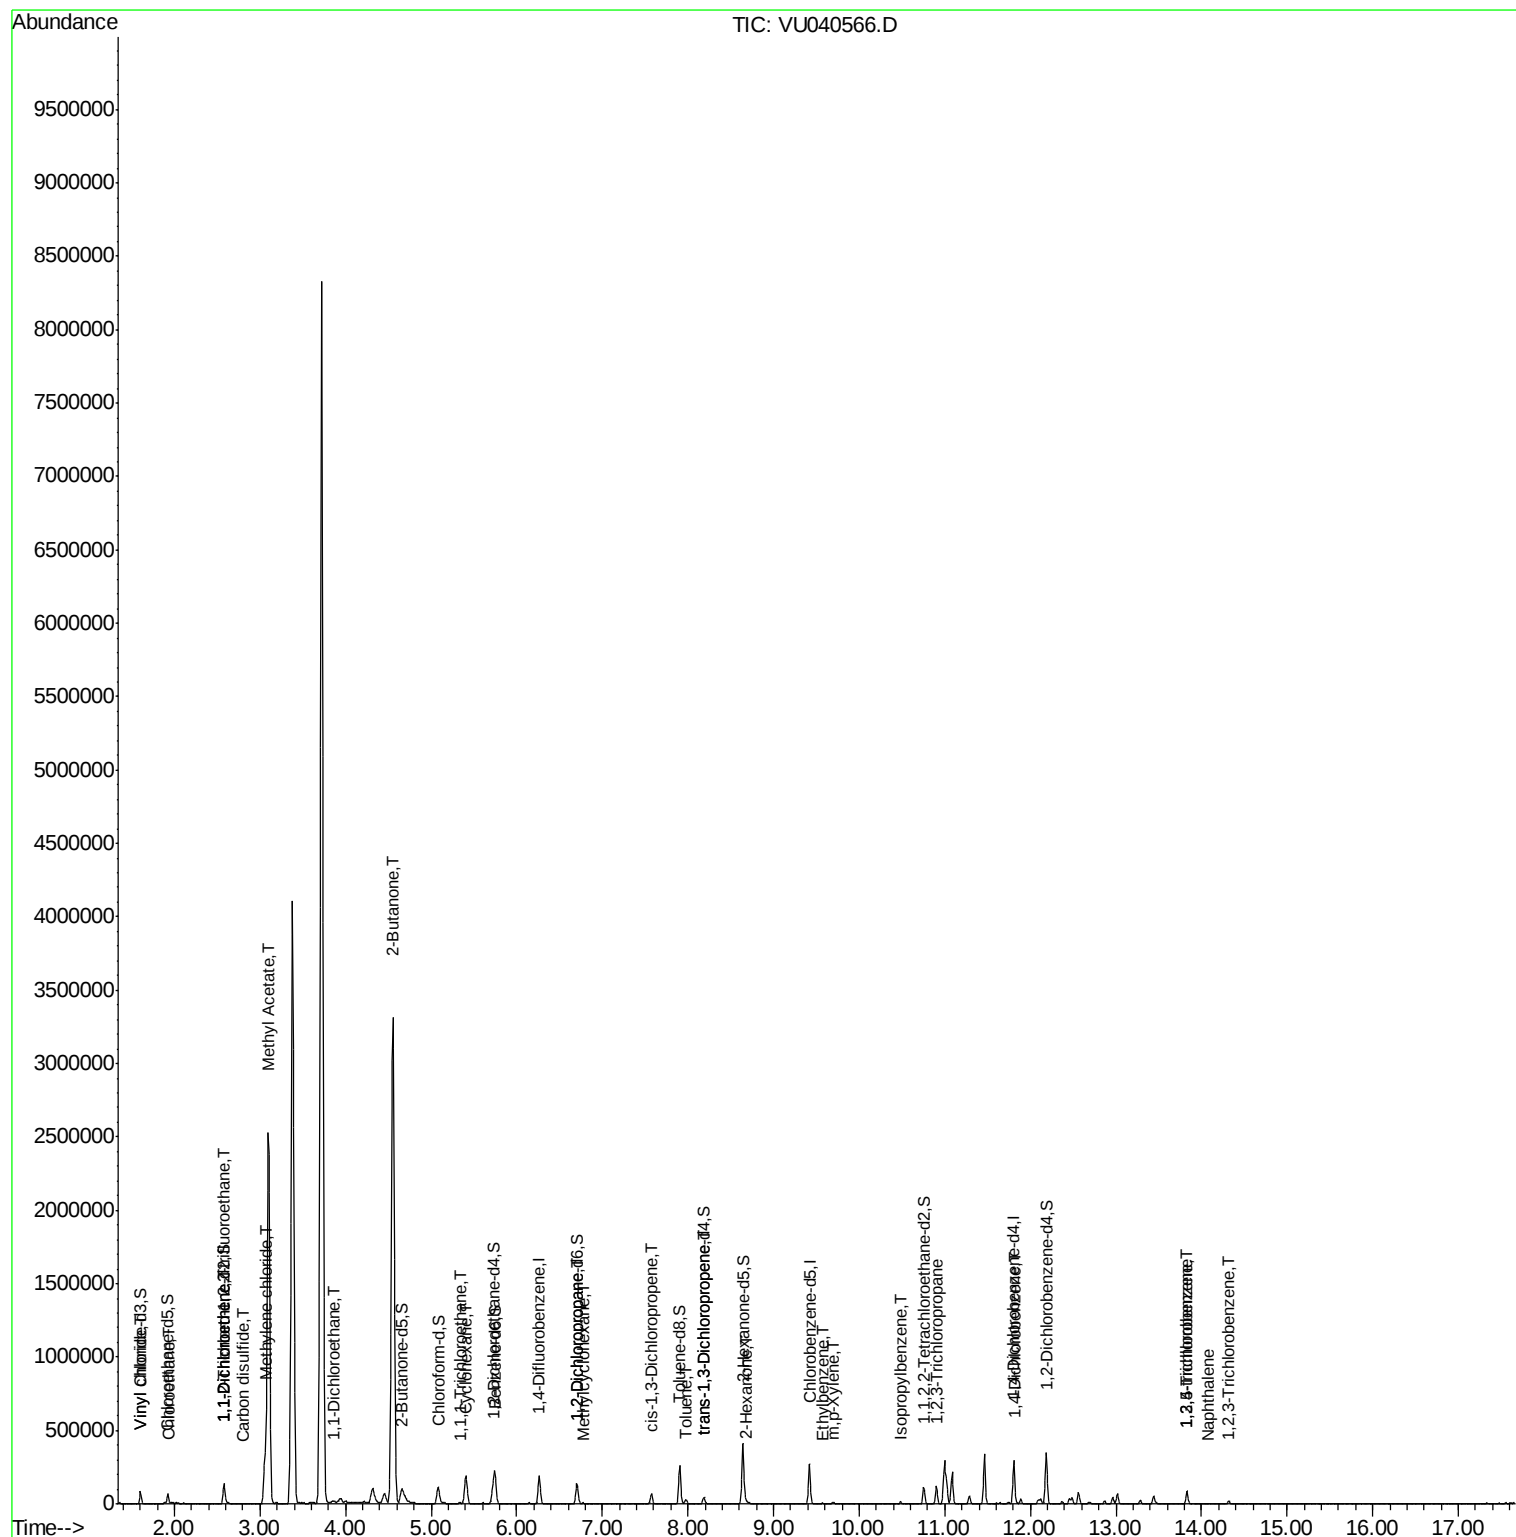



#5

Vinyl chloride

Concen: 0.056 ug/L

RT: 1.61 min Scan# 84

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleID :


BG3S5DL

Tot Ion: 62 Resp: 727

Ion Ratio Lower Upper




62 100

64 136.0 23.7 44.1#

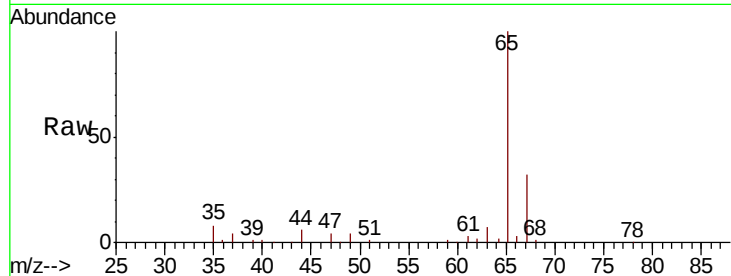

Abundance Ion 62.00 (61.70 to 62.70): VU0

Ion 64.10 (63.80 to 64.80): VU0

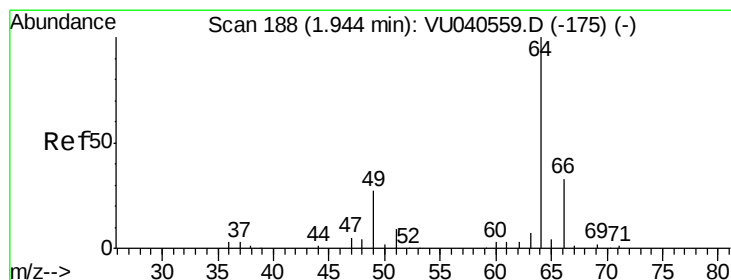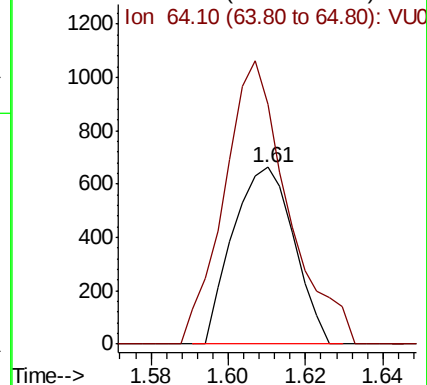

#8

Chloroethane

Concen: 0.120 ug/L

RT: 1.95 min Scan# 190

Delta R.T. 0.01 min

Lab File: VU040566.D


Acq: 08 Oct 2020 17:10

Tgt Ion: 64 Resp: 987

Ion Ratio Lower Upper



64 100


66 12.3 23.3 43.3#



Abundance Ion 64.10 (63.80 to 64.80): VU0

Ion 66.05 (65.75 to 66.75): VU0

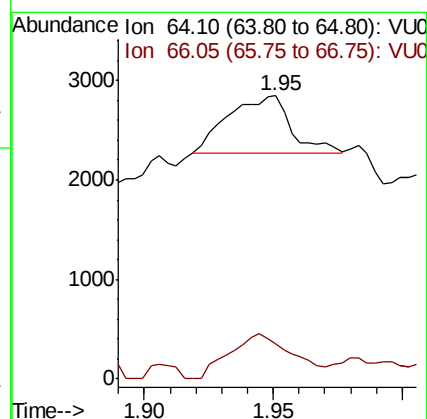

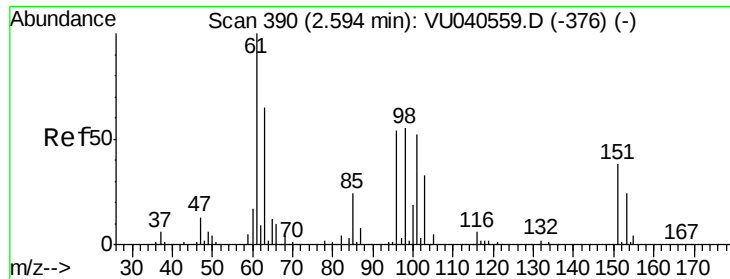

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.053 ug/L

RT: 2.58 min Scan# 385

Delta R.T. -0.02 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleId :

BG3S5DL


Tot Ion:101 Resp: 639

Ion Ratio Lower Upper

101 100

85 0.0 36.7 55.1#

151 0.0 58.0 87.0#

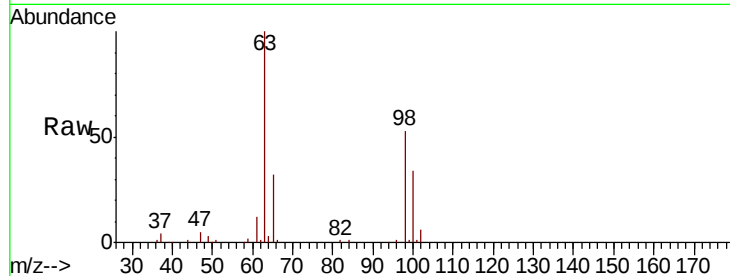

Abundance Ion 101.00 (100.70 to 101.70): V

Ion 85.00 (84.70 to 85.70): VU0

Ion 151.00 (150.70 to 151.70): V

600

500

400

300



200

100

0

2.54 2.56 2.58 2.60

Time-->

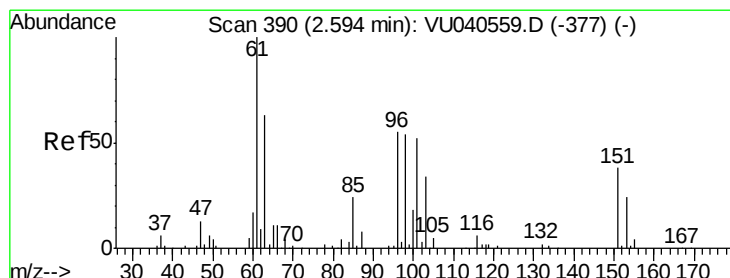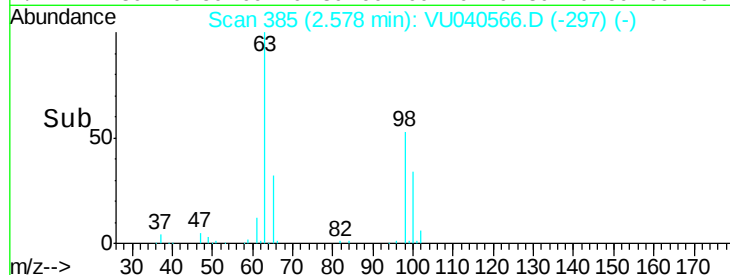

#12

1,1-Dichloroethene

Concen: 0.056 ug/L

RT: 2.59 min Scan# 388

Delta R.T. -0.01 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10


Tgt Ion: 96 Resp: 579

Ion Ratio Lower Upper

96 100

61 1431.1 128.8 239.2#

63 13059.0 84.6 157.2#

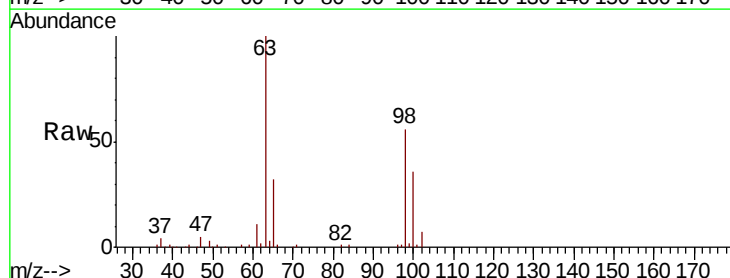

Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

Ion 63.00 (62.70 to 63.70): VU0

60000


40000


20000

0

2.54 2.56 2.58 2.60 2.62

Time-->

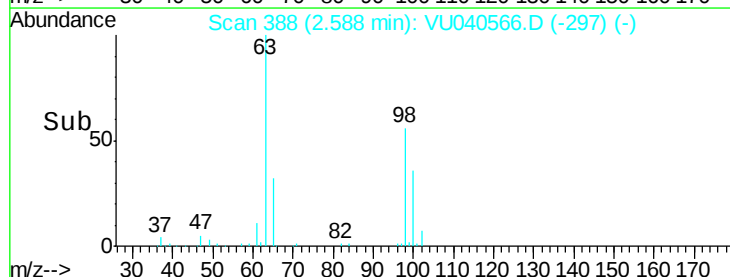



#14

Carbon disulfide

Concen: 0.055 ug/L

RT: 2.81 min Scan# 456

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleId :





BG3S5DL

Tot Ion: 76 Resp: 1599

Ion Ratio Lower Upper

76 100

78 0.0 6.8 10.2#

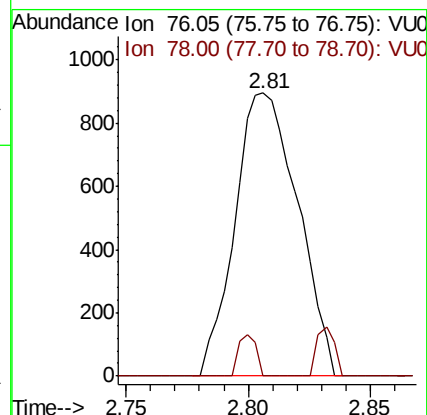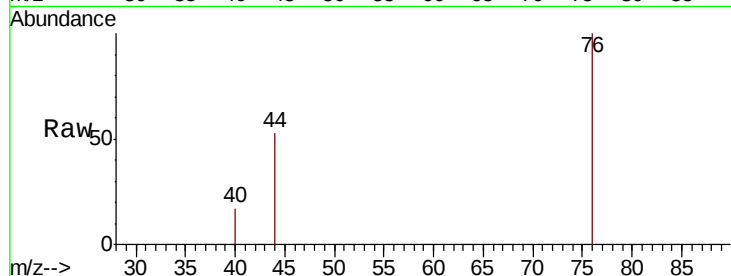

#15

Methyl Acetate

Concen: 271.093 ug/L

RT: 3.10 min Scan# 548

Delta R.T. 0.13 min

Lab File: VU040566.D




Acq: 08 Oct 2020 17:10


Tgt Ion: 43 Resp: 1842421

Ion Ratio Lower Upper

43 100

74 0.0 16.5 24.7#

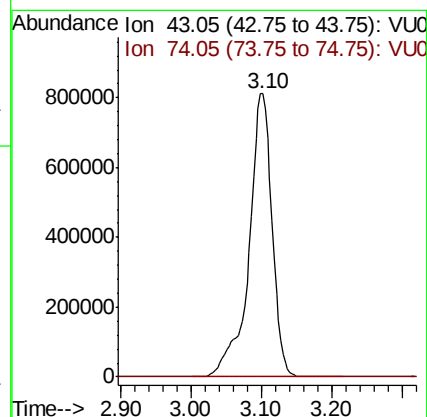



#16

Methylene chloride

Concen: 0.903 ug/L

RT: 3.06 min Scan# 535

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleId :

BG3S5DL





Tot Ion: 84 Resp: 11979

Ion Ratio Lower Upper

84 100

86 169.5 45.4 84.4#

49 99.9 99.8 185.3

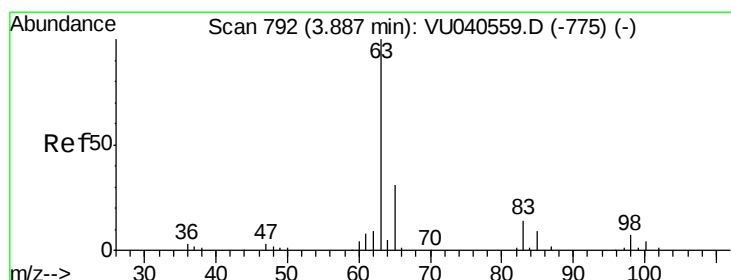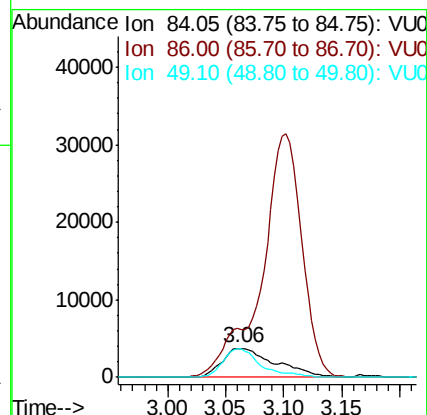

#19

1,1-Dichloroethane

Concen: 0.062 ug/L

RT: 3.88 min Scan# 790

Delta R.T. -0.01 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10




Tgt Ion: 63 Resp: 1387


Ion Ratio Lower Upper

63 100

65 25.9 21.9 40.7

83 17.4 9.6 17.8

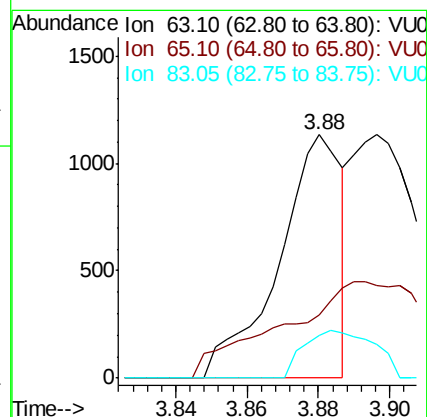



#21

2-Butanone

Concen: 44.970 ug/L

RT: 4.55 min Scan# 999

Delta R.T. -0.19 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleId :





BG3S5DL

Tot Ion: 43 Resp: 208672

Ion Ratio Lower Upper

43 100

72 0.0 11.4 34.2#

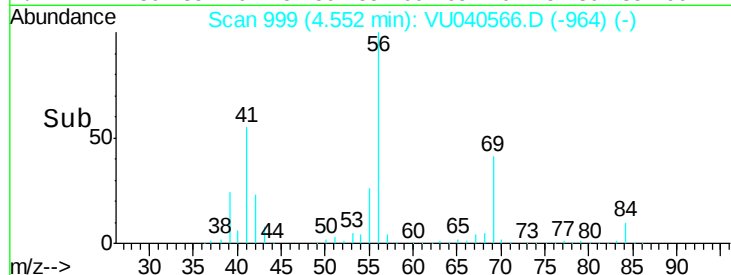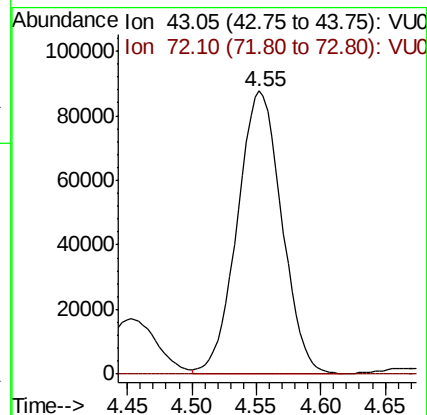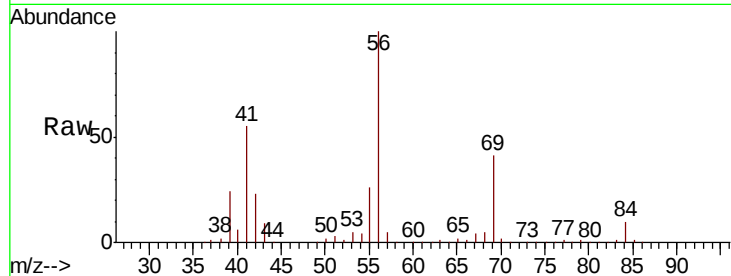

#29

1,1,1-Trichloroethane

Concen: 0.243 ug/L

RT: 5.34 min Scan# 1243

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10




Tgt Ion: 97 Resp: 4591


Ion Ratio Lower Upper

97 100

99 60.7 51.3 76.9

61 50.9 39.4 59.2



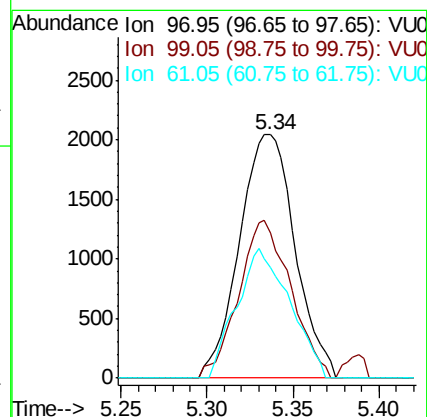





#30
Cyclohexane
Concen: 5.202 ug/L
RT: 5.41 min Scan# 1265
Delta R.T. 0.00 min
Lab File: VU040566.D
Acq: 08 Oct 2020 17:10




Instrument :
MSVOA_U
ClientSampleId :
BG3S5DL


Tot Ion: 56 Resp: 90747
Ion Ratio Lower Upper
56 100
69 29.4 23.8 35.8
84 81.1 64.0 96.0

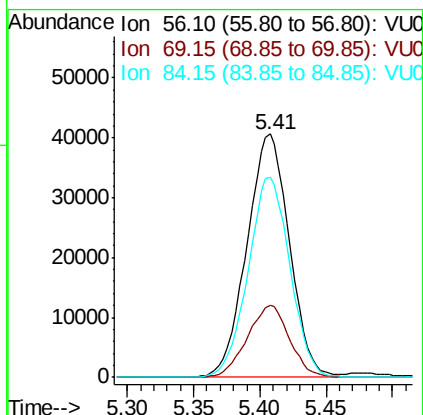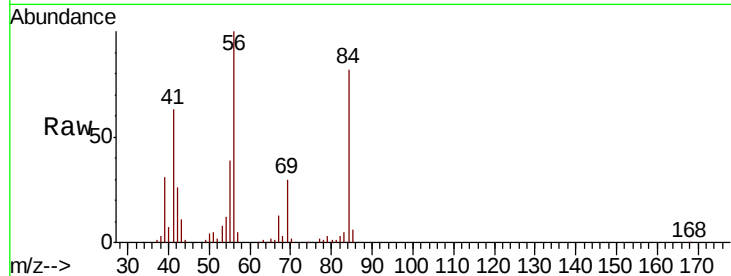

#35
Methylcyclohexane
Concen: 0.109 ug/L
RT: 6.77 min Scan# 1690
Delta R.T. 0.00 min
Lab File: VU040566.D
Acq: 08 Oct 2020 17:10

Tgt Ion: 83 Resp: 1807
Ion Ratio Lower Upper
83 100
55 97.3 70.7 106.1
98 36.9 38.4 57.6#



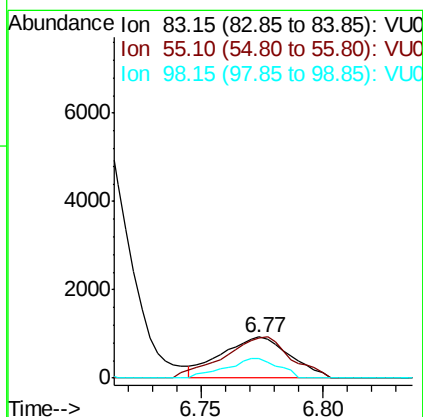



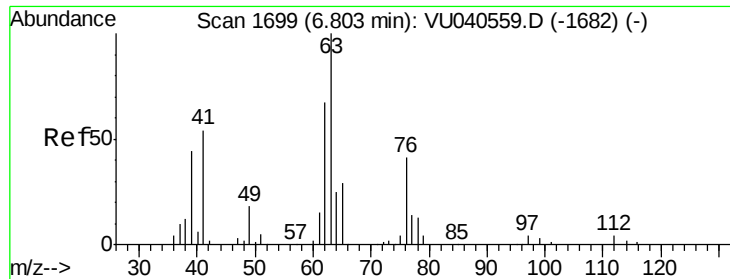

#37
 1,2-Dichloropropane
 Concen: 0.567 ug/L
 RT: 6.70 min Scan# 1668
 Delta R.T. -0.10 min
 Lab File: VU040566.D
 Acq: 08 Oct 2020 17:10




Instrument :
 MSVOA_U
 ClientSampleId :
 BG3S5DL


Tot Ion: 63 Resp: 7153
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.5 5.3#

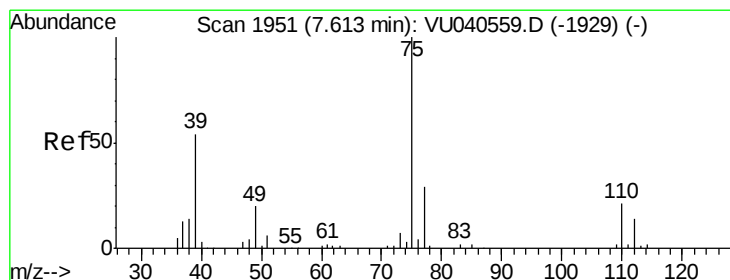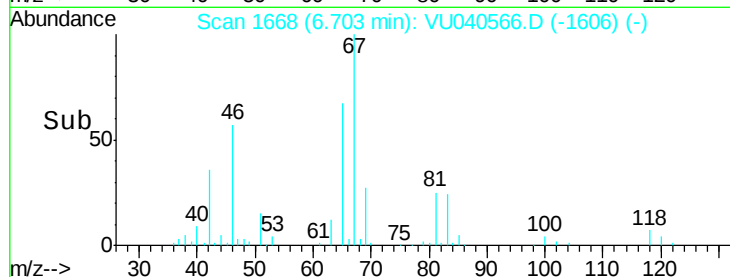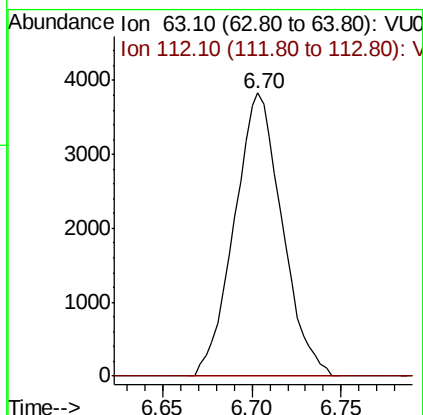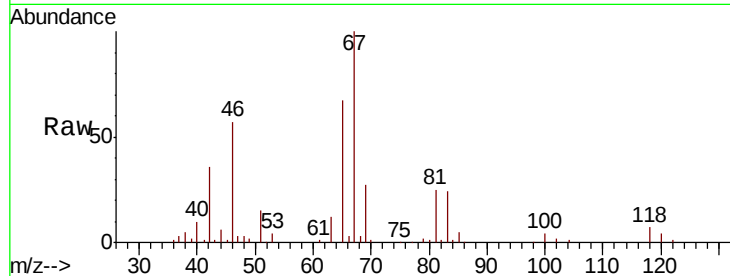

#39
 cis-1,3-Dichloropropene
 Concen: 0.106 ug/L
 RT: 7.57 min Scan# 1938
 Delta R.T. -0.04 min
 Lab File: VU040566.D
 Acq: 08 Oct 2020 17:10

Tgt Ion: 75 Resp: 1819
 Ion Ratio Lower Upper
 75 100
 77 47.8 20.5 38.1#

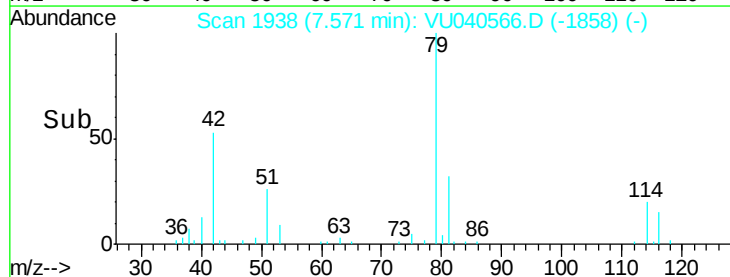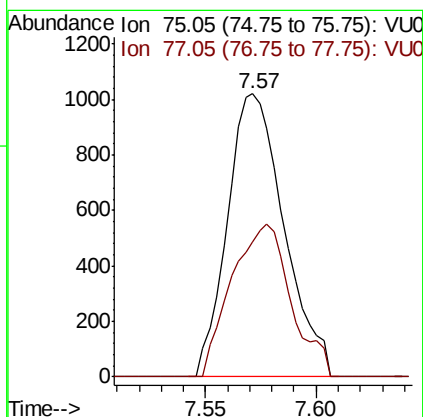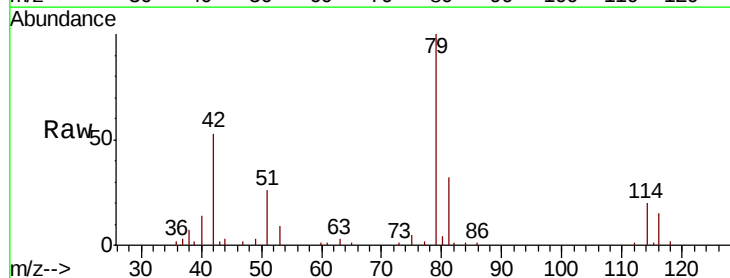



#42

Toluene

Concen: 0.406 ug/L

RT: 7.98 min Scan# 2064

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleId :


BG3S5DL

Tot Ion: 91 Resp: 18738

Ion Ratio Lower Upper




91 100

92 59.8 40.2 74.6

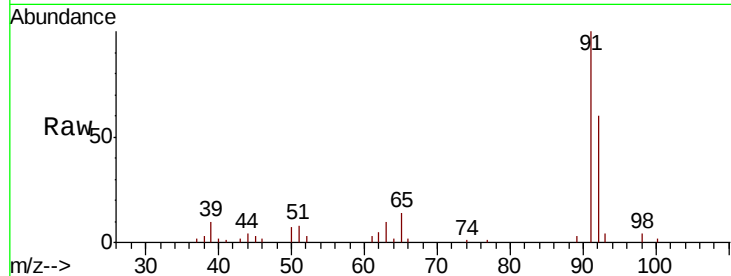

Abundance Ion 91.15 (90.85 to 91.85): VU040559.D (-2049) (-)

Ion 92.15 (91.85 to 92.85): VU040559.D (-2049) (-)

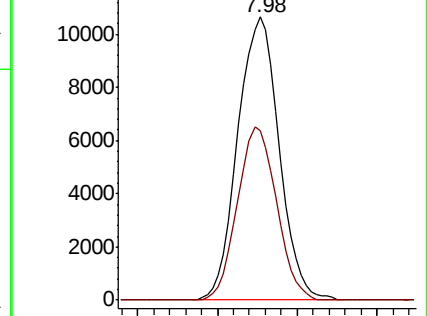

#44

trans-1,3-Dichloropropene

Concen: 0.083 ug/L

RT: 8.19 min Scan# 2130

Delta R.T. -0.03 min

Lab File: VU040566.D


Acq: 08 Oct 2020 17:10

Tgt Ion: 75 Resp: 1319

Ion Ratio Lower Upper



75 100


77 35.0 20.4 38.0



Abundance Ion 75.05 (74.75 to 75.75): VU040559.D (-2120) (-)

Ion 77.05 (76.75 to 77.75): VU040559.D (-2120) (-)




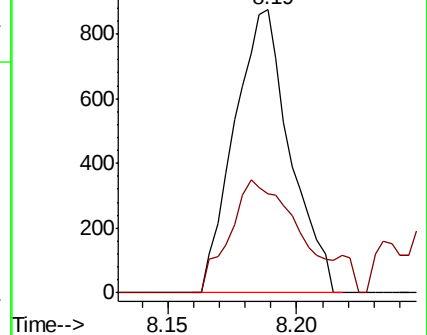




#48
2-Hexanone
Concen: 0.522 ug/L
RT: 8.69 min Scan# 2286
Delta R.T. 0.00 min
Lab File: VU040566.D
Acq: 08 Oct 2020 17:10




Instrument :
MSVOA_U
ClientSampleId :
BG3S5DL


Tot Ion: 43 Resp: 3910
Ion Ratio Lower Upper
43 100
58 53.2 41.0 61.6
57 0.0 14.4 21.6#
100 8.0 8.6 13.0#

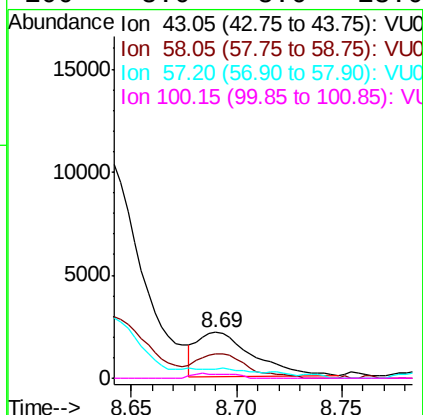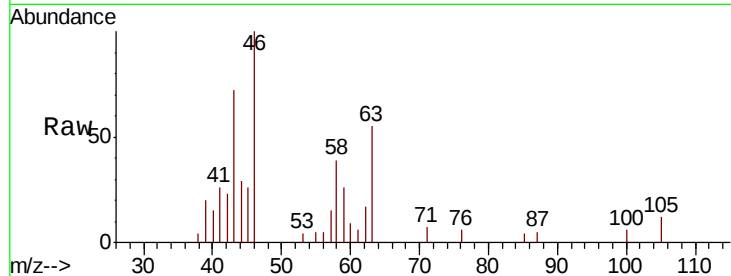

#52
Ethylbenzene
Concen: 0.079 ug/L
RT: 9.57 min Scan# 2559
Delta R.T. -0.00 min
Lab File: VU040566.D
Acq: 08 Oct 2020 17:10

Tgt Ion: 91 Resp: 3928
Ion Ratio Lower Upper
91 100
106 25.0 20.7 38.5

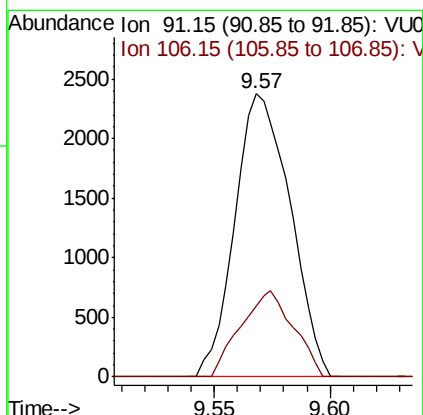



#53

m,p-Xylene

Concen: 0.218 ug/L

RT: 9.69 min Scan# 2598

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampled :


BG3S5DL

Tot Ion:106 Resp: 3966

Ion Ratio Lower Upper




106 100

91 198.2 148.5 275.7

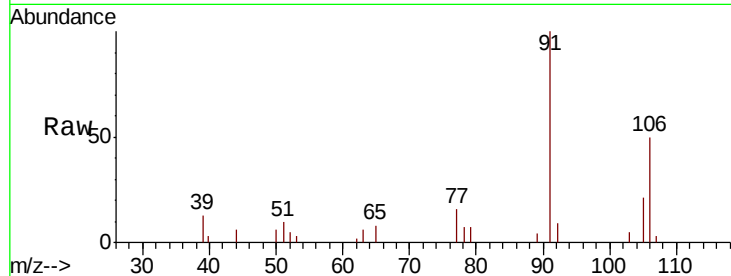

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VU0

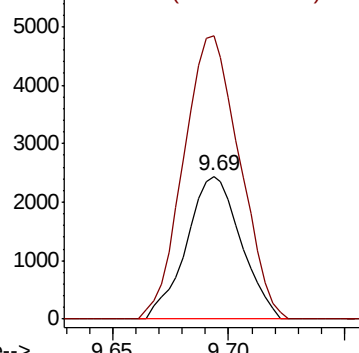

#56

Isopropylbenzene

Concen: 0.180 ug/L

RT: 10.48 min Scan# 2843

Delta R.T. -0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10


Tgt Ion:105 Resp: 8460

Ion Ratio Lower Upper

105 100

120 25.8 20.6 30.8



77 19.3 13.8 20.6




Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VU0




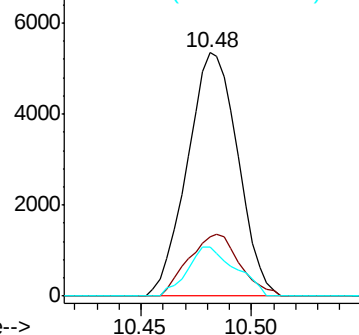




#59
 1,2,3-Trichloropropane
 Concen: 0.077 ug/L
 RT: 10.91 min Scan# 2976
 Delta R.T. 0.09 min
 Lab File: VU040566.D
 Acq: 08 Oct 2020 17:10




Instrument :
 MSVOA_U
 ClientSampleId :
 BG3S5DL


Tot Ion: 75 Resp: 710
 Ion Ratio Lower Upper
 75 100
 77 532.4 26.4 39.6#

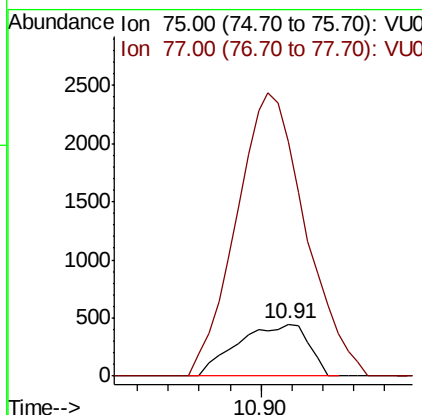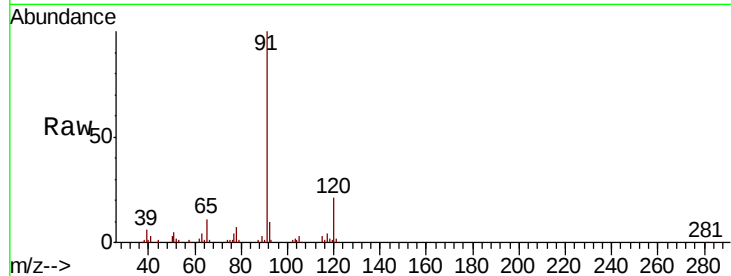

#63
 1,4-Dichlorobenzene
 Concen: 0.075 ug/L
 RT: 11.83 min Scan# 3262
 Delta R.T. -0.00 min
 Lab File: VU040566.D
 Acq: 08 Oct 2020 17:10

Tgt Ion: 146 Resp: 1843
 Ion Ratio Lower Upper
 146 100
 111 50.7 28.4 52.8
 148 62.4 44.0 81.6

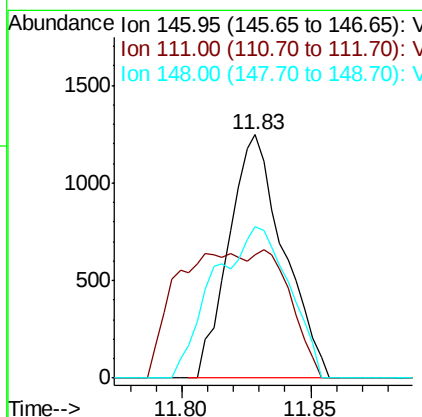


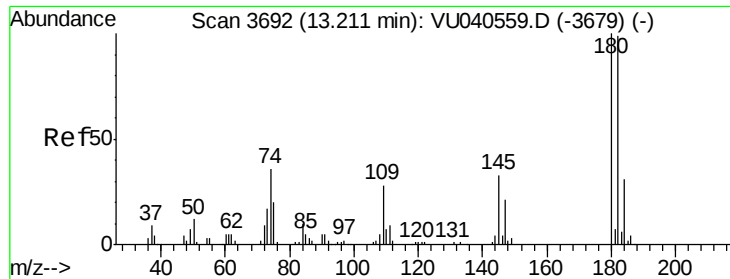




#67
1,3,5-Trichlorobenzene
Concen: 1.465 ug/L
RT: 13.83 min Scan# 3885
Delta R.T. 0.62 min
Lab File: VU040566.D
Acq: 08 Oct 2020 17:10

Instrument :
MSVOA_U
ClientSampleId :
BG3S5DL

Tot Ion:180 Resp: 24628
Ion Ratio Lower Upper
180 100
182 95.2 77.0 115.4
184 28.8 24.5 36.7
145 33.6 25.9 38.9

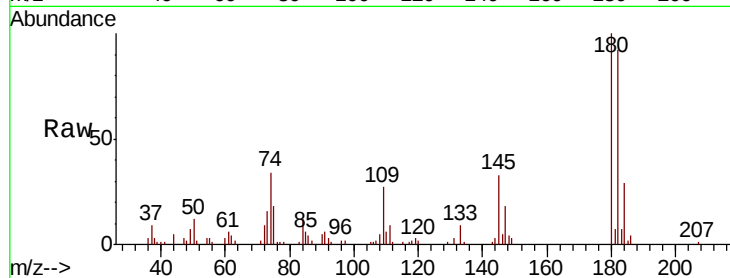


Abundance Ion 180.00 (179.70 to 180.70): V
Ion 182.00 (181.70 to 182.70): V
Ion 184.00 (183.70 to 184.70): V
Ion 145.00 (144.70 to 145.70): V

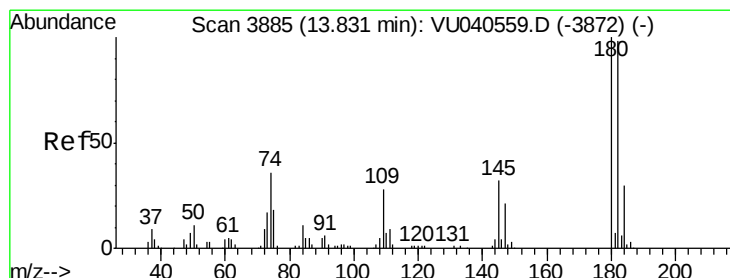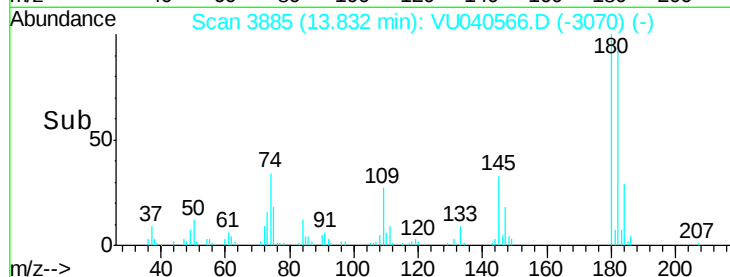
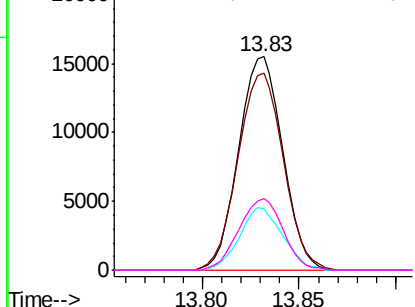



#68
1,2,4-trichlorobenzene
Concen: 1.896 ug/L
RT: 13.83 min Scan# 3885
Delta R.T. 0.00 min
Lab File: VU040566.D
Acq: 08 Oct 2020 17:10

Tgt Ion:180 Resp: 24628
Ion Ratio Lower Upper
180 100
182 95.2 78.8 118.2
145 33.6 26.1 39.1

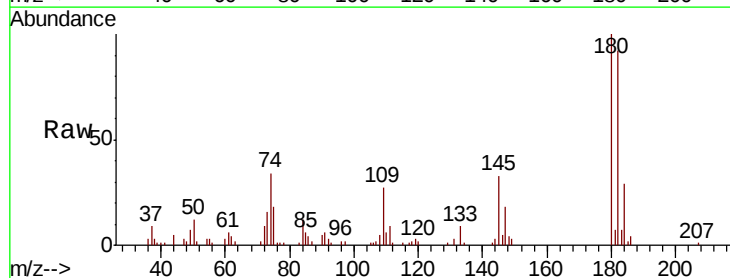

Abundance Ion 179.90 (179.60 to 180.60): V
Ion 182.00 (181.70 to 182.70): V
Ion 144.95 (144.65 to 145.65): V

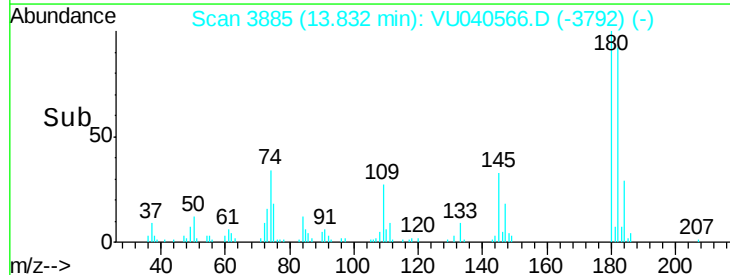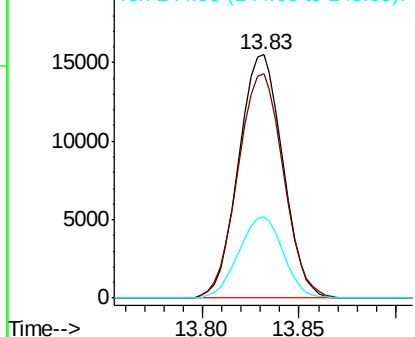



#69

Naphthalene

Concen: 0.127 ug/L

RT: 14.08 min Scan# 3961

Delta R.T. 0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10

Instrument :

MSVOA_U

ClientSampleId :

BG3S5DL


Tot Ion:128 Resp: 2688

Ion Ratio Lower Upper

128 100

129 8.3 9.0 13.4#




127 11.7 10.2 15.4



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 127.00 (126.70 to 127.70): V

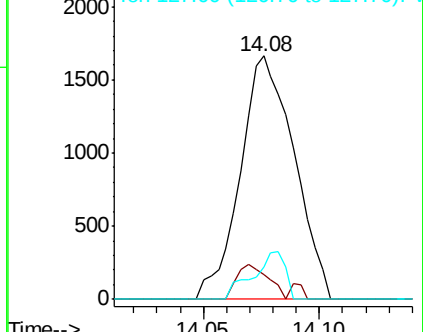

#70

1,2,3-Trichlorobenzene

Concen: 0.438 ug/L

RT: 14.32 min Scan# 4036

Delta R.T. -0.00 min

Lab File: VU040566.D

Acq: 08 Oct 2020 17:10


Tgt Ion:180 Resp: 5282

Ion Ratio Lower Upper

180 100

182 97.2 75.8 113.8

145 30.9 27.4 41.2



Abundance Ion 179.90 (179.60 to 180.60): V

Ion 181.90 (181.60 to 182.60): V

Ion 144.95 (144.65 to 145.65): V

