

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
 Data File : VU045240.D
 Acq On : 08 Oct 2021 10:43
 Operator : SY/MD
 Sample : VU1008WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M

Title : VOC Analysis

Signal : TIC: VU045240.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	34	41	53	rBV	16343	30076	2.21%	0.298%
2	1.600	74	81	94	rVB	216813	232465	17.11%	2.304%
3	1.899	165	174	195	rVB	149441	205469	15.12%	2.037%
4	2.565	368	381	401	rBV	288717	483547	35.59%	4.793%
5	2.735	432	434	438	rBV	216	158	0.01%	0.002%
6	2.755	438	440	444	rBV2	283	193	0.01%	0.002%
7	2.787	444	450	451	rBV	664	530	0.04%	0.005%
8	2.838	462	466	469	rBV2	177	194	0.01%	0.002%
9	2.951	497	501	503	rBV2	481	439	0.03%	0.004%
10	3.054	524	533	539	rBV3	1426	2355	0.17%	0.023%
11	3.186	567	574	575	rBV	678	721	0.05%	0.007%
12	3.272	598	601	607	rVB2	237	253	0.02%	0.003%
13	3.301	607	610	614	rVB2	197	185	0.01%	0.002%
14	3.359	623	628	631	rBV	183	169	0.01%	0.002%
15	3.507	671	674	678	rVB2	225	172	0.01%	0.002%
16	3.607	701	705	709	rBV2	225	212	0.02%	0.002%
17	3.874	784	788	791	rBV2	200	237	0.02%	0.002%
18	4.005	820	829	834	rVB2	253	553	0.04%	0.005%
19	4.034	834	838	842	rBV2	219	232	0.02%	0.002%
20	4.057	842	845	849	rVB	223	193	0.01%	0.002%
21	4.115	859	863	865	rBV2	203	181	0.01%	0.002%
22	4.346	932	935	943	rVB2	230	337	0.02%	0.003%
23	4.520	986	989	996	rBV2	161	255	0.02%	0.003%
24	4.626	1007	1022	1057	rBV	148744	351645	25.88%	3.485%
25	4.919	1109	1113	1118	rVV2	207	204	0.02%	0.002%
26	4.944	1119	1121	1129	rVB2	218	208	0.02%	0.002%
27	5.067	1141	1159	1192	rBV	235765	518826	38.19%	5.142%
28	5.218	1202	1206	1211	rVB2	485	407	0.03%	0.004%
29	5.253	1211	1217	1221	rBV2	223	301	0.02%	0.003%
30	5.288	1221	1228	1230	rBV3	626	717	0.05%	0.007%
31	5.356	1244	1249	1253	rVB2	138	149	0.01%	0.001%
32	5.462	1278	1282	1289	rBV2	203	324	0.02%	0.003%
33	5.729	1343	1365	1383	rBV2	513675	1358586	100.00%	13.466%
34	6.050	1458	1465	1471	rBV3	442	663	0.05%	0.007%
35	6.118	1481	1486	1487	rBV	324	264	0.02%	0.003%
36	6.253	1513	1528	1547	rBV	364209	683117	50.28%	6.771%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
 Data File : VU045240.D
 Acq On : 08 Oct 2021 10:43
 Operator : SY/MD
 Sample : VU1008WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

37	6.427	1579	1582	1584	rBV2	189	159	0.01%	0.002%
38	6.533	1605	1615	1625	rBV4	4146	7748	0.57%	0.077%
39	6.697	1651	1666	1687	rBV	319637	615703	45.32%	6.103%
40	6.796	1695	1697	1698	rBV	441	196	0.01%	0.002%
41	6.893	1724	1727	1731	rVB2	205	177	0.01%	0.002%
42	7.005	1759	1762	1766	rBV2	201	199	0.01%	0.002%
43	7.047	1766	1775	1783	rVV4	662	1137	0.08%	0.011%
44	7.153	1804	1808	1811	rBV2	299	299	0.02%	0.003%
45	7.173	1811	1814	1816	rBV3	627	433	0.03%	0.004%
46	7.333	1861	1864	1867	rBV	190	157	0.01%	0.002%
47	7.488	1902	1912	1917	rBV2	319	634	0.05%	0.006%
48	7.568	1924	1937	1958	rBV	176180	305968	22.52%	3.033%
49	7.693	1969	1976	1986	rVB5	490	871	0.06%	0.009%
50	7.796	2002	2008	2018	rVB2	781	1086	0.08%	0.011%
51	7.902	2027	2041	2055	rBV	624904	1055845	77.72%	10.465%
52	7.973	2057	2063	2075	rVB2	9412	15247	1.12%	0.151%
53	8.124	2104	2110	2111	rBV2	196	189	0.01%	0.002%
54	8.182	2116	2128	2144	rVV	123849	203981	15.01%	2.022%
55	8.282	2156	2159	2161	rBV2	284	206	0.02%	0.002%
56	8.478	2217	2220	2223	rBV	203	198	0.01%	0.002%
57	8.558	2241	2245	2248	rBV2	321	247	0.02%	0.002%
58	8.636	2257	2269	2304	rBV	425843	756530	55.69%	7.498%
59	9.105	2412	2415	2420	rBV2	142	173	0.01%	0.002%
60	9.176	2432	2437	2443	rBV2	241	303	0.02%	0.003%
61	9.208	2443	2447	2453	rBV2	185	198	0.01%	0.002%
62	9.420	2499	2513	2542	rBV	529255	859497	63.26%	8.519%
63	9.574	2553	2561	2574	rVB	936	1499	0.11%	0.015%
64	9.697	2591	2599	2607	rBV2	3324	4530	0.33%	0.045%
65	9.873	2651	2654	2660	rBV2	149	158	0.01%	0.002%
66	10.098	2719	2724	2725	rBV2	757	534	0.04%	0.005%
67	10.195	2752	2754	2757	rVB	240	154	0.01%	0.002%
68	10.234	2762	2766	2768	rBV2	274	173	0.01%	0.002%
69	10.349	2798	2802	2806	rBV	201	236	0.02%	0.002%
70	10.475	2835	2841	2842	rBV	263	267	0.02%	0.003%
71	10.488	2842	2845	2849	rVV2	285	309	0.02%	0.003%
72	10.674	2894	2903	2915	rVB3	3856	6245	0.46%	0.062%
73	10.761	2915	2930	2948	rBV	429227	700685	51.57%	6.945%
74	10.870	2958	2964	2966	rBV4	533	540	0.04%	0.005%
75	11.063	3020	3024	3027	rBV2	144	175	0.01%	0.002%
76	11.089	3029	3032	3035	rBV2	434	341	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
 Data File : VU045240.D
 Acq On : 08 Oct 2021 10:43
 Operator : SY/MD
 Sample : VU1008WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK024

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
 Title : VOC Analysis

77	11.115	3037	3040	3041	rBV2	281	185	0.01%	0.002%
78	11.205	3065	3068	3073	rVB2	246	248	0.02%	0.002%
79	11.272	3085	3089	3093	rBV2	138	193	0.01%	0.002%
80	11.459	3138	3147	3162	rVB5	2489	4445	0.33%	0.044%
81	11.587	3182	3187	3192	rVB4	558	617	0.05%	0.006%
82	11.635	3198	3202	3204	rBV2	196	171	0.01%	0.002%
83	11.696	3214	3221	3229	rBV3	1308	1754	0.13%	0.017%
84	11.815	3246	3258	3275	rBV	477643	757485	55.76%	7.508%
85	11.947	3293	3299	3302	rBV3	1242	1463	0.11%	0.015%
86	11.976	3304	3308	3321	rVB2	2411	3278	0.24%	0.032%
87	12.195	3362	3376	3394	rBV	547221	880295	64.79%	8.725%
88	12.330	3415	3418	3420	rBV2	645	495	0.04%	0.005%
89	12.565	3483	3491	3495	rBV2	281	401	0.03%	0.004%
90	12.751	3544	3549	3552	rBV2	221	219	0.02%	0.002%
91	13.156	3670	3675	3681	rVB3	418	502	0.04%	0.005%
92	13.227	3690	3697	3702	rBV6	1076	1555	0.11%	0.015%
93	13.777	3863	3868	3870	rBV	212	219	0.02%	0.002%
94	13.848	3883	3890	3897	rBV3	1826	2468	0.18%	0.024%
95	14.005	3935	3939	3946	rBV	238	388	0.03%	0.004%
96	14.092	3958	3966	3977	rBV	6173	9679	0.71%	0.096%
97	14.294	4024	4029	4033	rBV2	340	385	0.03%	0.004%
98	14.333	4034	4041	4052	rVV4	2827	4138	0.30%	0.041%
99	14.597	4114	4123	4126	rBV2	392	506	0.04%	0.005%
100	14.915	4217	4222	4226	rBV3	317	347	0.03%	0.003%


Sum of corrected areas: 10089200

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
Data File : VU045240.D
Acq On : 08 Oct 2021 10:43
Operator : SY/MD
Sample : VU1008WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

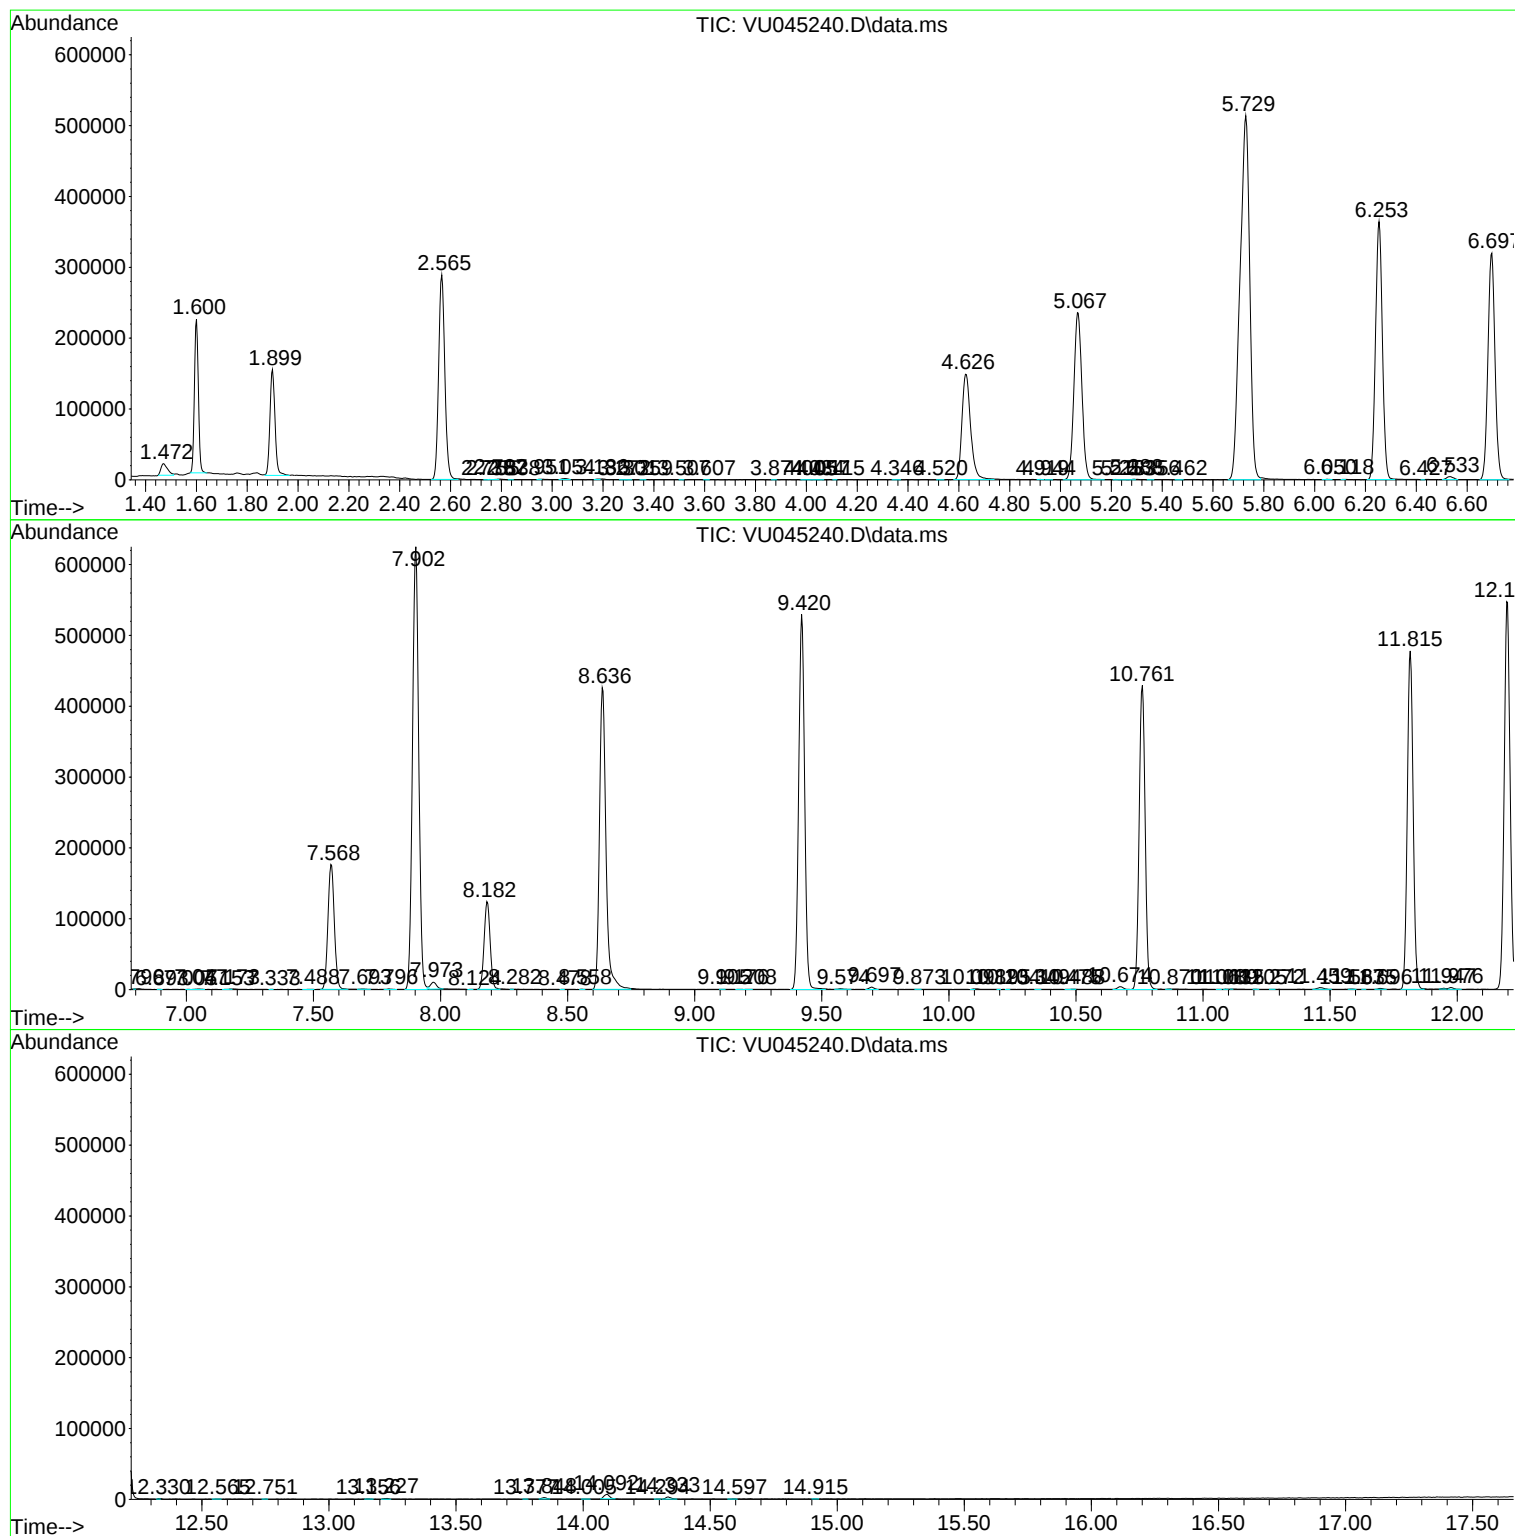

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
Data File : VU045240.D
Acq On : 08 Oct 2021 10:43
Operator : SY/MD
Sample : VU1008WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
Data File : VU045240.D
Acq On : 08 Oct 2021 10:43
Operator : SY/MD
Sample : VU1008WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK024

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
