


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100821\
Data File : VU045237.D
Acq On : 08 Oct 2021 09:11
Operator : SY/MD
Sample : BFB009
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB009

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092321WMA.M
Title : VOC Analysis
Last Update : Wed Oct 13 02:48:52 2021

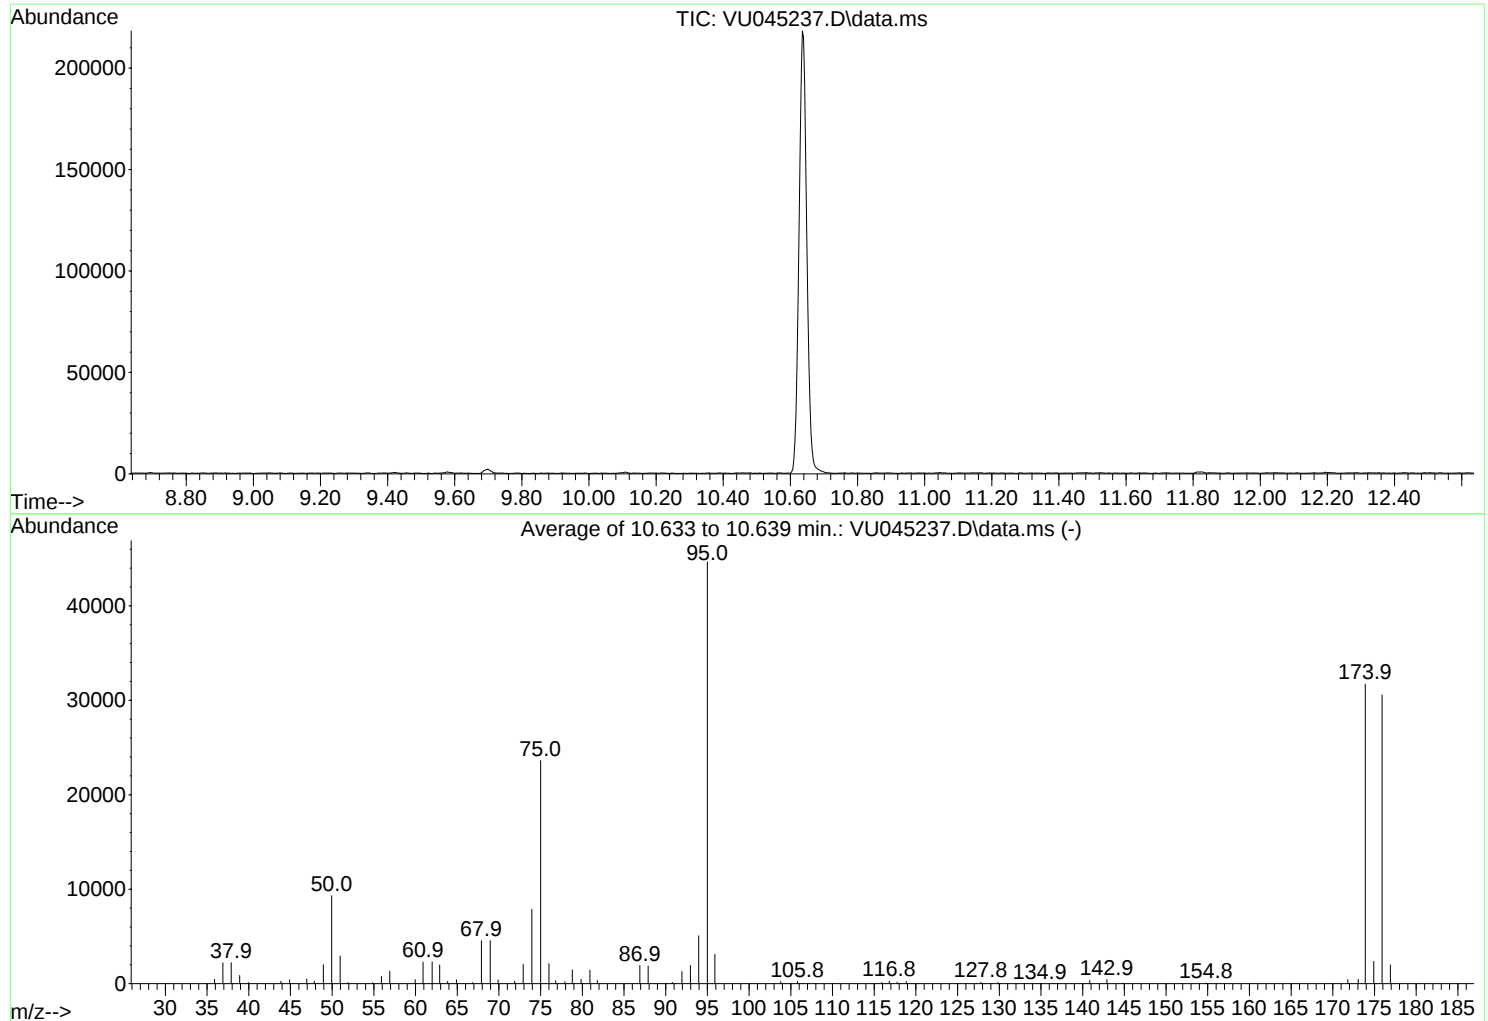

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	9307	PASS
75	95	30	80	52.9	23616	PASS
95	95	100	100	100.0	44664	PASS
96	95	5	9	6.9	3099	PASS
173	174	0.00	2	1.5	463	PASS
174	95	50	120	71.0	31715	PASS
175	174	5	9	7.4	2353	PASS
176	174	95	101	96.4	30579	PASS
177	176	5	9	6.5	1979	PASS

m/z	Abundance
43.80	314.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	440.0
36.90	2244.0
37.90	2267.0
38.90	847.0
40.00	125.0
43.90	539.0
44.90	397.0
47.00	482.0
47.90	255.0
48.90	1857.0
49.90	8789.0
50.90	2914.0
51.90	118.0
54.80	122.0
55.90	780.0
56.90	1245.0
59.90	414.0
60.90	2309.0
62.00	2207.0
62.90	1851.0
63.90	215.0
64.90	374.0
66.80	142.0
67.90	4232.0
68.90	4497.0
69.90	343.0
71.90	258.0
72.90	1996.0
74.00	7708.0
75.00	22256.0
76.00	1961.0
76.80	286.0
77.80	197.0
78.80	1409.0
79.80	409.0
80.90	1349.0
81.80	358.0
86.90	1834.0
87.90	1807.0
90.80	125.0
92.00	1200.0
93.00	1768.0
93.90	4805.0
95.00	42776.0
95.90	3000.0
103.80	211.0
105.80	210.0
115.90	107.0
116.80	282.0
117.70	144.0
118.80	200.0
127.80	139.0
129.90	117.0
140.80	304.0
142.90	398.0
144.80	100.0
154.80	101.0
171.80	398.0
173.00	430.0
173.90	29664.0
174.90	2225.0
175.90	28320.0
176.90	1898.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	468.0
36.90	2274.0
37.90	2319.0
38.90	882.0
40.00	130.0
43.90	591.0
44.90	422.0
47.00	489.0
47.80	289.0
48.90	2059.0
50.00	9559.0
50.90	3021.0
51.90	131.0
54.90	101.0
55.90	809.0
56.90	1372.0
60.00	414.0
60.90	2354.0
62.00	2404.0
62.90	2040.0
63.80	251.0
64.90	431.0
66.80	129.0
67.90	4642.0
68.90	4664.0
69.90	406.0
71.90	258.0
72.90	2061.0
73.90	8127.0
75.00	24392.0
76.00	2186.0
76.80	331.0
77.90	214.0
78.80	1519.0
79.90	475.0
80.90	1487.0
81.80	353.0
86.90	1980.0
87.90	1951.0
90.80	142.0
91.90	1313.0
93.00	1976.0
93.90	5183.0
95.00	46160.0
95.90	3204.0
103.80	224.0
105.80	236.0
115.90	128.0
116.80	292.0
117.80	155.0
118.80	233.0
127.80	149.0
129.90	136.0
140.90	361.0
142.90	436.0
144.80	105.0
154.80	109.0
171.80	422.0
173.00	494.0
173.90	32800.0
174.90	2416.0
175.90	31552.0
176.90	2044.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
35.90	471.0
36.90	2105.0
37.90	2091.0
38.90	865.0
39.90	136.0
43.90	582.0
44.90	380.0
46.90	512.0
47.80	299.0
49.00	2104.0
50.00	9574.0
51.00	2859.0
51.90	120.0
54.90	102.0
55.90	693.0
56.90	1340.0
60.00	419.0
60.90	2201.0
62.00	2321.0
62.90	2055.0
63.90	248.0
64.90	399.0
66.90	106.0
67.90	4735.0
69.00	4504.0
69.90	422.0
71.90	238.0
72.90	2042.0
73.90	7762.0
75.00	24200.0
76.00	2188.0
76.80	316.0
78.00	224.0
78.80	1456.0
79.90	480.0
80.90	1423.0
81.80	309.0
86.90	1934.0
87.90	1805.0
90.80	157.0
91.90	1316.0
92.90	1998.0
94.00	5238.0
95.00	45056.0
95.90	3094.0
103.80	208.0
105.80	221.0
115.90	134.0
116.80	251.0
117.80	149.0
118.90	222.0
127.80	138.0
129.80	135.0
134.90	100.0
140.90	369.0
142.90	422.0
171.80	470.0
173.10	466.0
173.90	32680.0
174.90	2419.0
175.90	31864.0
176.90	1996.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009