


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100918\
 Data File : VU027520.D
 Acq On : 09 Oct 2018 08:22
 Operator : MD/SY
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM100518WMA.M
 Title : VOC Analysis
 Last Update : Wed Oct 10 08:24:11 2018

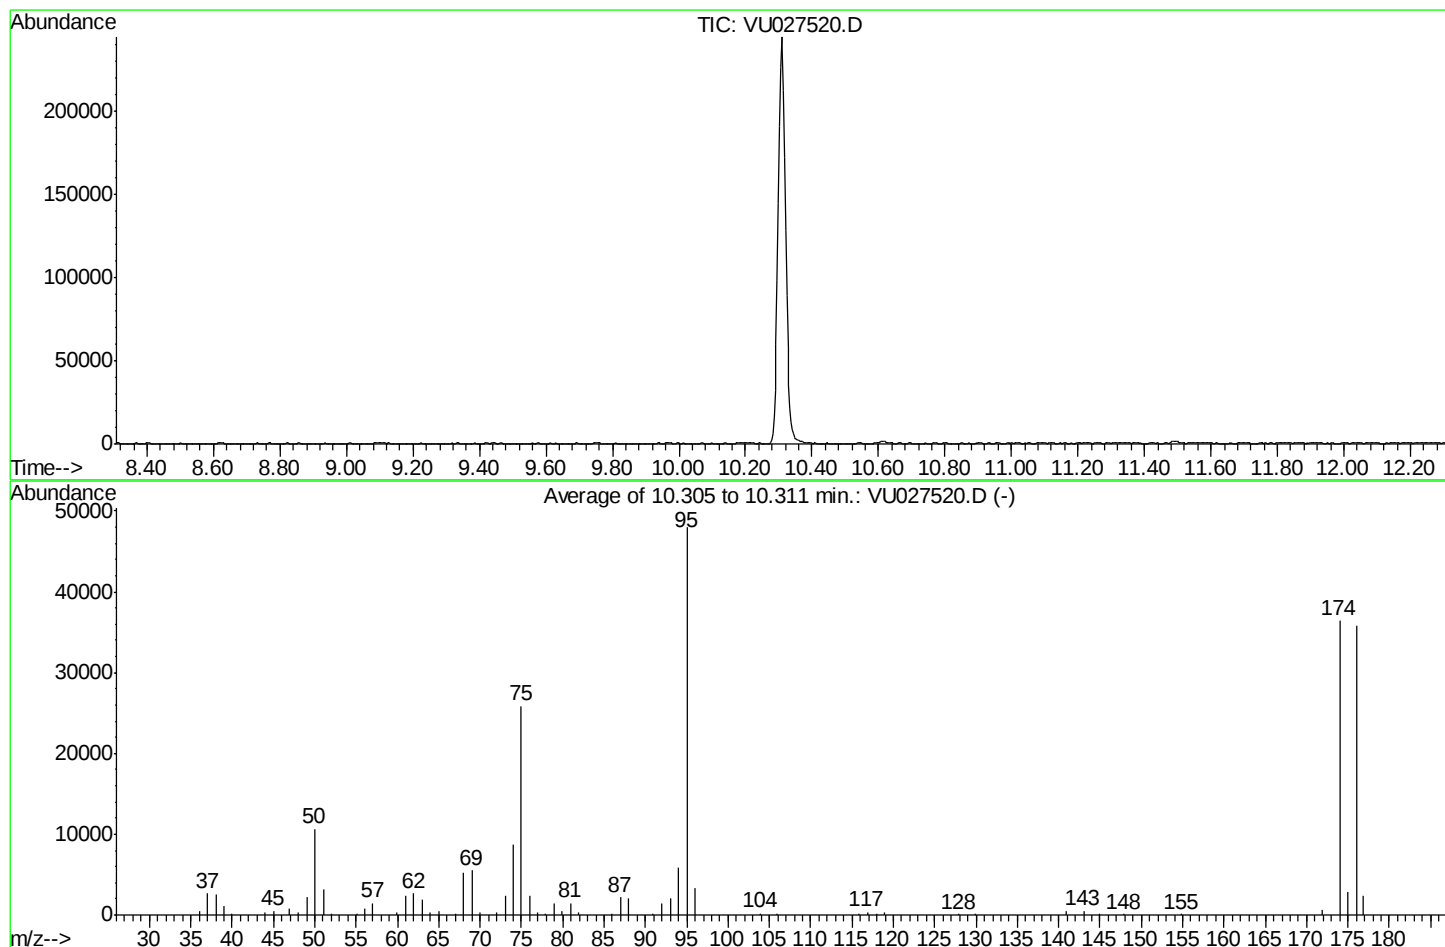

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	10640	PASS
75	95	30	80	53.9	25869	PASS
95	95	100	100	100.0	47989	PASS
96	95	5	9	7.0	3338	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.9	36440	PASS
175	174	5	9	7.7	2815	PASS
176	174	95	101	98.5	35880	PASS
177	176	5	9	6.6	2386	PASS

m/z	Abundance
43.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	437.0
37.00	2584.0
38.00	2524.0
39.00	1113.0
39.90	141.0
44.00	545.0
45.00	469.0
47.00	764.0
48.10	262.0
49.00	2156.0
50.00	10588.0
51.00	3198.0
52.00	103.0
55.10	137.0
56.00	741.0
57.00	1411.0
59.90	385.0
61.00	2361.0
62.00	2707.0
63.00	1872.0
64.00	312.0
65.00	472.0
67.00	148.0
68.00	5104.0
69.00	5332.0
70.00	360.0
71.90	284.0
73.00	2165.0
74.00	8520.0
75.00	24840.0
76.00	2236.0
77.00	314.0
77.90	209.0
78.90	1434.0
79.90	378.0
80.90	1346.0
81.90	248.0
85.90	127.0
87.00	2078.0
88.00	2045.0
90.90	136.0
92.00	1432.0
93.00	1950.0
94.10	5657.0
95.00	45576.0
96.00	3254.0
104.00	206.0
105.90	224.0
115.80	165.0
116.90	283.0
118.00	191.0
118.90	267.0
127.90	129.0
140.90	492.0
143.00	484.0
144.90	128.0
154.90	111.0
171.90	632.0
174.00	34168.0
175.00	2717.0
176.00	33448.0
176.90	2258.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	497.0
37.00	2712.0
38.00	2625.0
39.00	1174.0
39.90	142.0
44.00	576.0
45.00	522.0
46.90	788.0
48.10	296.0
49.00	2349.0
50.00	10935.0
51.10	3206.0
52.00	128.0
55.10	149.0
56.00	883.0
57.00	1490.0
60.00	407.0
61.00	2403.0
62.00	2790.0
63.00	2030.0
64.00	275.0
65.00	494.0
67.00	154.0
68.00	5395.0
69.00	5674.0
70.00	387.0
72.00	314.0
73.00	2420.0
74.00	9037.0
75.00	26776.0
76.00	2400.0
77.00	315.0
77.90	200.0
79.00	1435.0
80.00	436.0
80.90	1478.0
81.90	240.0
85.90	120.0
87.00	2254.0
88.00	2178.0
90.90	133.0
92.00	1448.0
93.00	2082.0
94.10	6130.0
95.00	49384.0
96.00	3463.0
104.00	245.0
105.90	206.0
115.80	171.0
116.90	359.0
117.90	239.0
118.90	252.0
127.90	128.0
129.90	130.0
140.90	517.0
143.00	526.0
145.00	123.0
147.90	122.0
154.90	133.0
171.90	584.0
174.00	37688.0
175.00	2919.0
176.00	37144.0
176.90	2482.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	486.0
37.00	2651.0
38.00	2468.0
39.00	1109.0
39.90	130.0
44.00	593.0
45.00	531.0
46.90	750.0
47.90	299.0
49.00	2349.0
50.00	10398.0
51.10	3070.0
52.00	152.0
55.10	138.0
56.00	921.0
57.00	1425.0
60.00	411.0
61.00	2186.0
62.00	2524.0
63.00	1990.0
64.00	247.0
65.00	434.0
67.00	160.0
68.00	5214.0
69.00	5496.0
70.00	378.0
72.00	316.0
73.00	2413.0
74.00	8551.0
75.00	25992.0
76.00	2299.0
76.90	289.0
78.00	178.0
79.00	1368.0
80.00	427.0
80.90	1532.0
82.00	249.0
85.90	109.0
87.00	2163.0
88.00	2046.0
90.80	131.0
92.00	1331.0
93.00	2032.0
94.00	5929.0
95.00	49008.0
96.00	3298.0
103.90	268.0
106.00	172.0
115.80	168.0
116.90	392.0
117.90	210.0
119.00	223.0
127.90	147.0
129.90	145.0
140.90	447.0
143.00	486.0
145.00	116.0
147.90	136.0
154.90	142.0
171.90	514.0
174.00	37464.0
175.00	2809.0
176.00	37048.0
176.90	2420.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41