


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU100919\
Data File : VU035000.D
Acq On : 09 Oct 2019 09:25
Operator : JC/SP
Sample : BFB16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Oct 10 03:36:45 2019

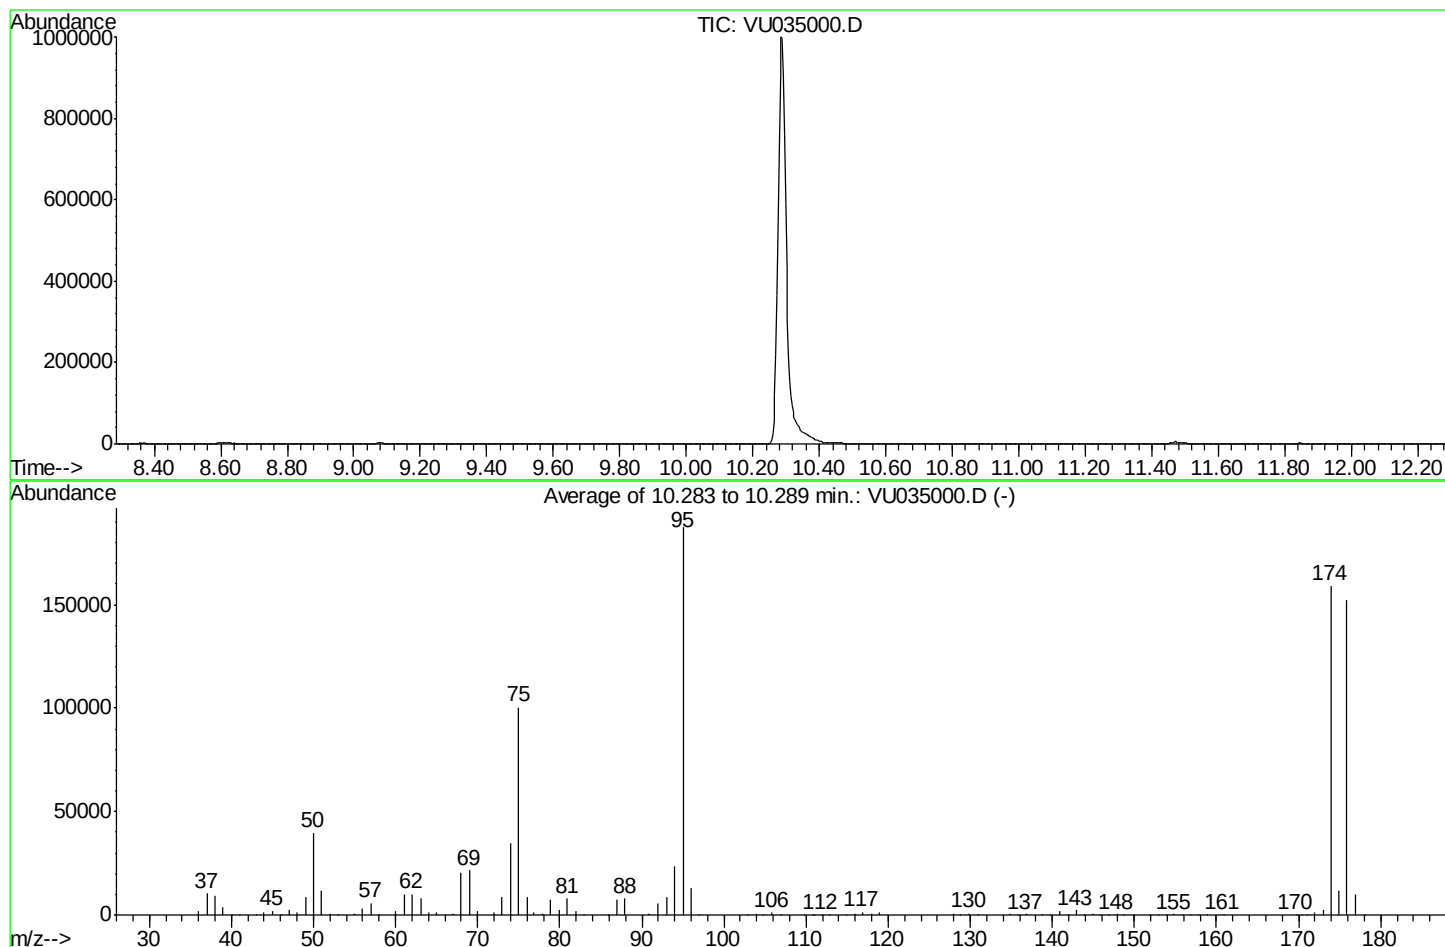

AutoFind: Scans 2859, 2860, 2861; Background Corrected with Scan 2846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	39808	PASS
75	95	30	80	53.6	100528	PASS
95	95	100	100	100.0	187392	PASS
96	95	5	9	6.9	12972	PASS
173	174	0.00	2	1.4	2211	PASS
174	95	50	120	85.0	159210	PASS
175	174	5	9	7.5	11981	PASS
176	174	95	101	95.7	152405	PASS
177	176	5	9	6.5	9935	PASS

m/z	Abundance
36.00	1732.0
37.00	9995.0
38.00	8923.0
39.00	3628.0
40.00	281.0
44.00	1509.0
45.00	1956.0
45.90	122.0
46.20	118.0
47.00	2383.0
48.00	1321.0
49.00	8640.0
50.00	37432.0
51.00	11294.0
52.00	539.0
52.90	194.0
55.00	562.0
56.00	3000.0
57.00	5315.0
58.00	246.0
60.00	1759.0
61.00	9359.0
62.00	9973.0
63.10	7652.0
64.00	1073.0
65.00	1123.0
66.00	106.0
67.00	564.0
68.00	19448.0
69.00	20832.0
70.00	1626.0
72.00	1307.0
73.00	8402.0
74.00	32464.0
75.00	96336.0
76.00	8635.0
76.90	1006.0
77.90	877.0
78.90	7084.0
79.90	2282.0
80.90	7432.0
81.90	1689.0
82.90	205.0
85.90	297.0
87.00	7156.0
88.00	7319.0
90.90	726.0
92.00	5440.0
93.00	7950.0
94.00	22272.0
95.00	176704.0
96.00	12594.0
97.00	292.0
102.80	102.0
103.90	810.0
104.80	262.0
105.90	1003.0
106.80	149.0
109.80	128.0
110.80	191.0
111.90	212.0
112.80	240.0
114.90	205.0
115.90	771.0
116.90	1378.0
118.00	727.0
118.90	1065.0
127.90	654.0
128.80	240.0
129.90	748.0
130.90	311.0
134.90	335.0
135.80	140.0
136.80	322.0
138.80	104.0
140.90	1963.0
141.90	290.0
142.90	2164.0
143.80	114.0
144.90	324.0
145.70	241.0
146.90	135.0
147.80	416.0
149.90	230.0
152.90	222.0
154.80	432.0
156.80	223.0
157.80	118.0
158.80	153.0
160.80	253.0
169.60	142.0
171.90	1460.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

173.00	2030.0
173.90	146688.0
174.90	10926.0
175.90	139072.0
176.90	9238.0
178.00	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	2010.0
37.00	10561.0
38.00	9651.0
39.00	3780.0
40.00	324.0
41.00	107.0
43.00	128.0
44.00	1798.0
45.00	2043.0
45.90	141.0
46.20	157.0
47.00	2675.0
47.90	1497.0
49.00	9297.0
50.00	41120.0
51.00	12290.0
52.00	512.0
53.00	265.0
54.90	555.0
56.00	3210.0
57.00	6046.0
58.00	237.0
60.00	1934.0
61.00	10210.0
62.00	10453.0
63.10	8494.0
64.00	1045.0
65.00	1102.0
66.00	118.0
67.00	679.0
68.00	21384.0
69.00	22104.0
70.00	1679.0
72.10	1281.0
73.00	9217.0
74.00	35496.0
75.00	103824.0
76.00	9134.0
76.90	1151.0
77.90	905.0
78.90	7606.0
79.90	2499.0
80.90	8115.0
81.90	1803.0
82.80	257.0
85.90	269.0
87.00	7834.0
88.00	8178.0
90.90	813.0
92.00	6043.0
93.00	8916.0
94.00	24264.0
95.00	193536.0
96.00	13336.0
97.00	324.0
103.90	894.0
104.80	319.0
105.90	1095.0
106.90	211.0
109.80	116.0
111.00	223.0
111.90	179.0
112.80	277.0
114.80	246.0
115.90	840.0
116.90	1559.0
117.90	760.0
119.00	1195.0
127.90	715.0
128.80	272.0
129.90	816.0
130.90	337.0
134.80	364.0
135.80	114.0
136.80	383.0
138.80	131.0
140.90	2071.0
141.90	339.0
142.90	2511.0
143.80	104.0
144.90	367.0
145.70	229.0
146.90	141.0
147.90	469.0
148.70	104.0
149.90	262.0
152.90	222.0
153.80	117.0
154.80	442.0
155.90	119.0
156.80	257.0
157.80	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

158.80	183.0
160.80	311.0
169.70	128.0
171.90	1584.0
173.00	2271.0
173.90	164480.0
174.90	12345.0
175.90	157120.0
176.90	10279.0
178.00	269.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
36.00	2063.0
37.00	10228.0
38.00	9502.0
39.00	3680.0
40.00	327.0
43.00	171.0
44.00	1940.0
45.00	1894.0
45.90	161.0
46.10	161.0
47.00	2532.0
47.90	1473.0
49.00	8936.0
50.00	40872.0
51.00	12061.0
52.00	428.0
53.00	274.0
54.90	542.0
56.00	3179.0
57.00	6246.0
58.00	210.0
60.00	1958.0
61.00	10271.0
62.00	10010.0
63.00	8125.0
64.00	933.0
65.00	1042.0
67.00	741.0
68.00	21024.0
69.00	21432.0
70.00	1691.0
72.00	1170.0
73.00	9187.0
74.00	35672.0
75.00	101424.0
76.00	8876.0
76.90	1251.0
78.00	842.0
78.90	7700.0
79.90	2399.0
80.90	7999.0
81.90	1707.0
82.80	234.0
85.90	272.0
87.00	7866.0
87.90	8206.0
90.90	742.0
92.00	6116.0
93.00	9161.0
94.00	23728.0
95.00	191936.0
96.00	12986.0
97.00	343.0
103.90	964.0
104.80	354.0
105.90	1072.0
106.90	217.0
109.80	106.0
111.00	234.0
111.90	161.0
112.80	263.0
114.90	228.0
115.90	751.0
116.90	1576.0
117.90	771.0
119.00	1254.0
127.90	729.0
128.80	281.0
129.90	837.0
130.90	318.0
134.90	381.0
136.80	413.0
138.80	114.0
139.70	112.0
140.90	2035.0
141.90	337.0
142.90	2475.0
144.90	369.0
145.80	231.0
146.80	126.0
147.90	458.0
148.70	110.0
149.90	228.0
151.80	108.0
152.90	173.0
153.80	117.0
154.80	436.0
155.90	160.0
156.80	288.0
157.80	135.0
158.80	218.0
160.80	257.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

169.80	120.0
170.40	122.0
171.00	268.0
171.90	1611.0
173.00	2333.0
173.90	166464.0
174.90	12672.0
175.90	161024.0
176.90	10288.0
178.00	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

Scan 2846 (10.241 min): VU035000.D
BFB16

m/z	Abundance
39.90	183.0
44.00	669.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16