
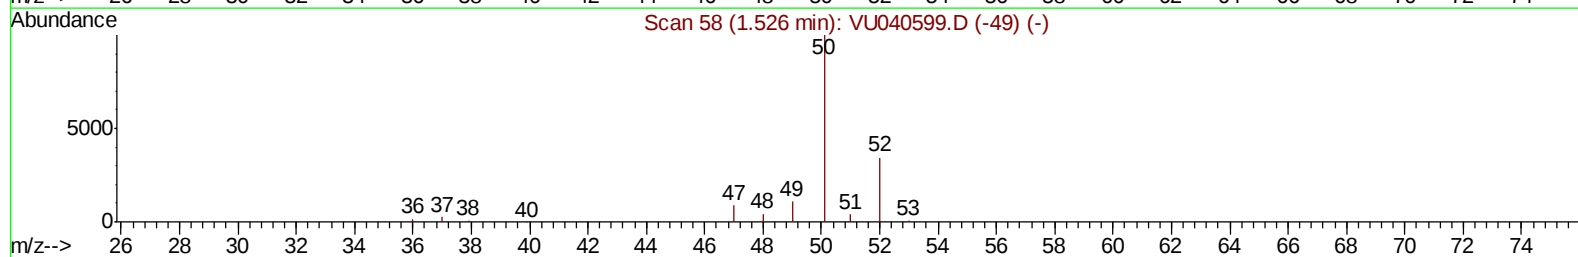
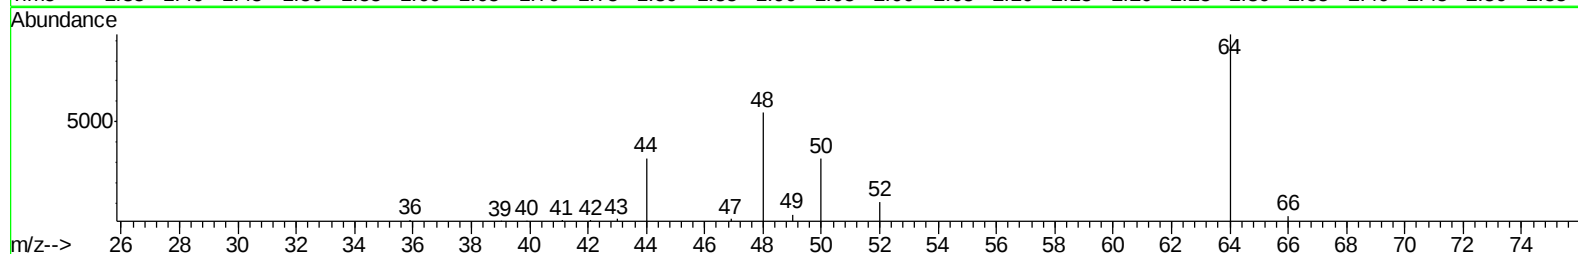


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU100920\
Data File : VU040622.D
Acq On : 10 Oct 2020 06:43
Operator : SY/MD
Sample : L4352-22
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Oct 10 07:41:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR100820WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 10 05:58:50 2020
Response via : Initial Calibration

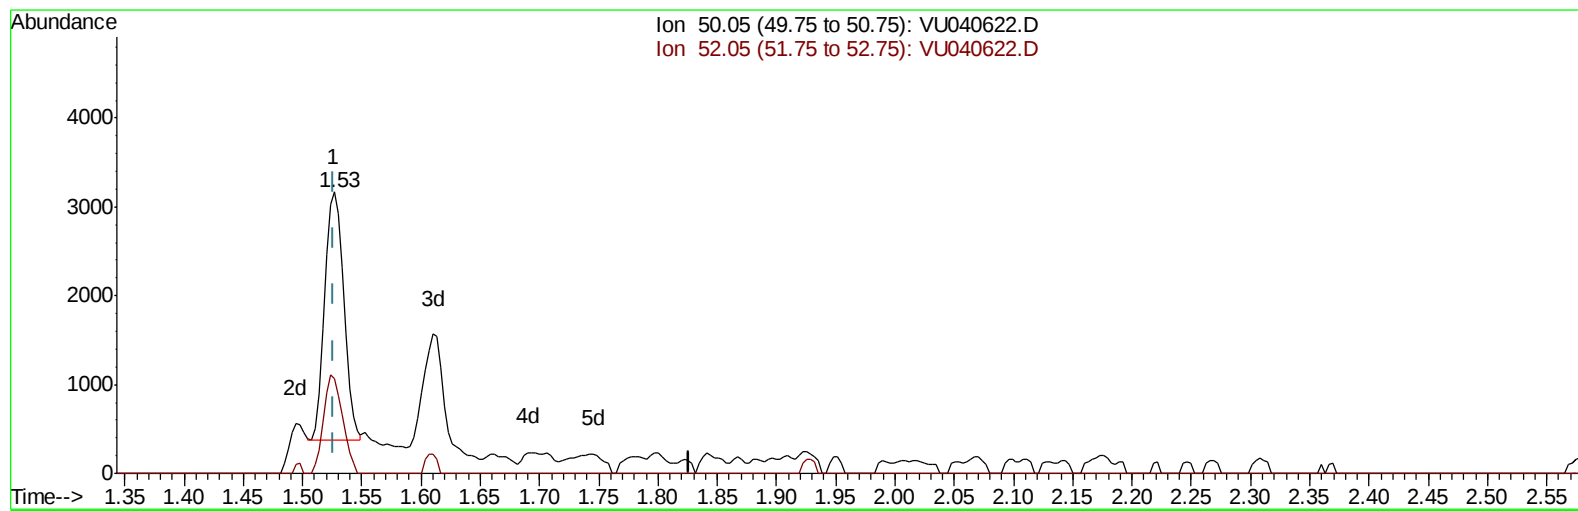

TIC: VU040622.D

(3) Chloromethane (T)

1.527min (+0.000) 0.27ug/L m

response 3129

Ion	Exp%	Act%
50.05	100	100
52.05	31.30	33.69
0.00	0.00	0.00
0.00	0.00	0.00